


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050223\
Data File : VD075953.D
Acq On : 02 May 2023 09:02
Operator : KP/SY
Sample : BFB124
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB124

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Title : SFAM01.0
Last Update : Wed May 03 02:37:35 2023

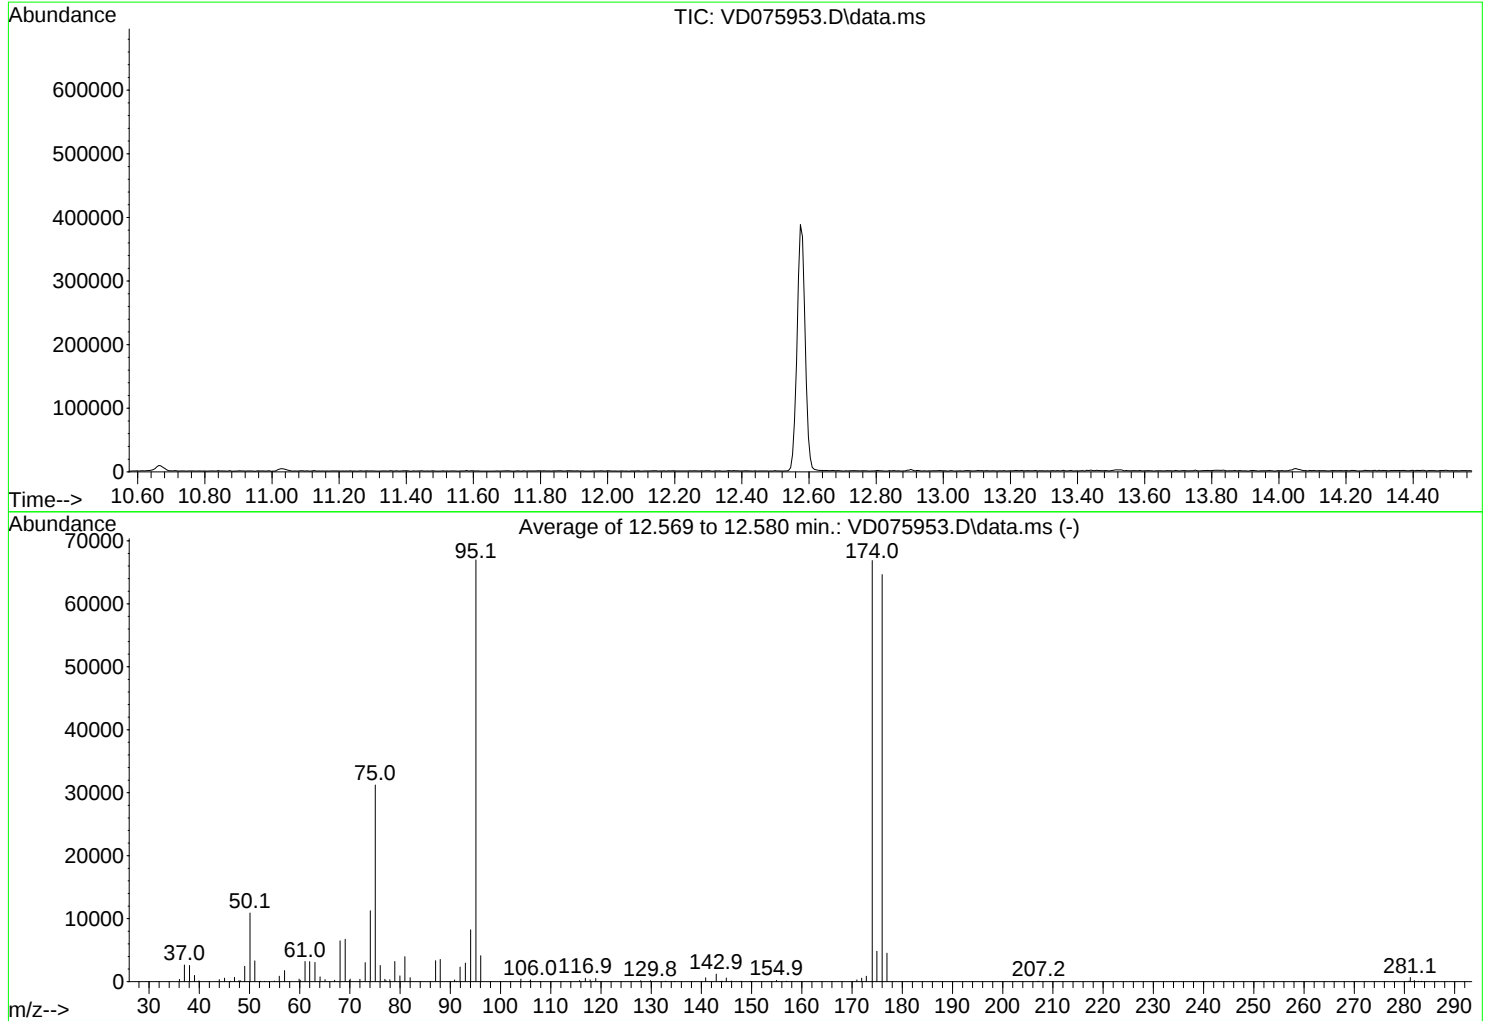

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.3	10903	PASS
75	95	30	80	46.6	31221	PASS
95	95	100	100	100.0	66979	PASS
96	95	5	9	6.2	4124	PASS
173	174	0.00	2	1.3	876	PASS
174	95	50	120	99.9	66883	PASS
175	174	5	9	7.2	4843	PASS
176	174	95	105	96.6	64632	PASS
177	176	5	10	7.0	4533	PASS

Scan 1860 (12.527 min): VD075953.D\data.ms
BFB124

m/z	Abundance
39.90	912.0
44.00	566.0
207.00	166.0

Instrument :
MSVOA_D
ClientSampleId :
BFB124

m/z	Abundance
36.00	523.0
37.00	2301.0
38.00	2288.0
39.10	873.0
40.10	1052.0
44.10	807.0
45.00	623.0
47.00	618.0
48.20	189.0
49.00	2124.0
50.10	9294.0
51.10	3397.0
52.20	182.0
53.00	201.0
56.00	768.0
57.00	1644.0
59.90	657.0
61.10	2547.0
62.00	2932.0
63.10	3230.0
64.10	783.0
65.00	191.0
67.00	189.0
68.10	5592.0
69.10	6084.0
69.90	576.0
71.90	320.0
73.00	2561.0
74.10	10526.0
75.00	26960.0
76.10	2235.0
76.90	493.0
78.10	260.0
78.90	2526.0
80.00	734.0
80.90	3512.0
82.00	641.0
87.00	3020.0
88.00	3032.0
90.90	258.0
91.90	1539.0
93.00	2442.0
94.00	7125.0
95.10	58520.0
96.10	3613.0
104.00	506.0
105.70	268.0
117.00	387.0
117.90	208.0
118.90	489.0
129.90	273.0
141.00	561.0
142.90	880.0
144.90	568.0
146.00	151.0
155.00	256.0
170.90	287.0
171.90	379.0
172.80	390.0
174.00	56768.0
175.00	4017.0
176.00	54176.0
177.00	3959.0
207.00	330.0
280.90	302.0
281.30	251.0
282.80	194.0

Instrument :
MSVOA_D
ClientSampleId :
BFB124

m/z	Abundance
36.10	346.0
37.10	3094.0
38.10	2683.0
39.00	1062.0
40.10	801.0
44.00	1056.0
45.00	575.0
46.20	228.0
47.10	633.0
48.10	281.0
49.10	2635.0
50.10	12442.0
51.00	3364.0
55.00	160.0
56.00	893.0
57.00	2021.0
60.10	661.0
61.00	3239.0
62.00	3478.0
63.00	3069.0
64.00	720.0
65.00	515.0
66.90	250.0
68.00	7445.0
69.10	8144.0
70.10	684.0
72.00	403.0
73.00	3256.0
74.00	12744.0
75.00	34232.0
76.10	2941.0
77.20	449.0
77.90	286.0
78.90	3708.0
80.00	887.0
80.90	4456.0
82.00	608.0
87.00	3899.0
88.00	4039.0
90.90	330.0
92.00	2788.0
93.00	3557.0
94.10	8767.0
95.10	71680.0
96.10	4583.0
104.10	429.0
106.00	533.0
107.90	199.0
115.70	185.0
116.80	933.0
117.80	245.0
119.00	563.0
127.90	292.0
140.80	734.0
143.00	1026.0
144.10	217.0
145.00	580.0
145.90	172.0
155.00	162.0
157.00	274.0
170.90	268.0
172.00	528.0
172.90	1131.0
174.00	72800.0
174.90	5814.0
176.00	70752.0
176.90	5181.0
207.00	322.0
281.20	606.0
282.00	284.0
283.40	207.0

Instrument :
MSVOA_D
ClientSampleId :
BFB124

m/z	Abundance
36.10	221.0
37.10	2554.0
38.00	2762.0
39.10	1009.0
40.00	1231.0
44.10	812.0
45.10	492.0
46.90	822.0
47.90	469.0
49.00	2557.0
50.10	10973.0
51.00	3141.0
54.90	185.0
55.90	951.0
57.00	1581.0
59.90	564.0
61.10	3829.0
62.00	3157.0
63.10	2853.0
64.10	819.0
65.10	315.0
66.90	234.0
68.00	6374.0
69.00	6007.0
70.00	544.0
72.10	436.0
73.10	3288.0
74.00	10540.0
75.10	32472.0
76.00	2554.0
77.00	676.0
77.90	343.0
79.00	3353.0
79.90	1100.0
81.00	3963.0
82.00	639.0
87.10	3084.0
88.00	3502.0
90.80	225.0
91.30	198.0
92.00	2602.0
93.00	2849.0
94.00	8805.0
95.10	70736.0
96.00	4177.0
104.00	257.0
105.90	345.0
115.80	340.0
117.00	314.0
117.90	411.0
119.00	518.0
127.90	157.0
129.80	190.0
132.90	221.0
134.70	193.0
140.80	509.0
142.80	865.0
143.10	810.0
143.80	154.0
145.00	587.0
147.90	256.0
149.80	158.0
154.80	206.0
171.00	328.0
171.80	746.0
172.90	1106.0
174.00	71080.0
175.00	4697.0
176.00	68968.0
177.00	4458.0
207.20	249.0
281.10	1132.0
281.90	252.0

Instrument :
MSVOA_D
ClientSampleId :
BFB124