



Methyl methacrylate

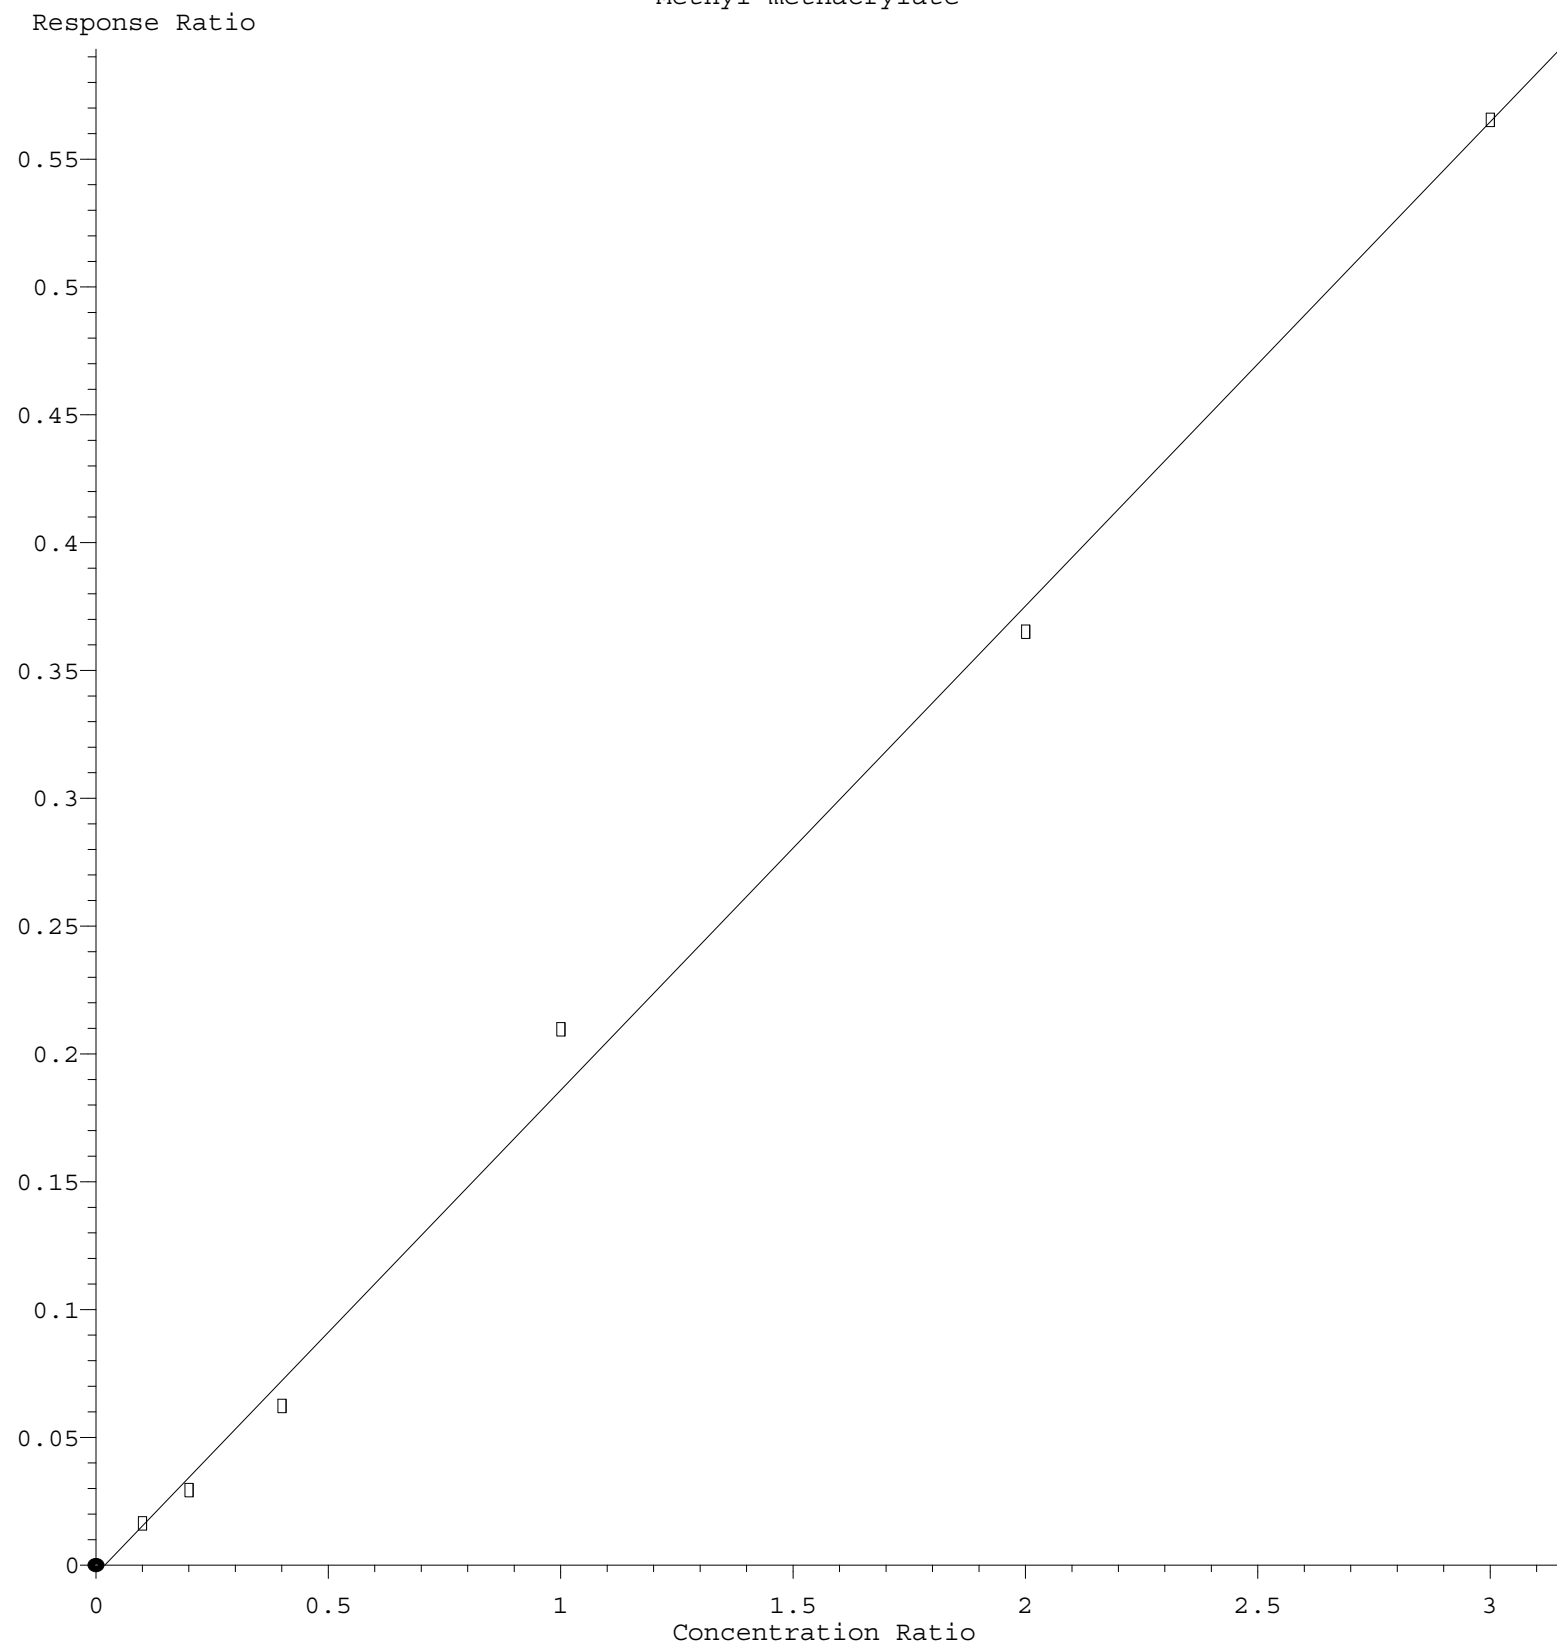

$\text{Response} = 1.894\text{e-}001 * \text{Amt} - 3.524\text{e-}003$
 Coef of Det (r^2) = 0.996727 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D050321S.M
 Calibration Table Last Updated: Tue May 04 03:51:01 2021

Methyl Iodide

Response Ratio

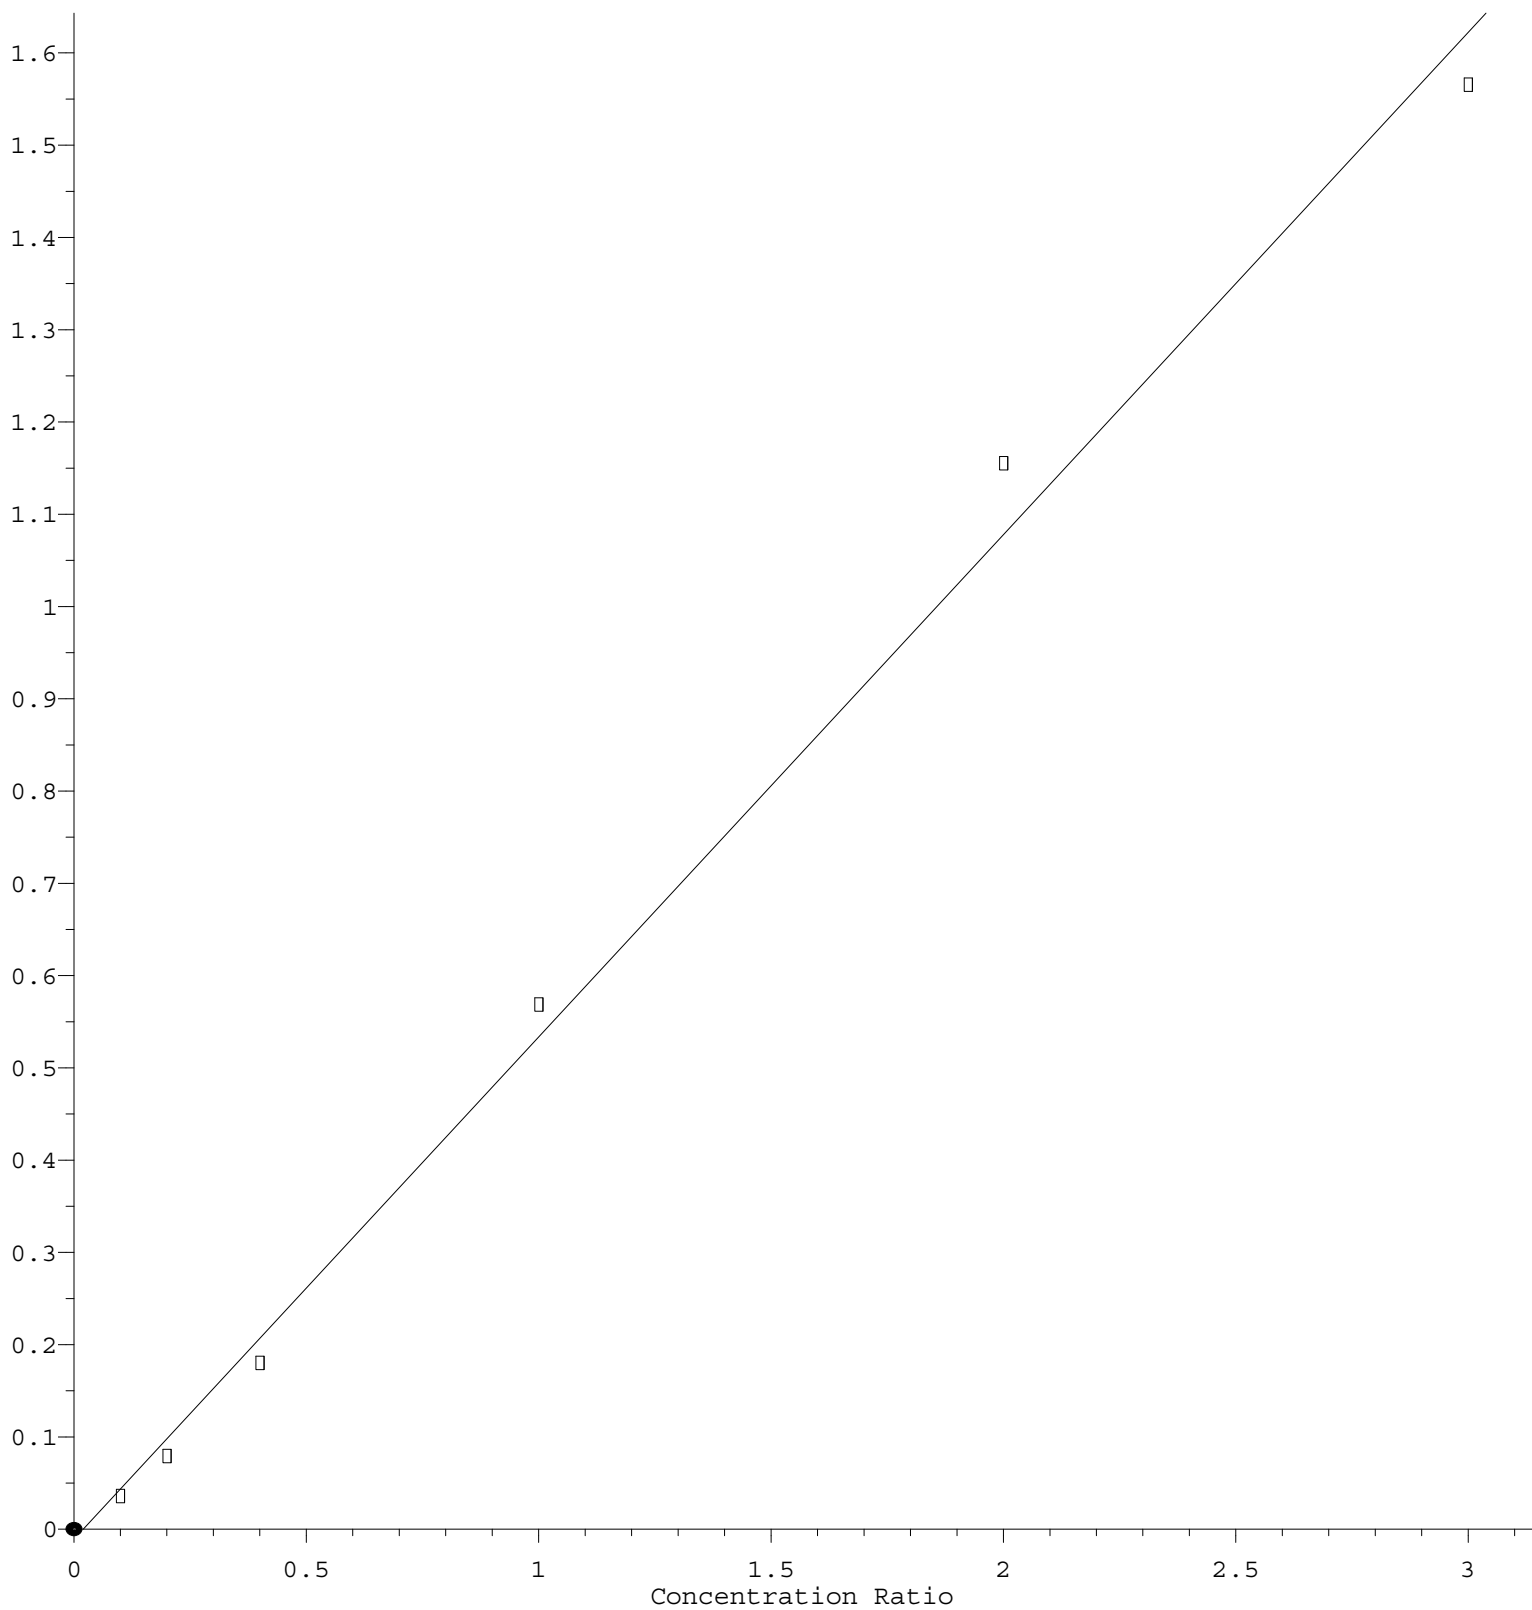


$$\text{Response} = 5.446\text{e-}001 * \text{Amt} - 1.068\text{e-}002$$

Coef of Det (r^2) = 0.994253 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D050321S.M

Calibration Table Last Updated: Tue May 04 03:51:01 2021


Tert butyl alcohol

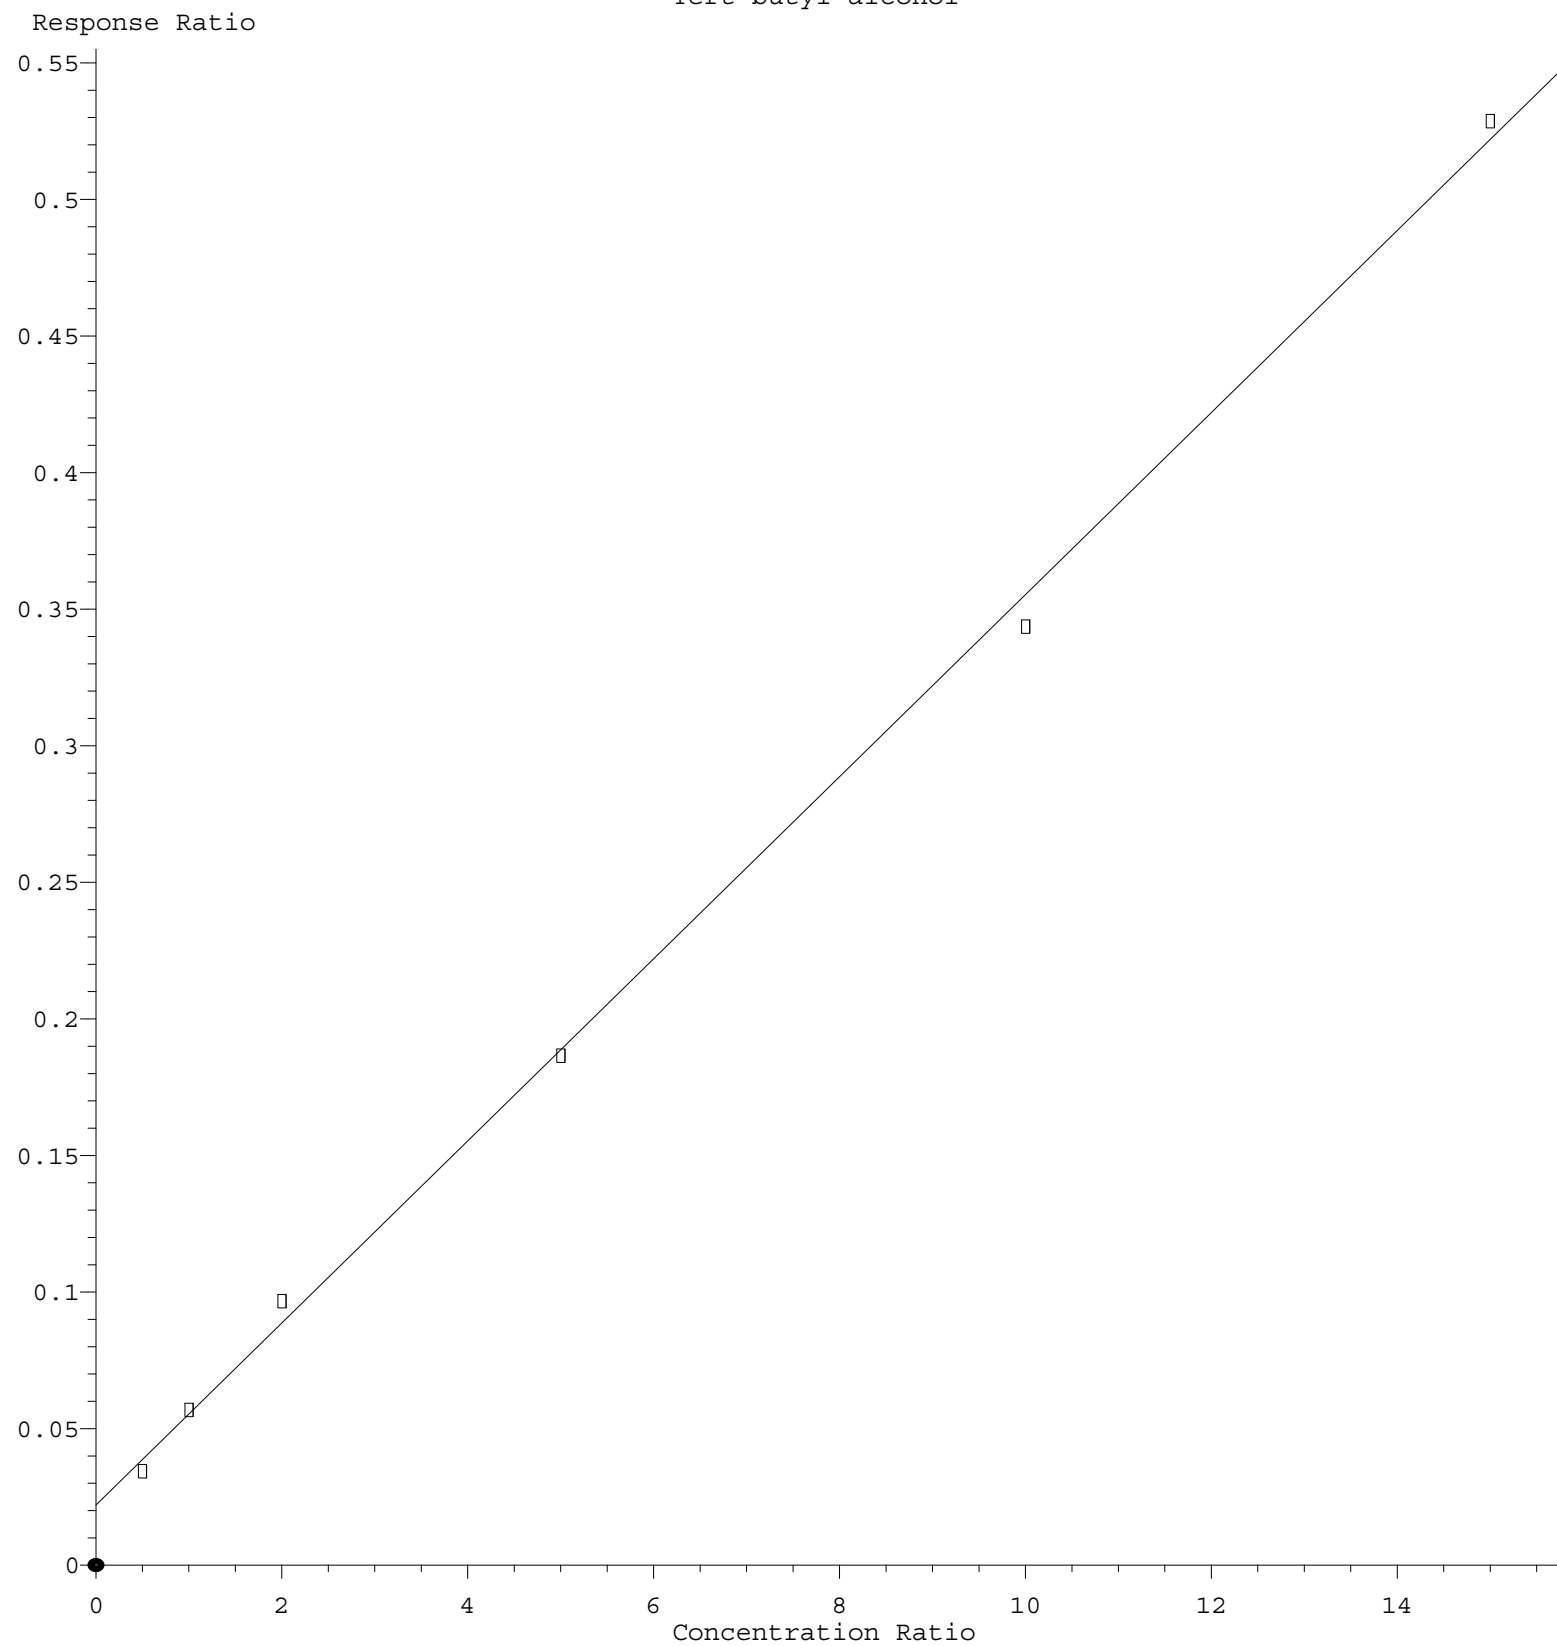

Response = $3.332 \times 10^{-2} \times \text{Amt} + 2.172 \times 10^{-2}$
Coef of Det (r^2) = 0.998556 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D050321S.M
Calibration Table Last Updated: Tue May 04 03:51:01 2021

Methylene Chloride

Response Ratio

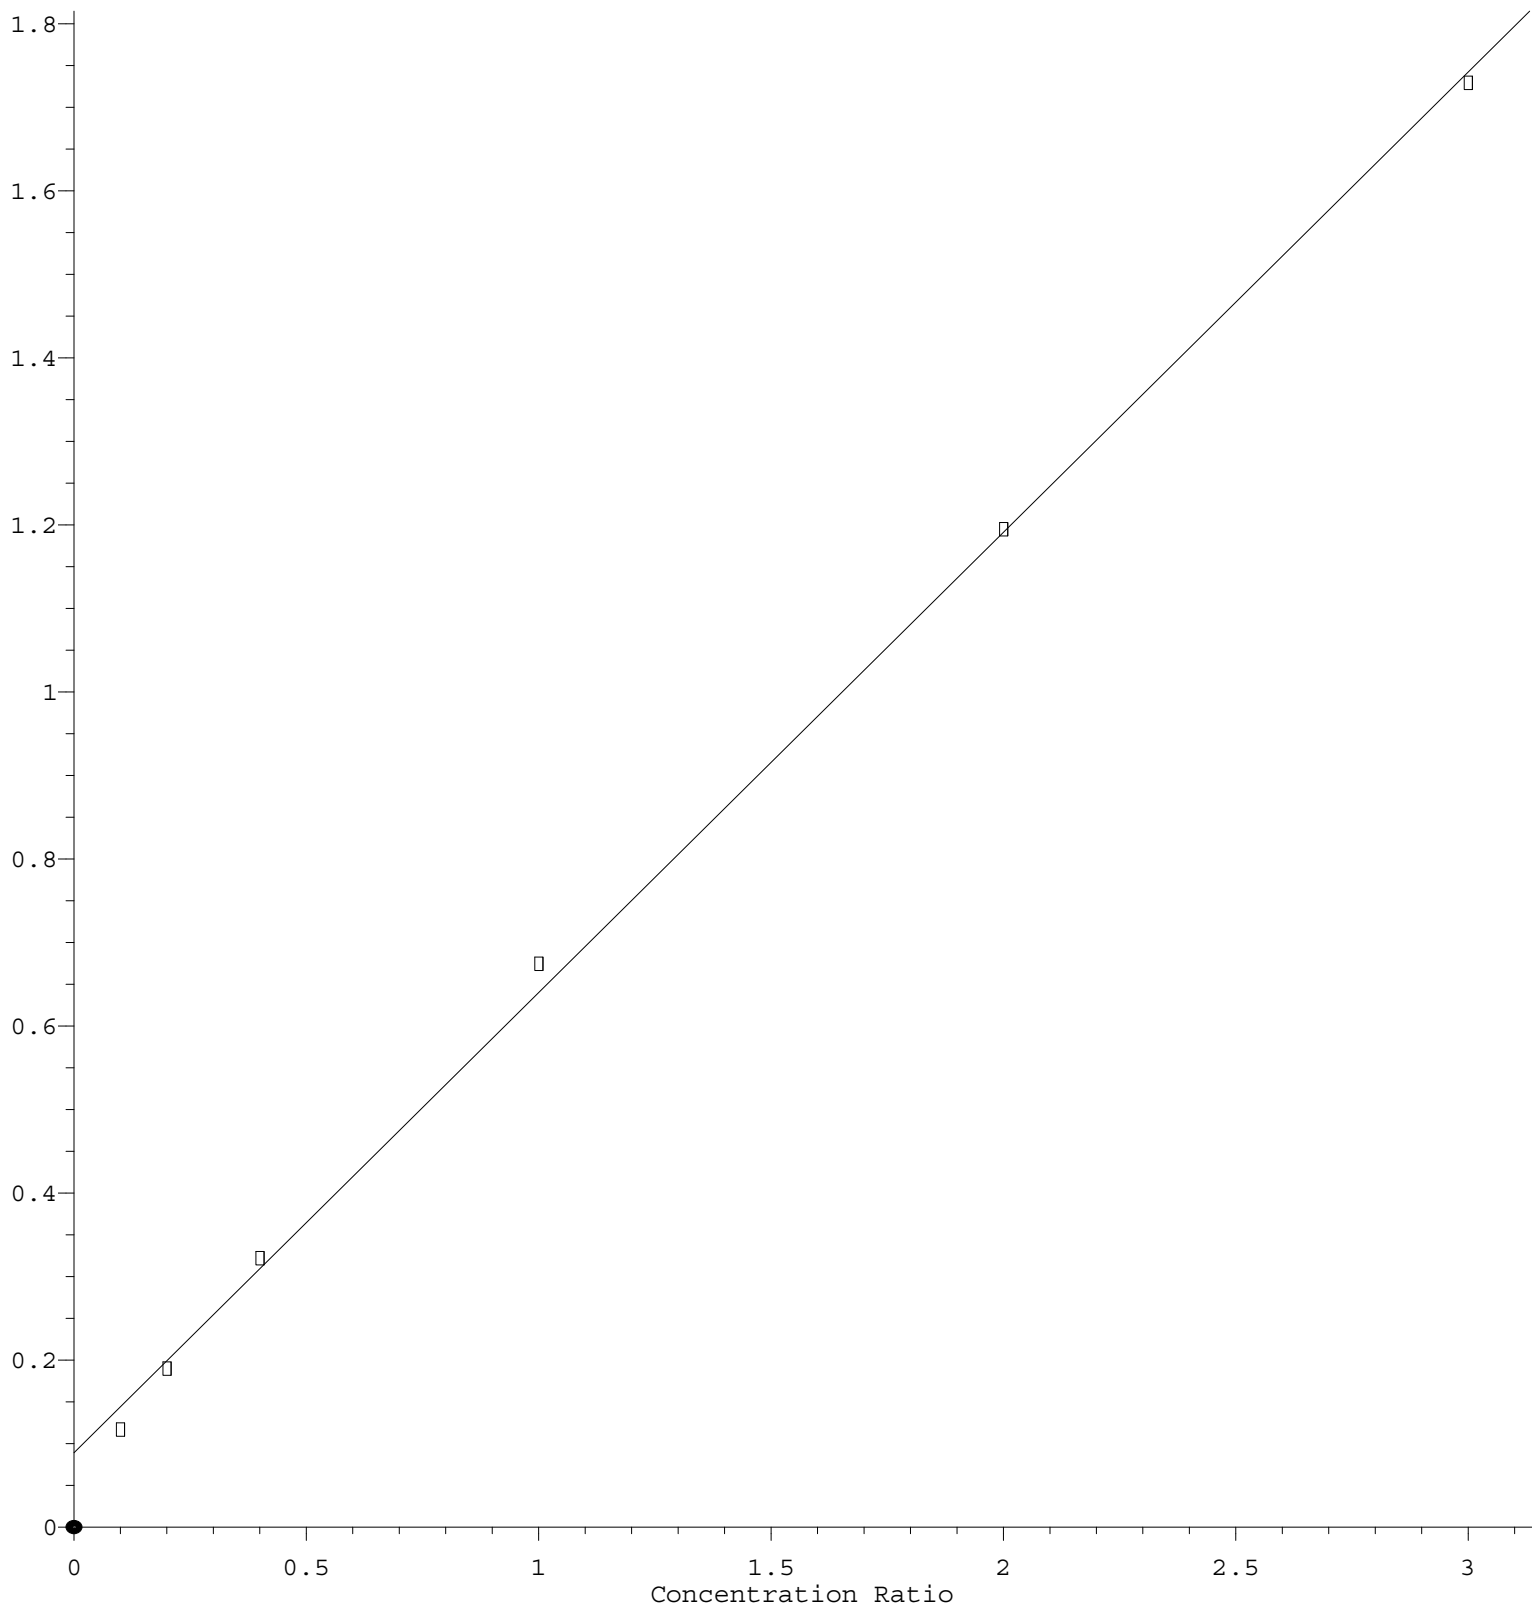

$$\text{Response} = 5.513\text{e-}001 * \text{Amt} + 8.886\text{e-}002$$


Coef of Det (r^2) = 0.998850 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D050321S.M

Calibration Table Last Updated: Tue May 04 03:51:01 2021

Chloroethane

Response Ratio

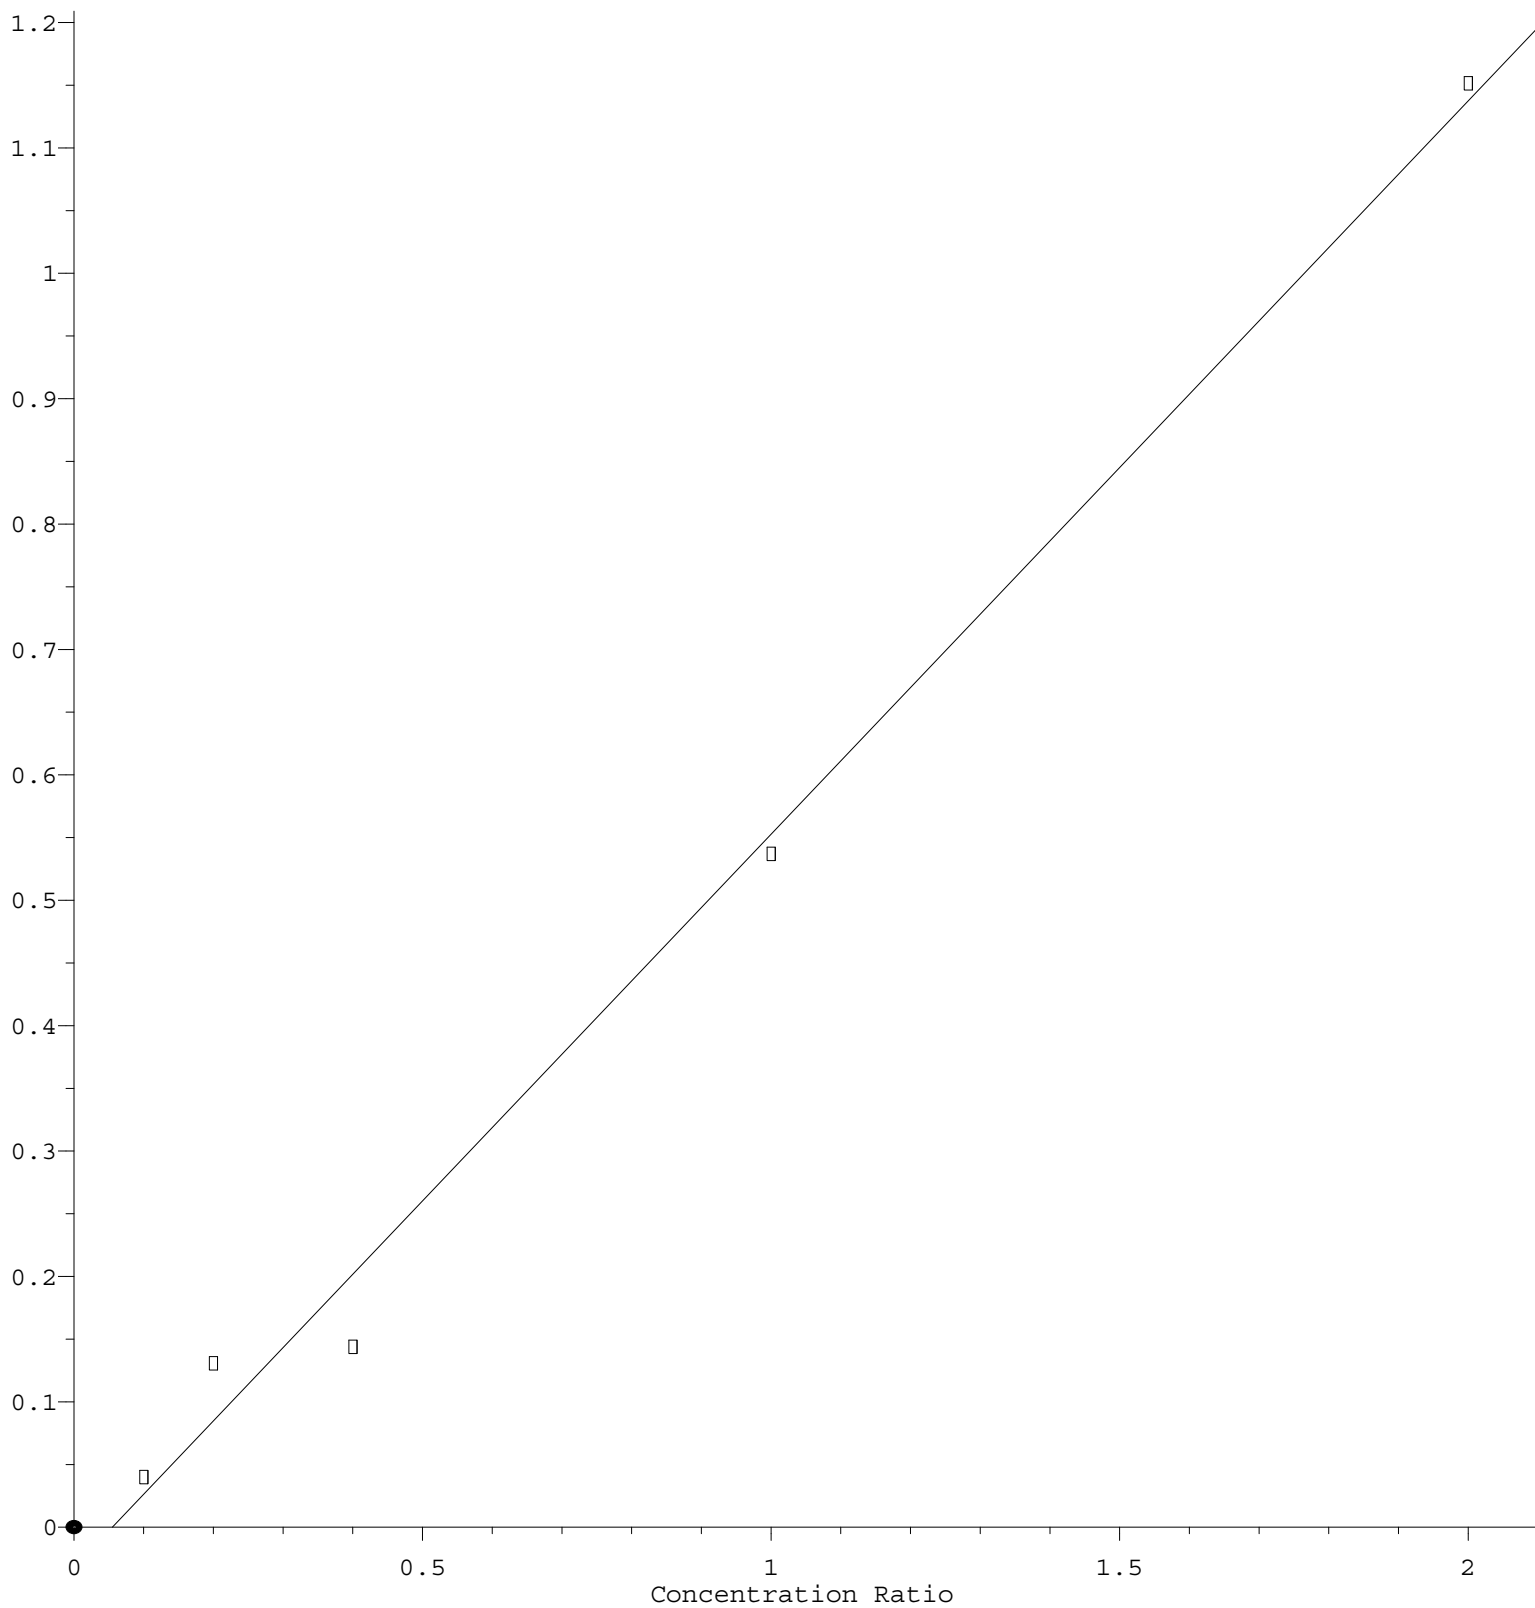

$$\text{Response} = 5.847\text{e-}001 * \text{Amt} - 3.213\text{e-}002$$

Coef of Det (r^2) = 0.992831 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D050321S.M

Calibration Table Last Updated: Tue May 04 03:51:01 2021