
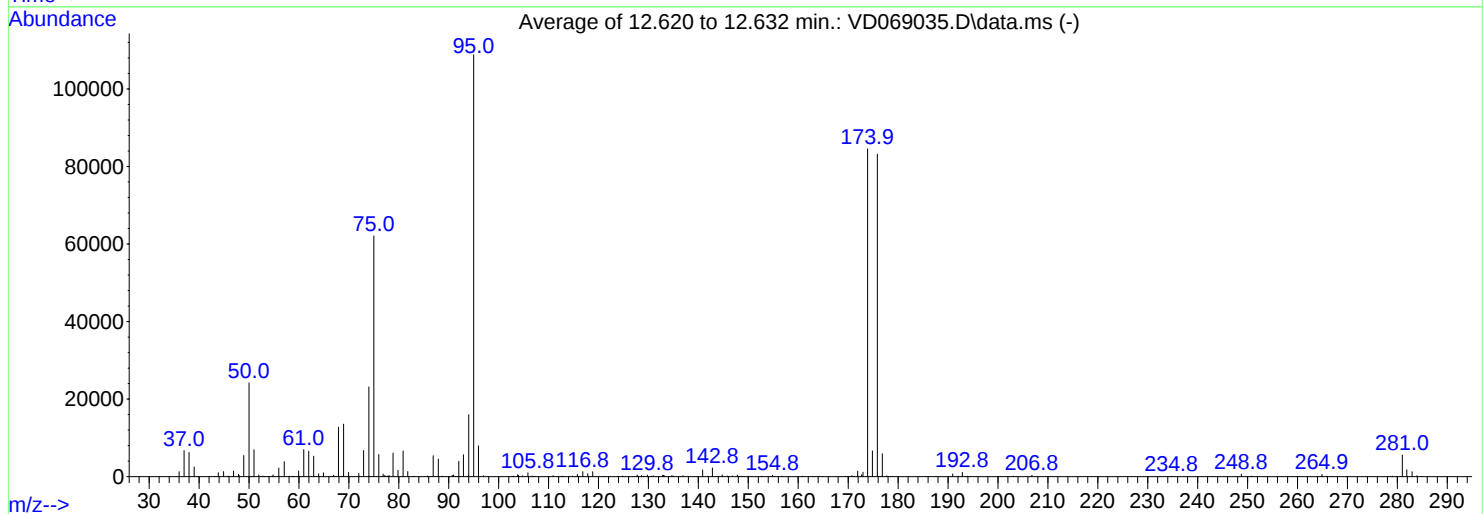


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050321\
Data File : VD069035.D
Acq On : 03 May 2021 10:14
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050321S.M
Title : SW846 8260
Last Update : Tue May 04 03:51:01 2021

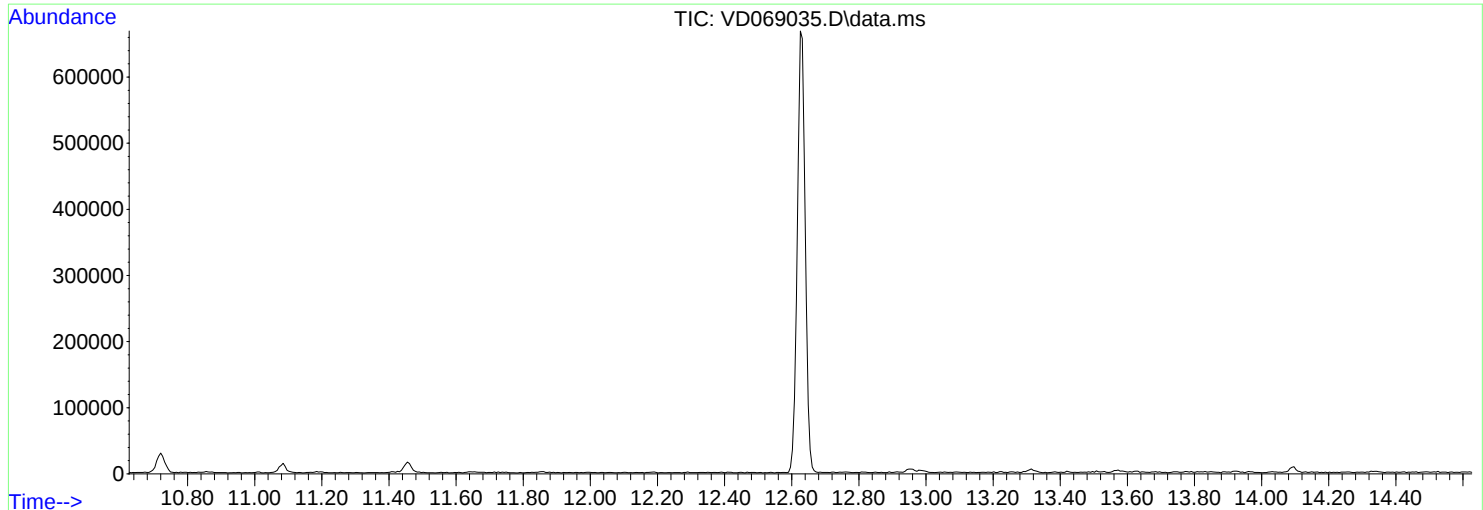

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	24192	PASS
75	95	30	60	57.1	62075	PASS
95	95	100	100	100.0	108795	PASS
96	95	5	9	7.3	7941	PASS
173	174	0.00	2	1.4	1145	PASS
174	95	50	100	77.7	84579	PASS
175	174	5	9	7.8	6634	PASS
176	174	95	101	98.4	83184	PASS
177	176	5	9	7.1	5918	PASS