
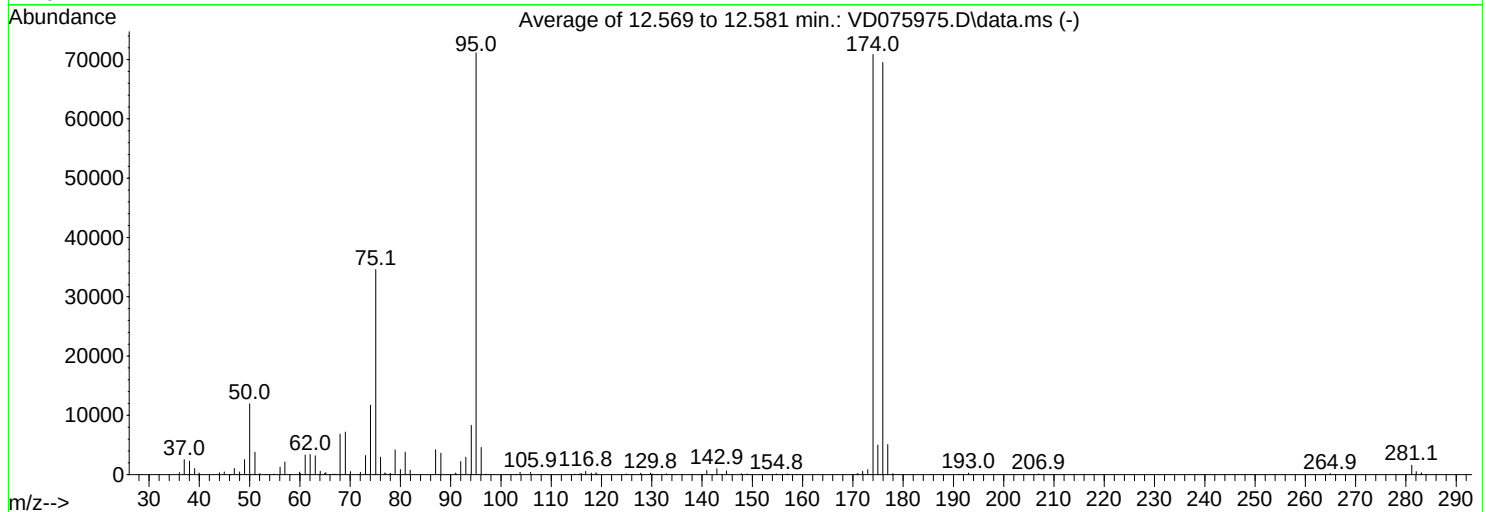


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050323\
 Data File : VD075975.D
 Acq On : 03 May 2023 10:04
 Operator : KP/SY
 Sample : BFB125
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB125

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Title : SFAM01.0
 Last Update : Thu May 04 02:54:49 2023

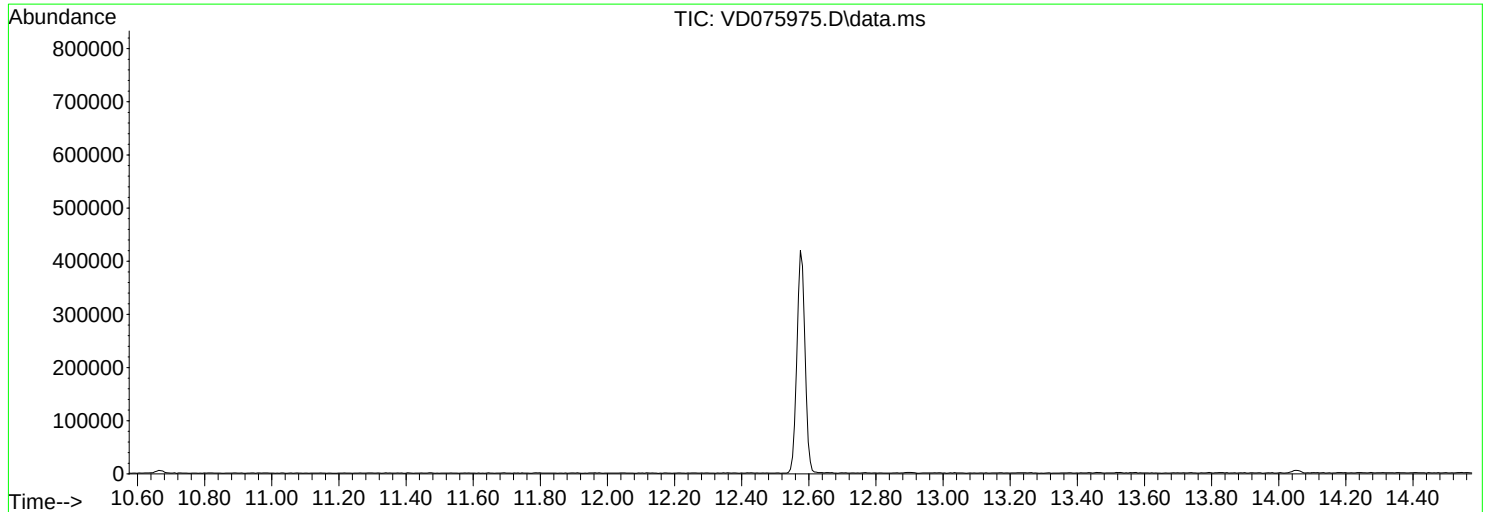

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	11950	PASS
75	95	30	80	48.6	34595	PASS
95	95	100	100	100.0	71133	PASS
96	95	5	9	6.5	4595	PASS
173	174	0.00	2	1.2	846	PASS
174	95	50	120	99.6	70864	PASS
175	174	5	9	7.1	5004	PASS
176	174	95	105	98.1	69517	PASS
177	176	5	10	7.3	5074	PASS

Scan 1860 (12.528 min): VD075975.D\data.ms
BFB125

m/z	Abundance
40.00	826.0
44.00	815.0

Instrument :
MSVOA_D
ClientSampleId :
BFB125

m/z	Abundance
36.10	320.0
37.00	2560.0
38.10	2303.0
39.10	826.0
40.00	990.0
44.10	1005.0
44.90	445.0
47.00	1114.0
48.10	334.0
49.00	2513.0
50.00	11138.0
51.10	3484.0
52.00	188.0
56.00	1377.0
57.00	1895.0
60.00	670.0
61.10	3009.0
62.10	2871.0
63.10	2764.0
64.00	391.0
65.00	297.0
66.80	168.0
68.00	6372.0
69.00	6405.0
70.00	526.0
72.10	337.0
73.10	3006.0
74.00	10455.0
75.10	30328.0
76.00	2513.0
76.90	420.0
78.10	315.0
78.90	3799.0
80.10	912.0
81.00	3513.0
81.90	609.0
85.90	196.0
87.00	3793.0
88.00	3517.0
90.90	310.0
92.00	1718.0
93.00	2951.0
94.10	7589.0
95.10	61160.0
96.00	4136.0
103.80	352.0
105.90	396.0
116.00	279.0
116.80	367.0
118.00	329.0
118.90	400.0
127.80	200.0
129.80	230.0
133.00	205.0
140.90	491.0
143.00	888.0
144.80	462.0
154.80	175.0
170.90	409.0
172.00	465.0
173.00	694.0
174.00	62472.0
174.90	4364.0
175.90	60864.0
177.00	4057.0
178.00	178.0
193.10	207.0
281.10	945.0
282.00	326.0
282.90	229.0

Instrument :
MSVOA_D
ClientSampleId :
BFB125

m/z	Abundance
35.90	390.0
37.00	2783.0
38.10	2085.0
39.10	1137.0
39.90	1225.0
44.10	966.0
45.00	482.0
46.20	158.0
46.90	1058.0
48.00	603.0
49.00	2619.0
50.00	12495.0
51.00	3811.0
52.10	194.0
53.20	184.0
53.80	191.0
54.80	212.0
56.10	1201.0
57.00	2300.0
59.80	630.0
61.00	4078.0
62.00	4001.0
63.00	3759.0
64.10	930.0
64.90	391.0
65.20	474.0
66.80	182.0
67.20	241.0
68.00	7503.0
69.10	8105.0
70.10	525.0
71.90	496.0
73.00	3463.0
74.10	13680.0
75.10	38336.0
76.10	3483.0
76.90	498.0
77.80	299.0
78.90	4182.0
79.90	699.0
80.90	4097.0
82.00	923.0
87.00	5205.0
88.10	4187.0
90.90	480.0
92.00	2772.0
93.00	3281.0
94.10	9515.0
95.10	80096.0
96.00	4734.0
97.00	322.0
103.70	159.0
106.00	366.0
108.10	183.0
115.90	399.0
116.90	790.0
117.90	314.0
118.90	545.0
124.80	171.0
127.80	266.0
129.70	198.0
130.10	295.0
131.00	176.0
133.20	152.0
140.90	679.0
142.90	1118.0
144.90	948.0
147.90	259.0
149.00	216.0
157.00	156.0
171.10	331.0
171.80	587.0
172.90	822.0
174.00	77120.0
174.90	5393.0
176.00	73424.0
177.00	5764.0
177.90	204.0
192.90	322.0
206.90	263.0
265.00	417.0
281.20	1660.0
282.00	318.0
283.10	538.0

Instrument :
MSVOA_D
ClientSampleId :
BFB125

m/z	Abundance
36.10	312.0
37.00	2263.0
38.00	2386.0
39.00	1111.0
39.90	1156.0
44.00	1444.0
45.00	419.0
46.90	947.0
47.90	417.0
49.00	2521.0
50.00	12218.0
51.00	4048.0
52.00	172.0
54.00	195.0
54.90	158.0
56.10	1207.0
57.00	2235.0
58.10	185.0
60.10	672.0
61.00	2884.0
62.10	3297.0
63.10	3049.0
64.10	461.0
65.10	567.0
68.00	6577.0
69.00	7015.0
70.10	471.0
72.10	420.0
73.00	3158.0
74.00	11040.0
75.10	35120.0
76.10	2848.0
77.10	508.0
78.00	362.0
79.00	4555.0
80.00	994.0
80.90	3786.0
82.00	759.0
87.00	3621.0
88.00	3187.0
91.10	401.0
92.00	2164.0
93.00	2602.0
94.10	7820.0
95.00	72144.0
96.10	4914.0
102.90	177.0
103.80	693.0
105.80	419.0
114.70	248.0
115.70	297.0
116.80	559.0
117.90	196.0
119.10	349.0
125.00	350.0
127.80	300.0
129.70	400.0
132.80	316.0
134.70	153.0
141.00	955.0
142.90	987.0
144.80	455.0
147.70	196.0
148.90	208.0
154.80	245.0
156.90	250.0
158.80	166.0
170.80	150.0
172.00	643.0
173.00	1021.0
174.00	73000.0
175.00	5255.0
176.00	74264.0
176.90	5401.0
178.00	189.0
191.00	258.0
193.00	302.0
207.00	191.0
264.90	152.0
281.10	2140.0
282.10	885.0
283.10	366.0

Instrument :
MSVOA_D
ClientSampleId :
BFB125