


Methyl Iodide

Response Ratio

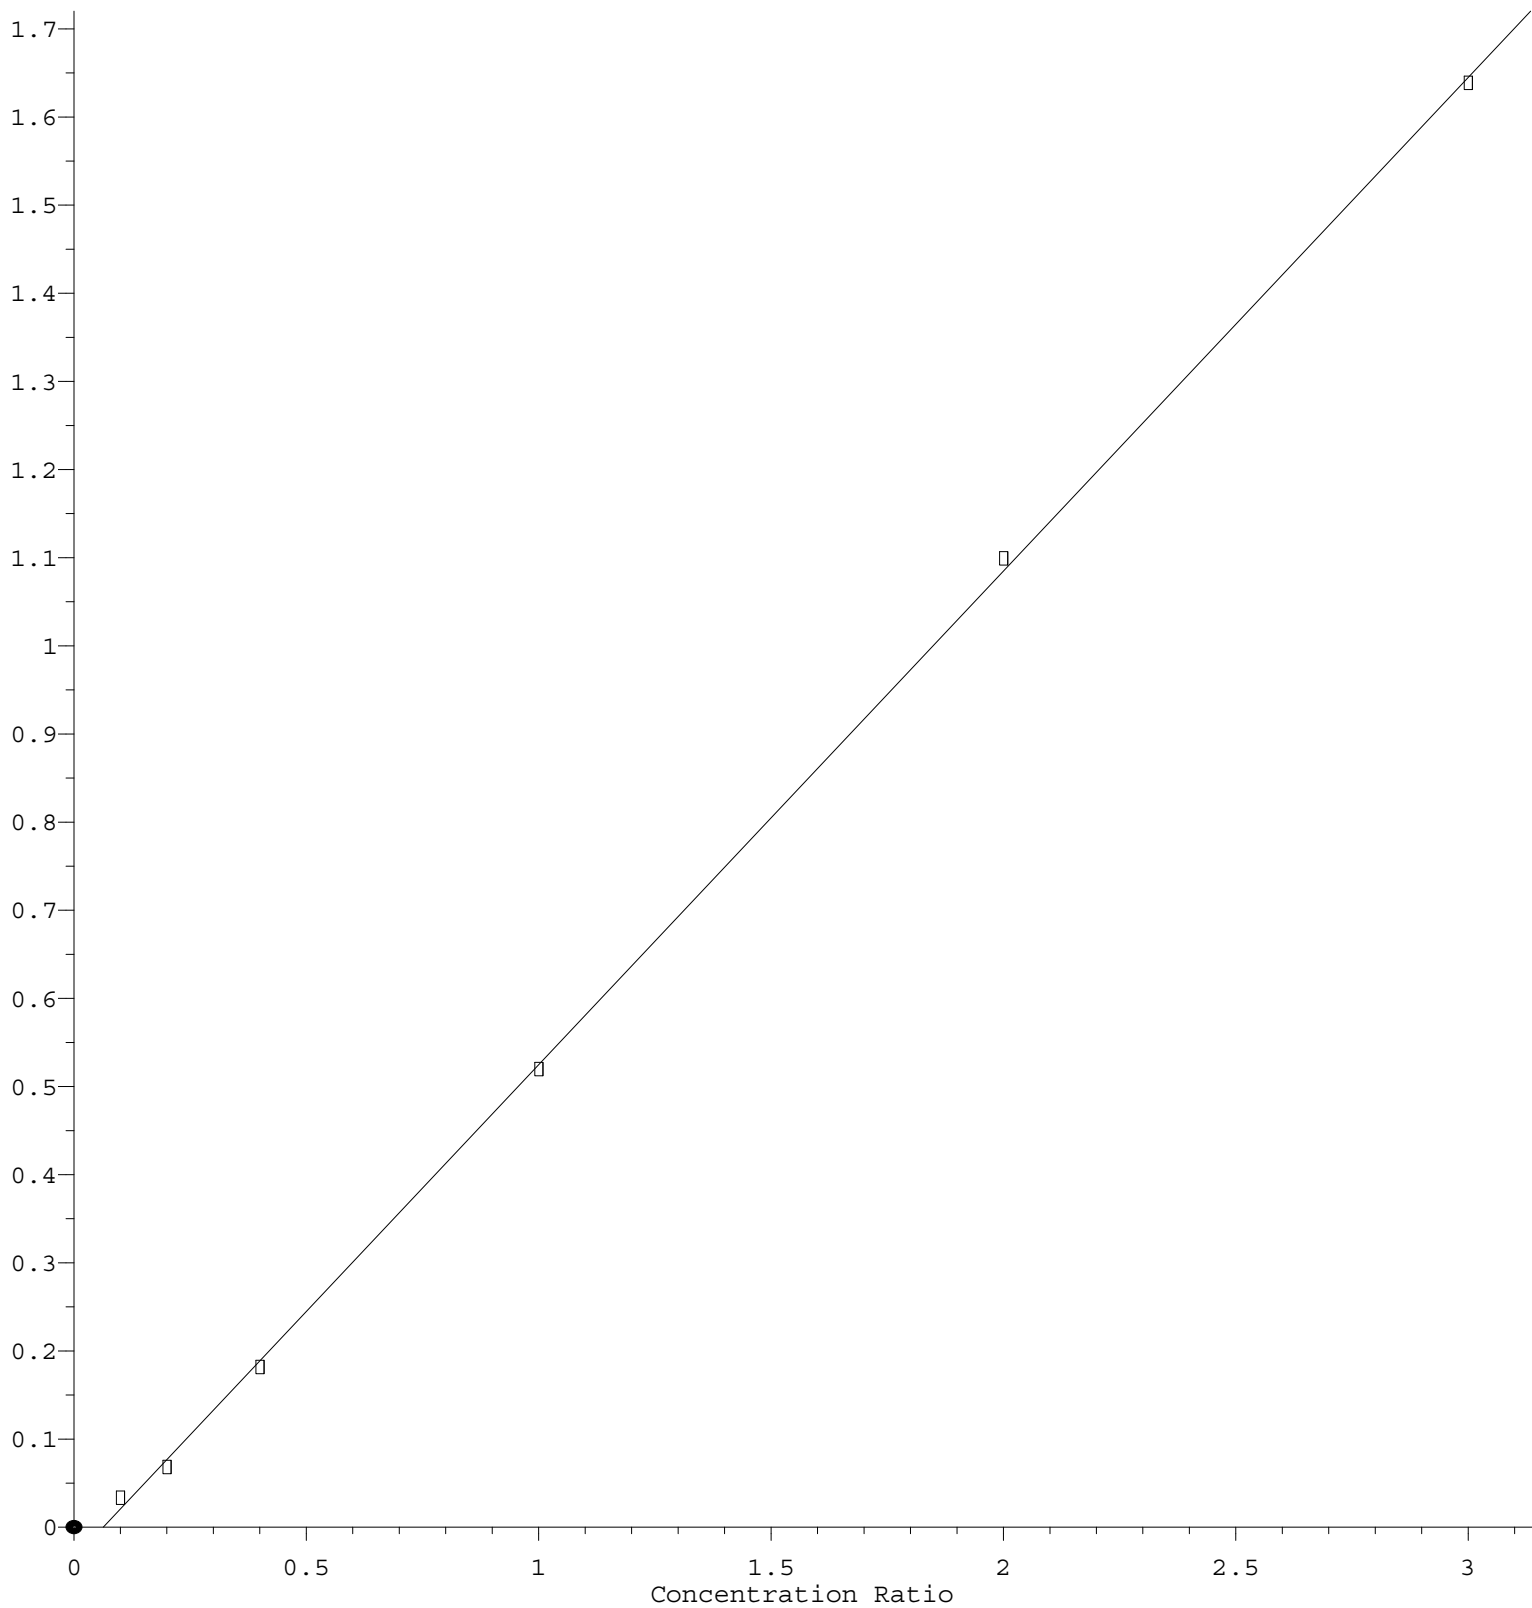

$$\text{Response} = 5.603\text{e-}001 * \text{Amt} - 3.551\text{e-}002$$


Coef of Det (r^2) = 0.999738 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D050421S.M

Calibration Table Last Updated: Wed May 05 04:16:41 2021

Ethyl methacrylate

Response Ratio

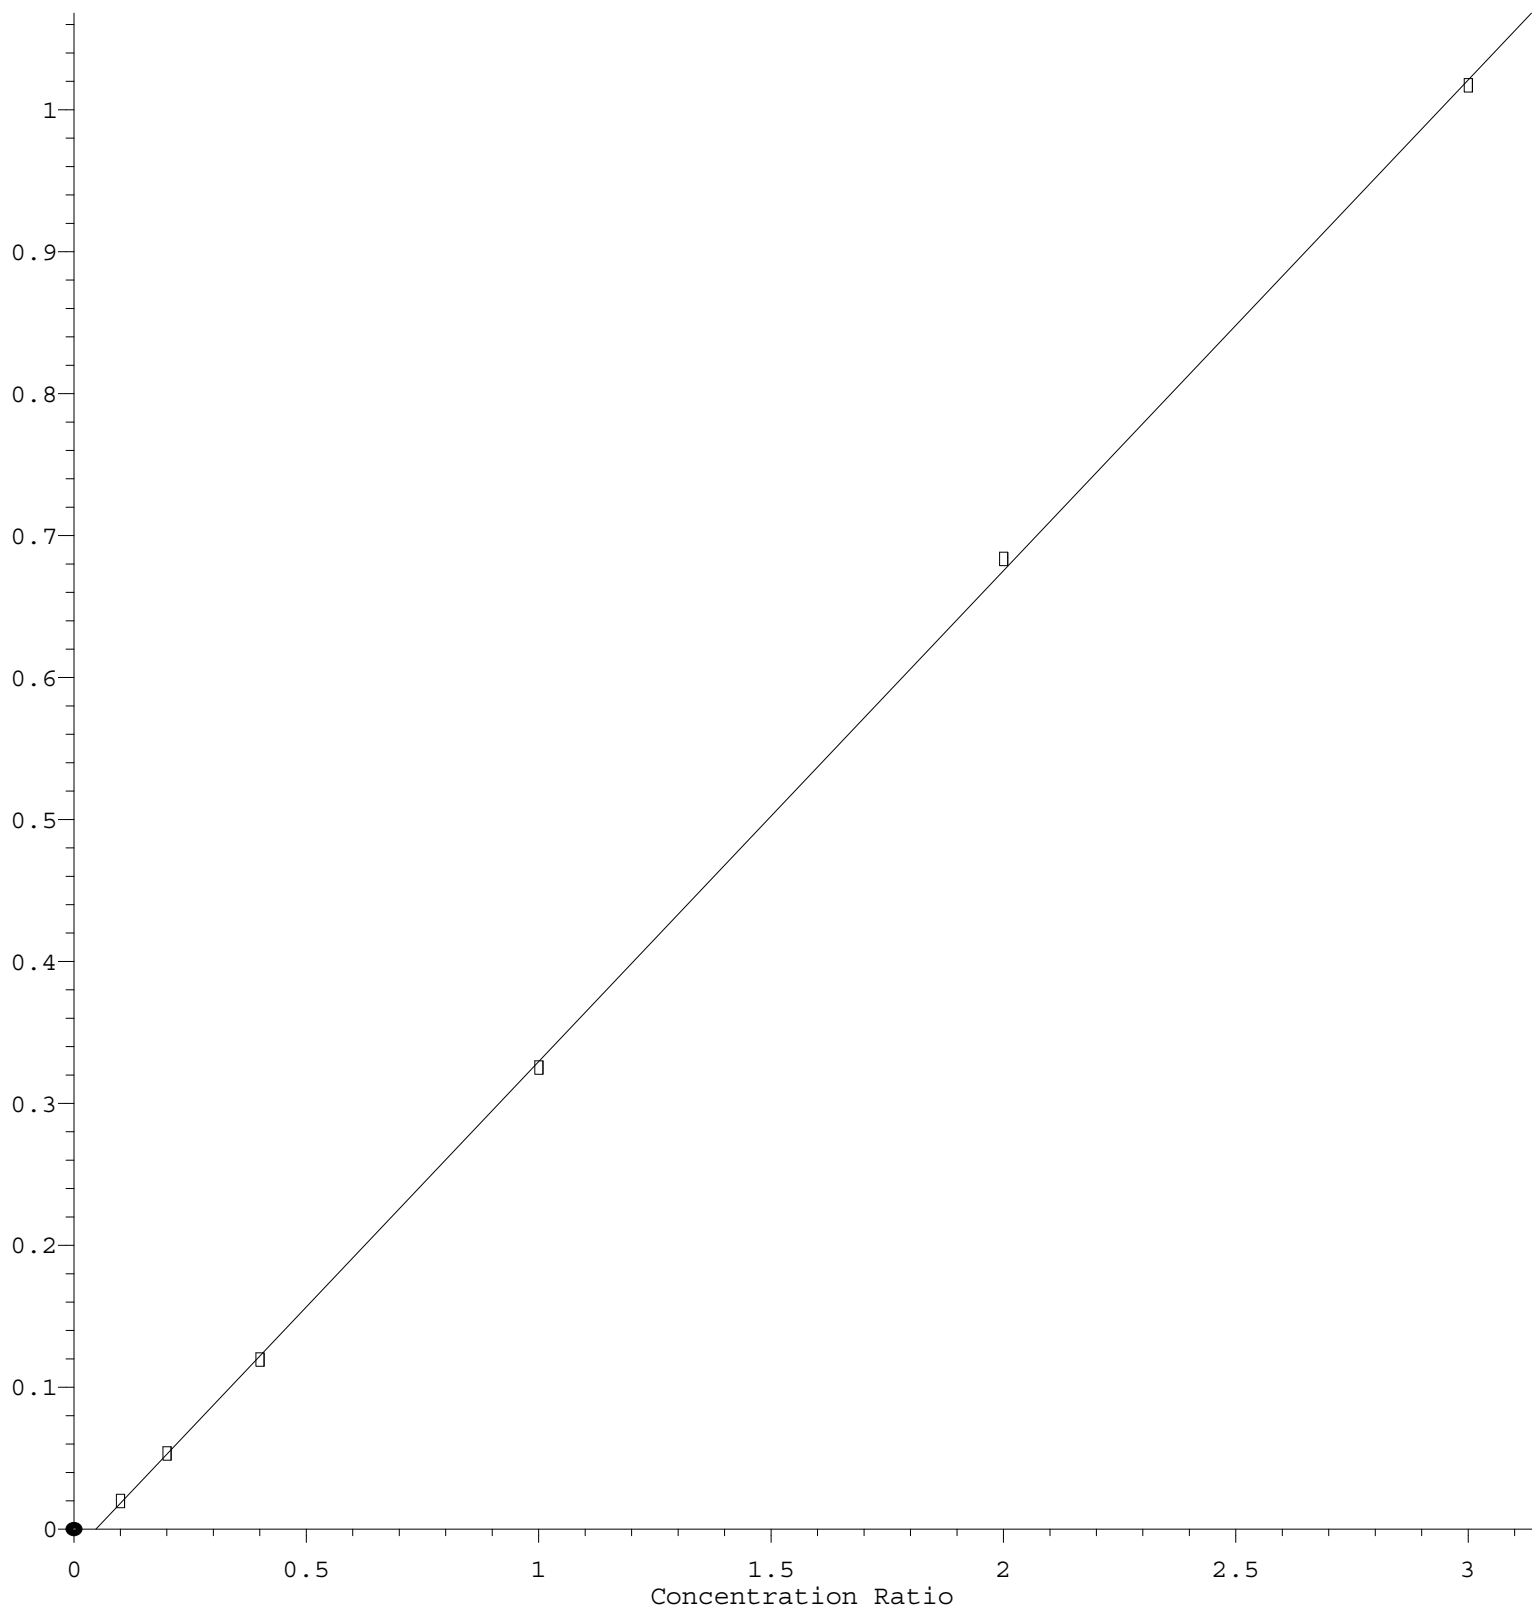

$$\text{Response} = 3.458\text{e-}001 * \text{Amt} - 1.641\text{e-}002$$


Coef of Det (r^2) = 0.999864 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D050421S.M

Calibration Table Last Updated: Wed May 05 04:16:41 2021

Naphthalene

Response Ratio

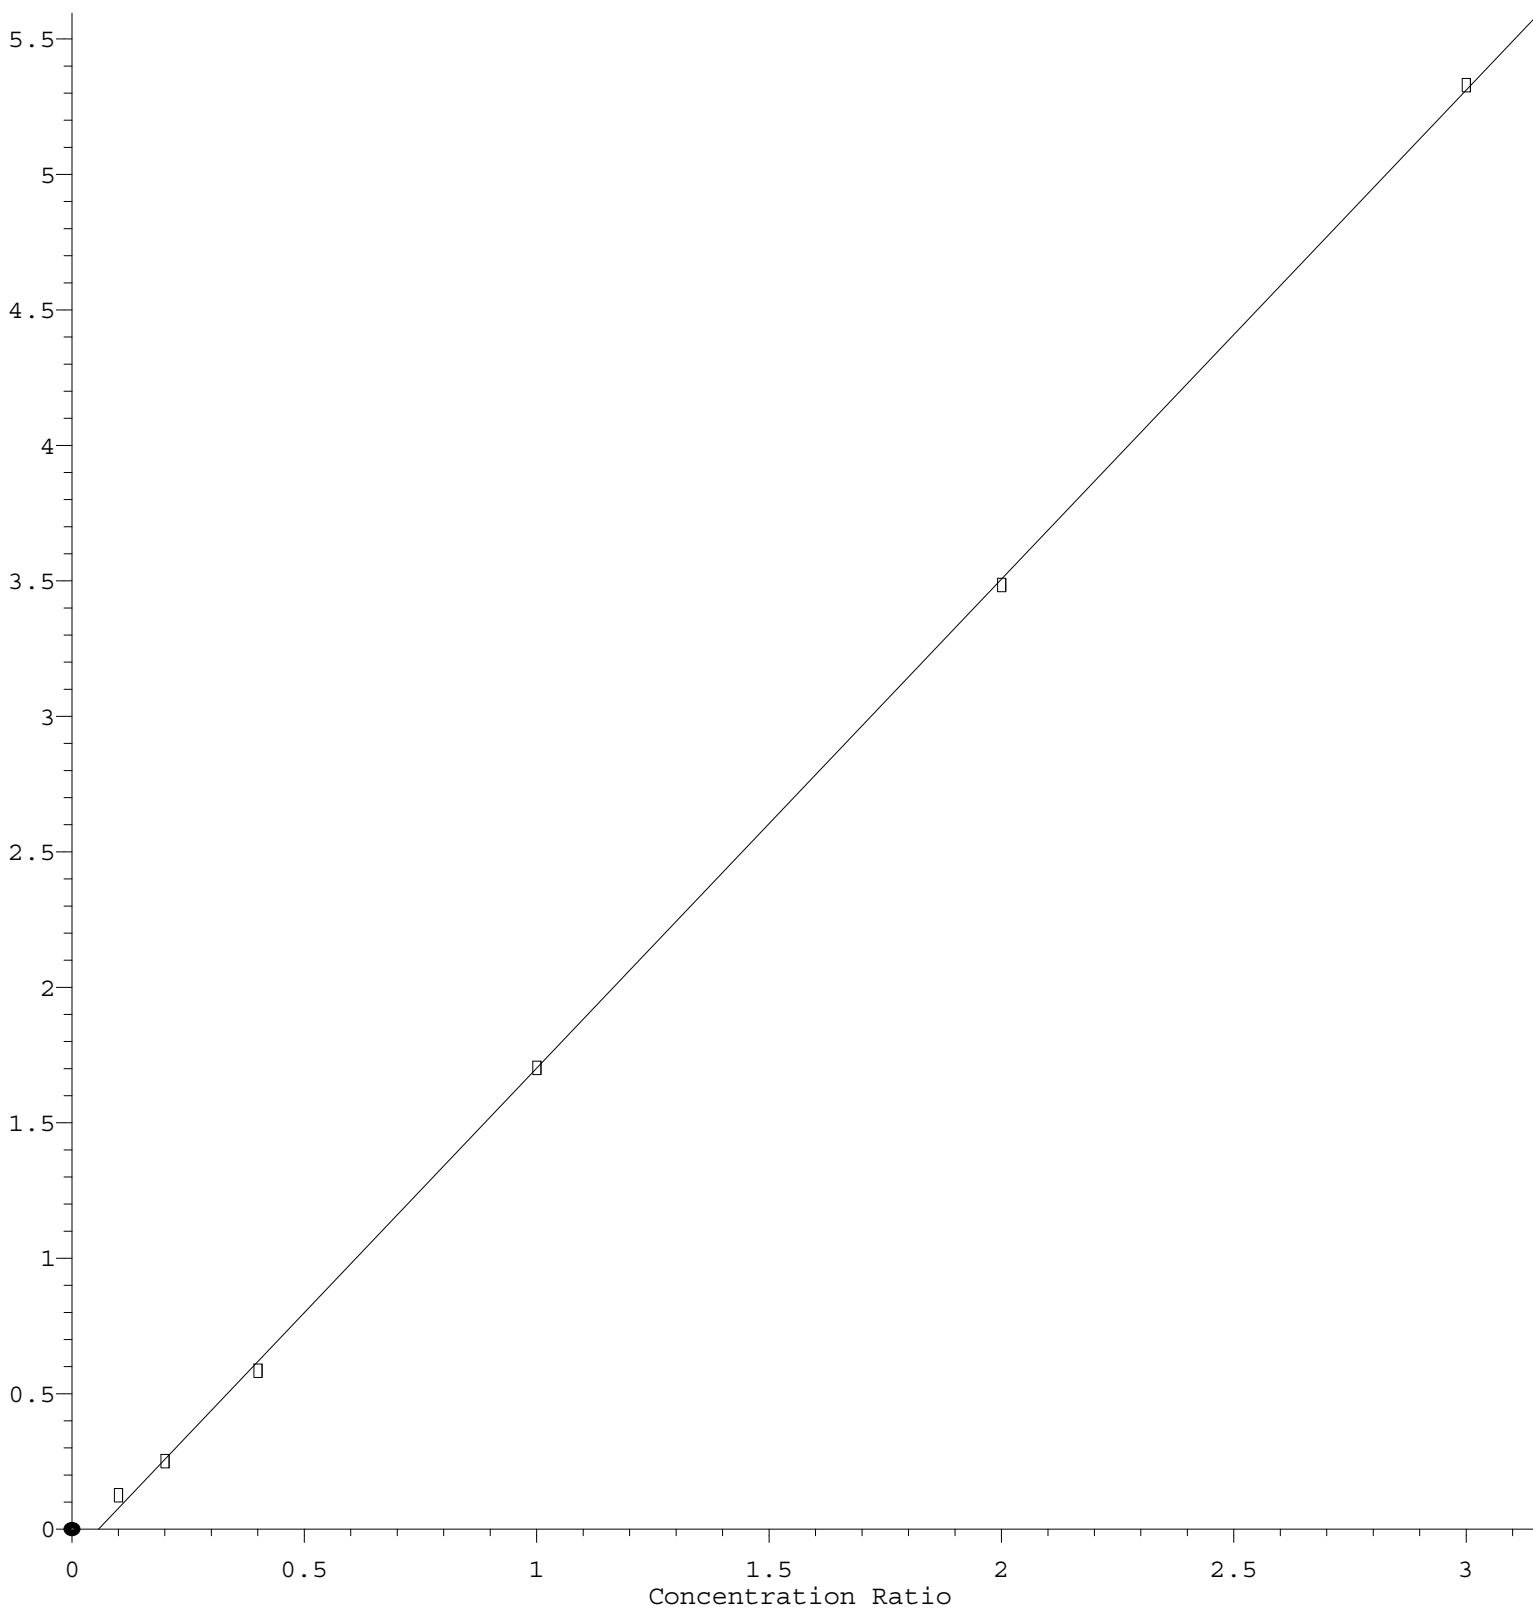


$$\text{Response} = 1.804\text{e}+000 * \text{Amt} - 1.021\text{e}-001$$

Coef of Det (r^2) = 0.999803 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D050421S.M

Calibration Table Last Updated: Wed May 05 04:16:41 2021


Tert butyl alcohol

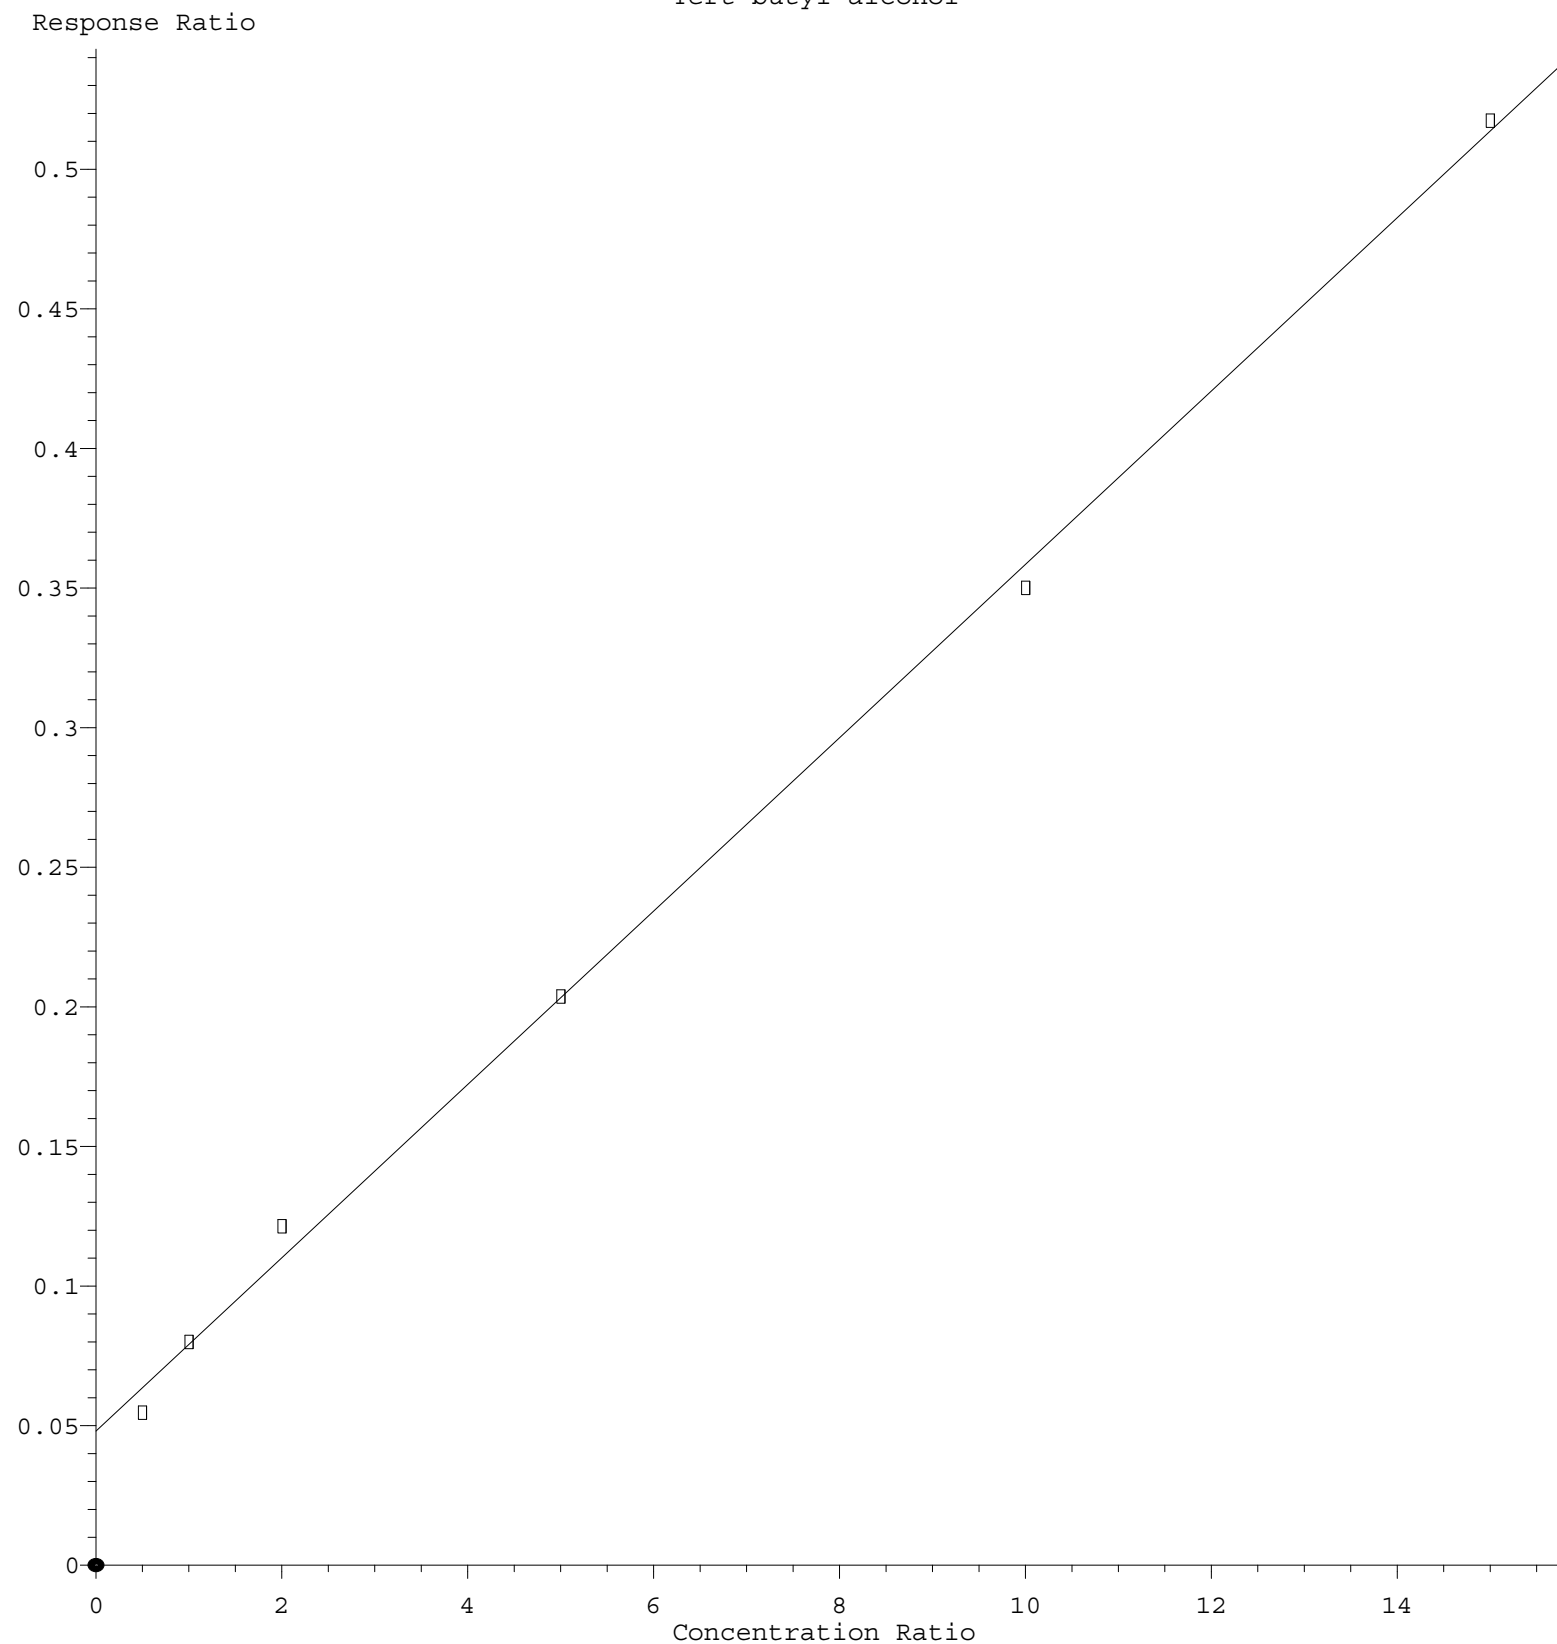

Response = $3.104 \times 10^{-2} \times \text{Amt} + 4.789 \times 10^{-2}$
 Coef of Det (r^2) = 0.998201 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D050421S.M
 Calibration Table Last Updated: Wed May 05 04:16:41 2021

Acetone

Response Ratio

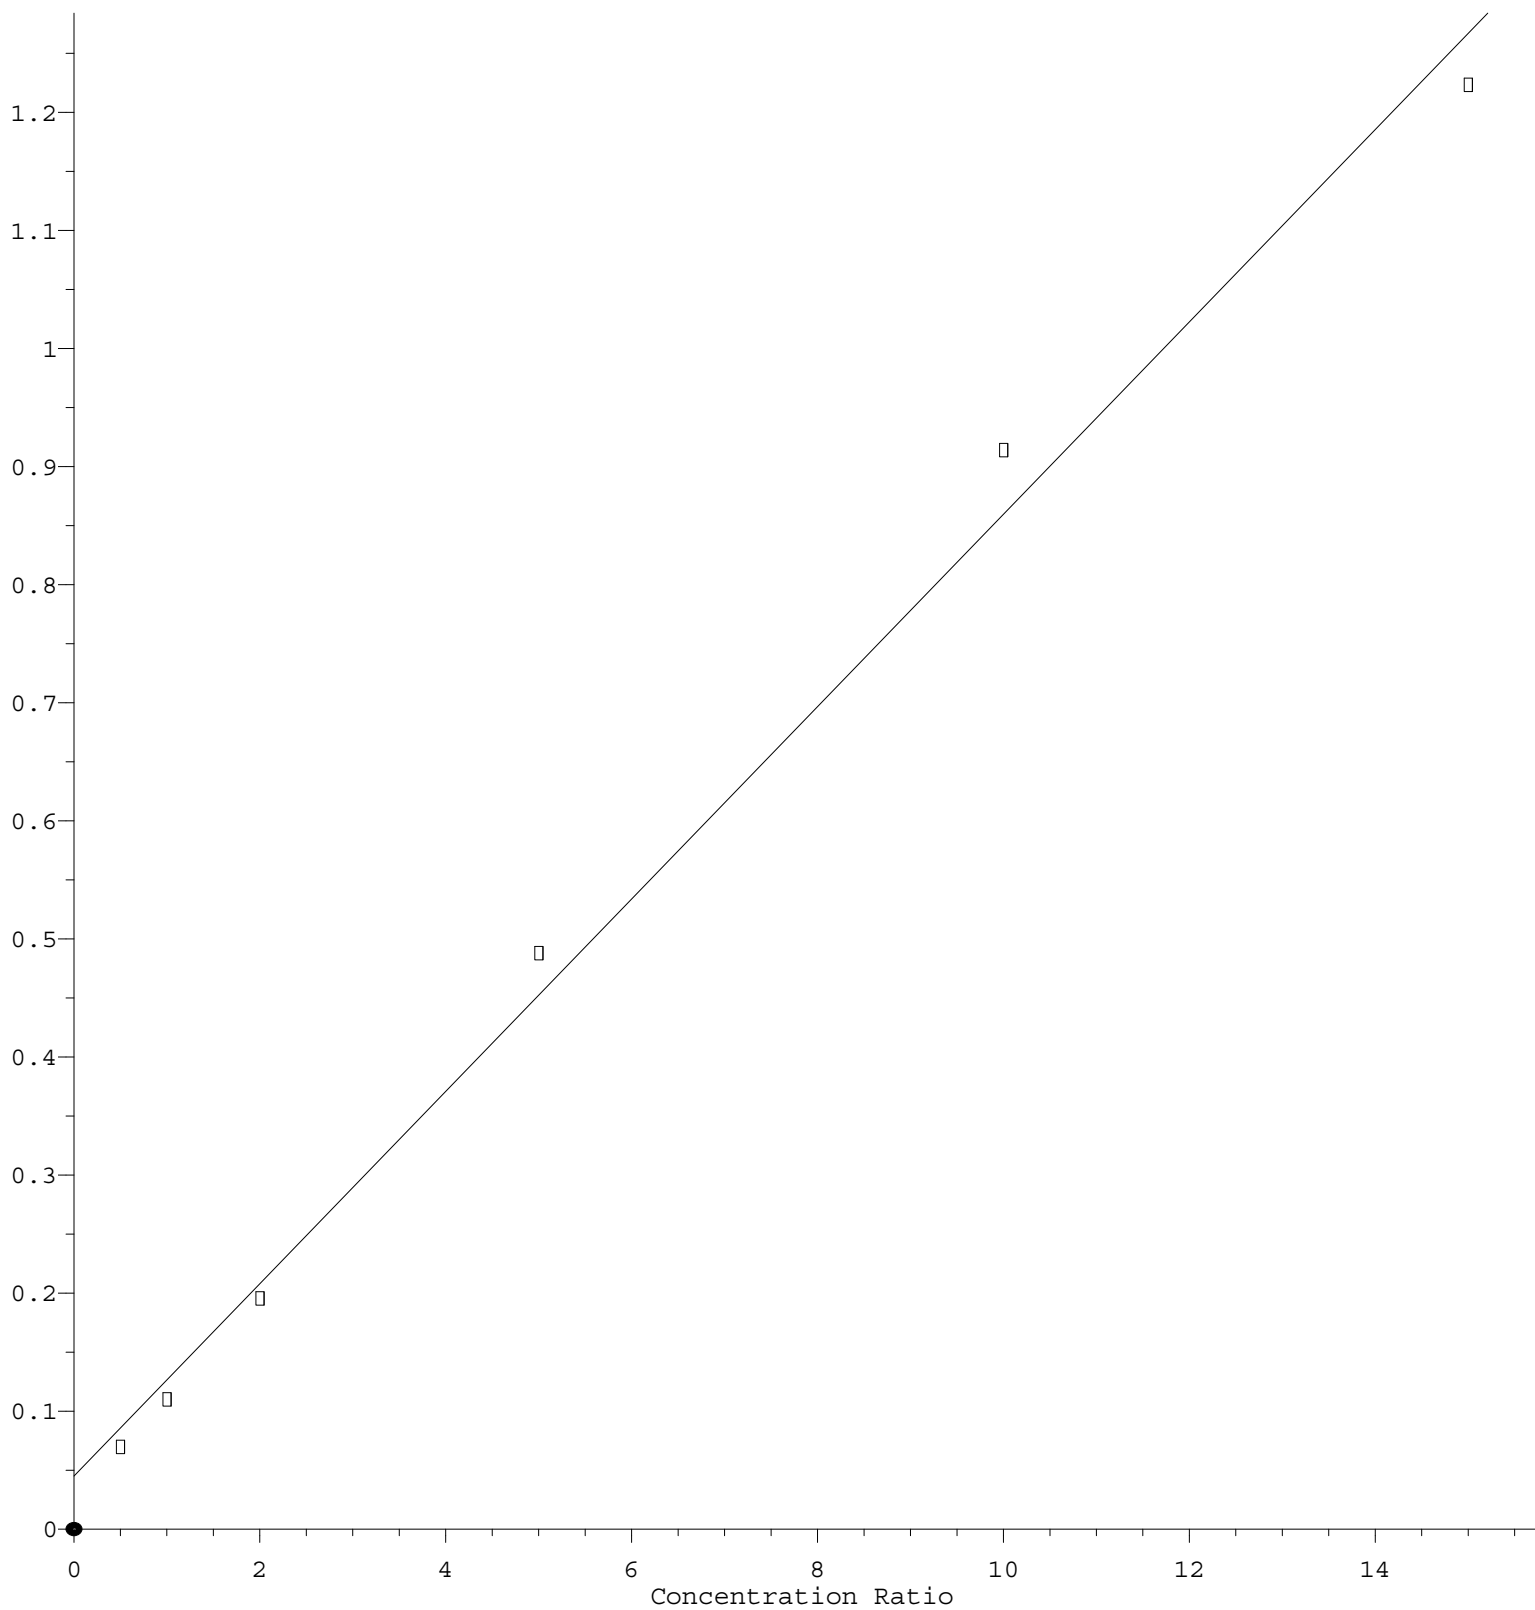

$$\text{Response} = 8.153\text{e-}002 * \text{Amt} + 4.481\text{e-}002$$


Coef of Det (r^2) = 0.993948 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D050421S.M

Calibration Table Last Updated: Wed May 05 04:16:41 2021

Methylene Chloride

Response Ratio

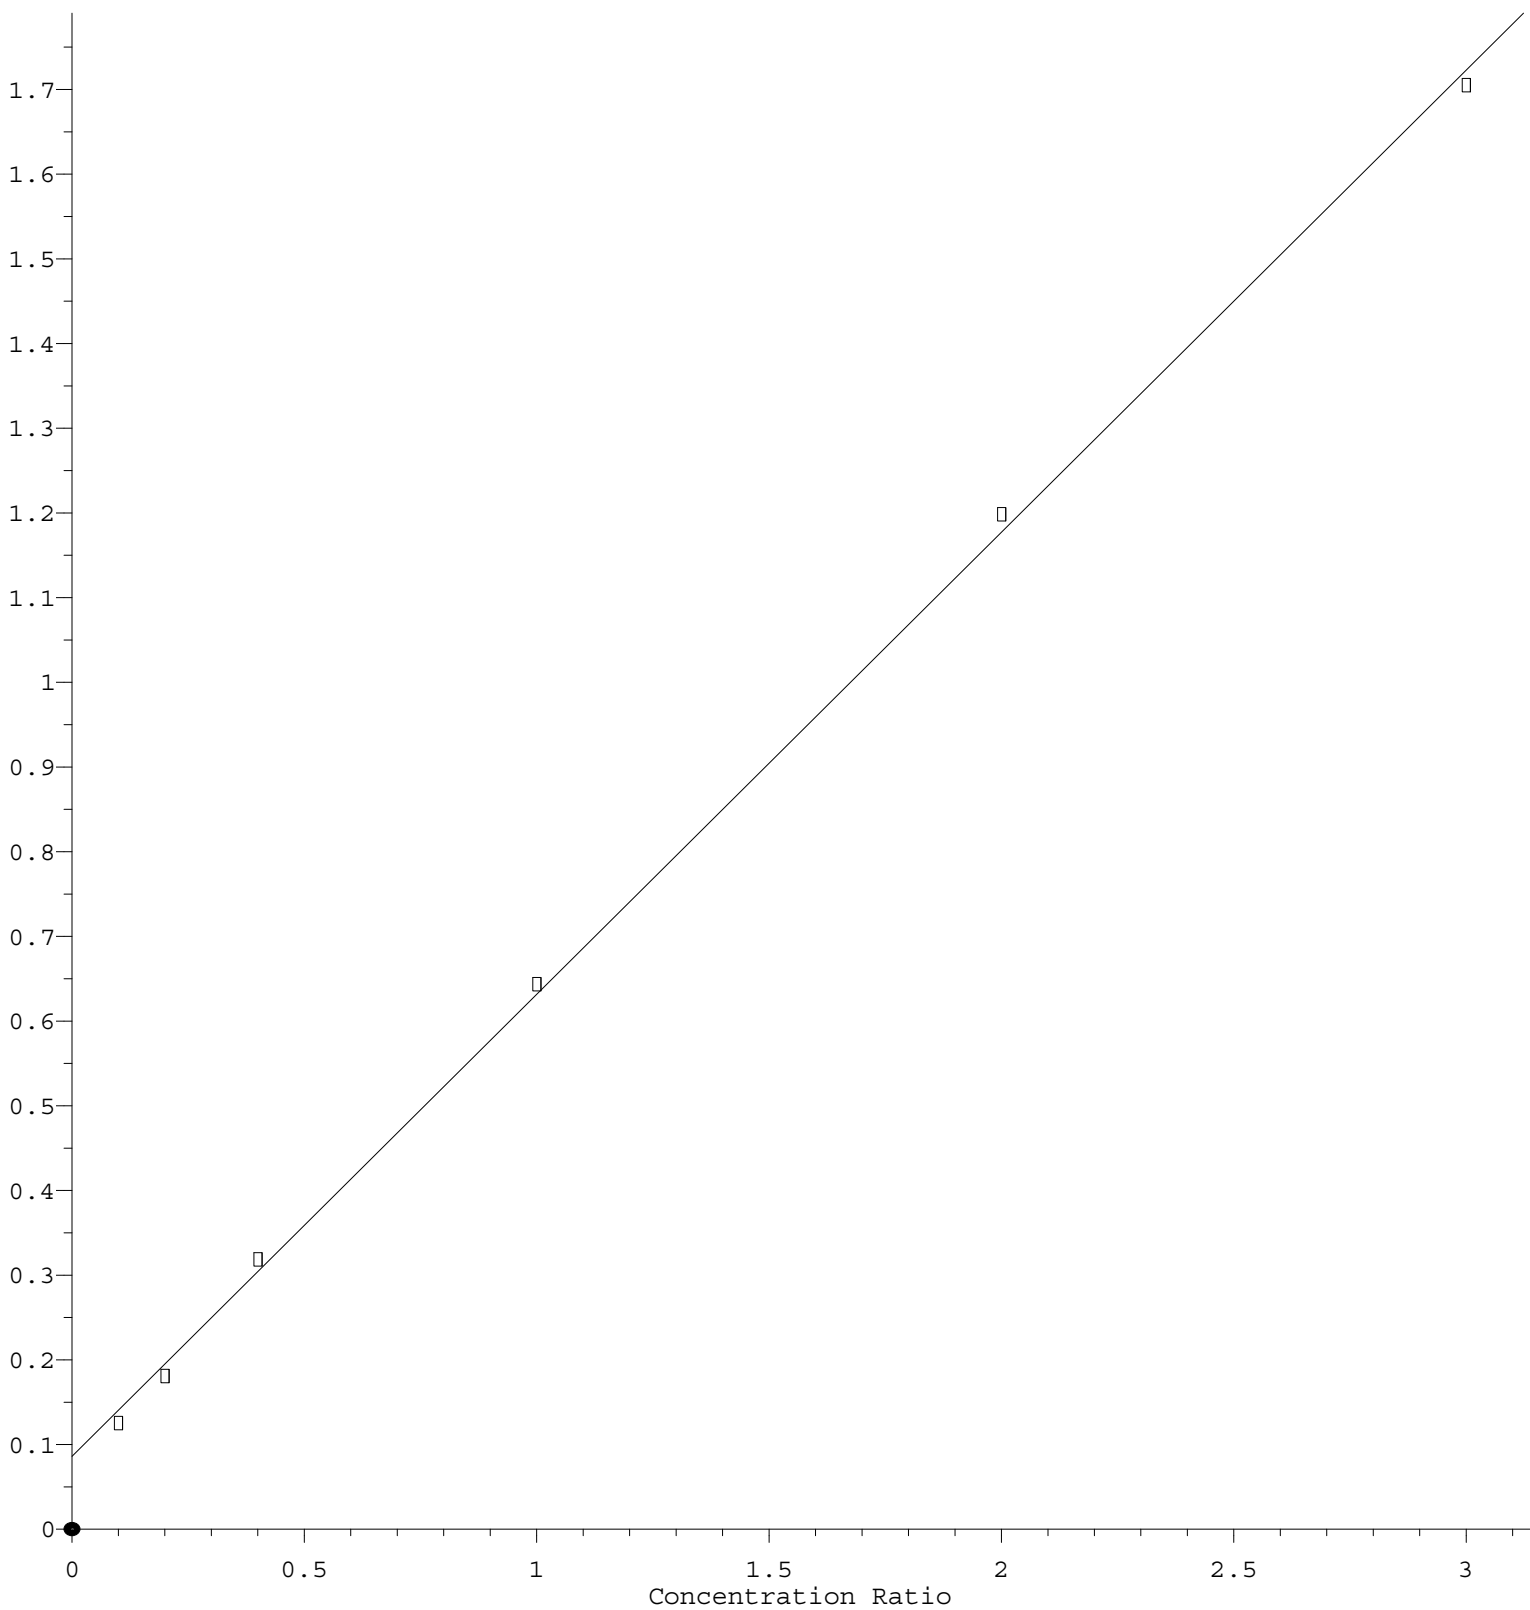

$$\text{Response} = 5.459\text{e-}001 * \text{Amt} + 8.559\text{e-}002$$

Coef of Det (r^2) = 0.999231 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D050421S.M

Calibration Table Last Updated: Wed May 05 04:16:41 2021