


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050421\
Data File : VD069055.D
Acq On : 04 May 2021 08:22
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050421S.M
Title : SW846 8260
Last Update : Wed May 05 04:16:41 2021

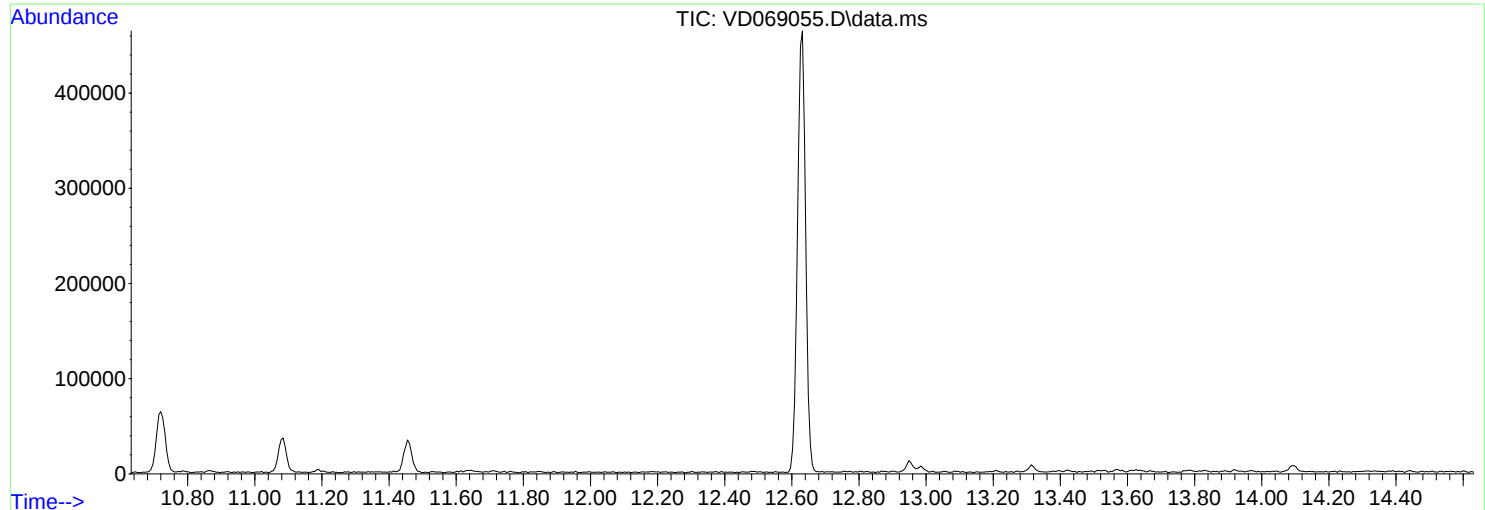

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	14867	PASS
75	95	30	60	54.4	41152	PASS
95	95	100	100	100.0	75680	PASS
96	95	5	9	6.0	4545	PASS
173	174	0.00	2	1.5	868	PASS
174	95	50	100	78.6	59501	PASS
175	174	5	9	7.9	4715	PASS
176	174	95	101	96.9	57659	PASS
177	176	5	9	7.3	4188	PASS