
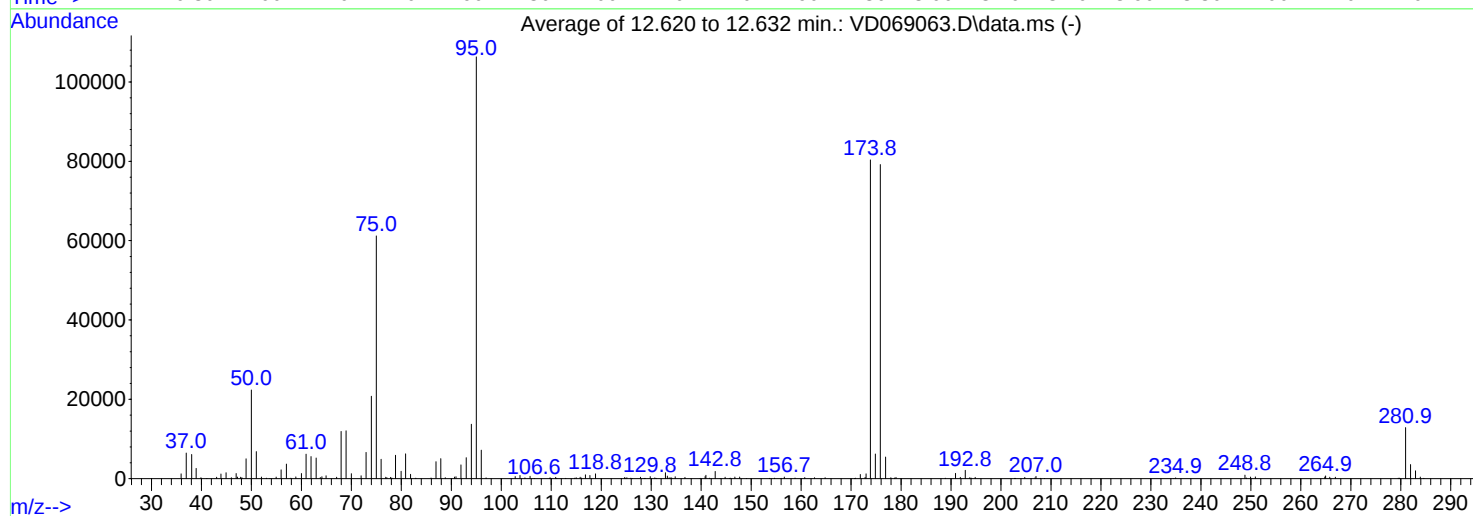


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD050521\  
Data File : VD069063.D  
Acq On : 05 May 2021 09:42  
Operator : VA/SY  
Sample : BFB  
Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D050421S.M  
Title : SW846 8260  
Last Update : Wed May 05 04:16:41 2021

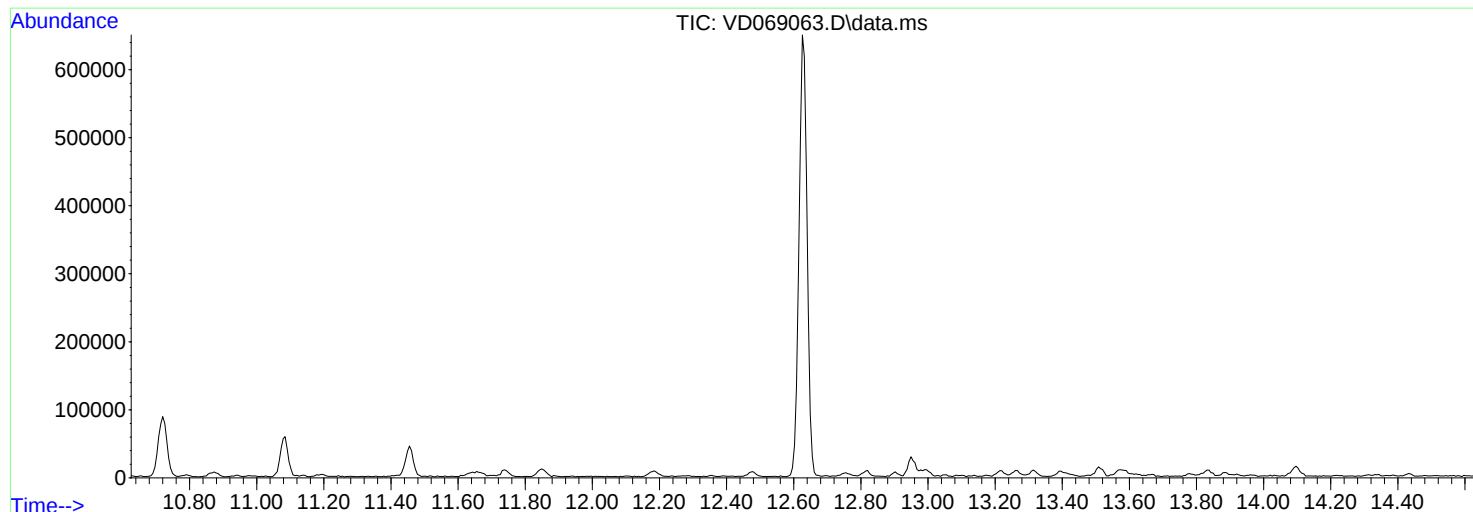

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 50     | 95      | 15     | 40     | 21.0  | 22333  | PASS      |
| 75     | 95      | 30     | 60     | 57.5  | 61171  | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 106325 | PASS      |
| 96     | 95      | 5      | 9      | 6.8   | 7190   | PASS      |
| 173    | 174     | 0.00   | 2      | 1.5   | 1203   | PASS      |
| 174    | 95      | 50     | 100    | 75.6  | 80333  | PASS      |
| 175    | 174     | 5      | 9      | 7.7   | 6201   | PASS      |
| 176    | 174     | 95     | 101    | 98.6  | 79189  | PASS      |
| 177    | 176     | 5      | 9      | 6.9   | 5464   | PASS      |