


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050523\
Data File : VD076015.D
Acq On : 05 May 2023 09:29
Operator : KP/SY
Sample : BFB127
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB127

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Title : SFAM01.0
Last Update : Sat May 06 00:21:26 2023

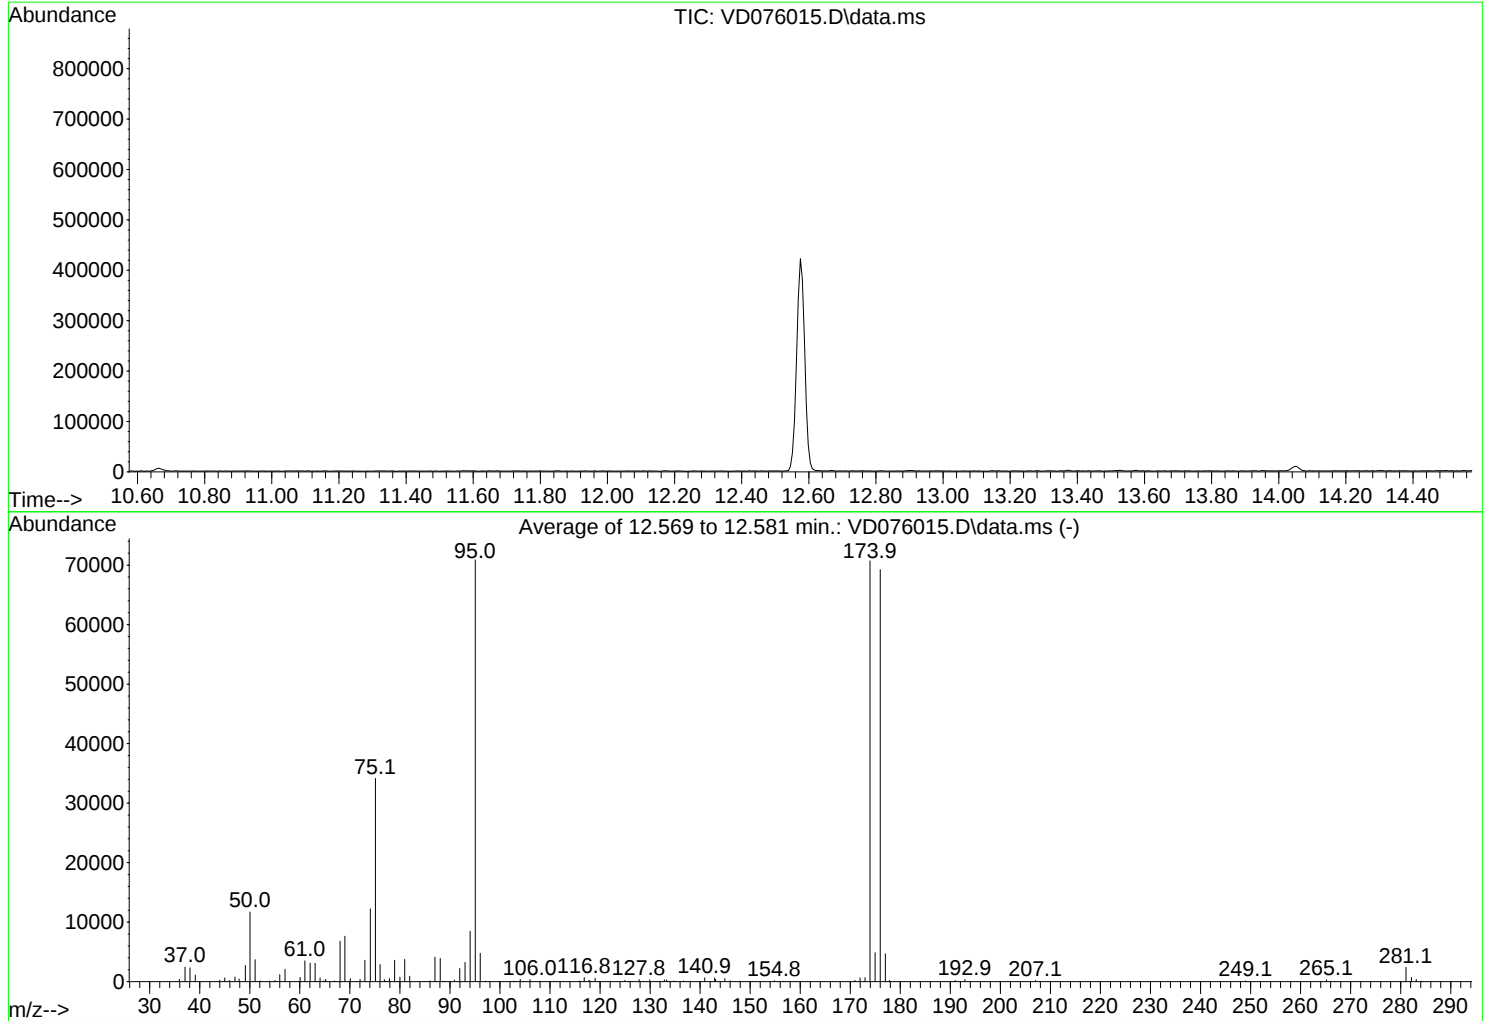

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.5	11706	PASS
75	95	30	80	48.2	34149	PASS
95	95	100	100	100.0	70885	PASS
96	95	5	9	6.7	4765	PASS
173	174	0.00	2	1.0	682	PASS
174	95	50	120	99.8	70725	PASS
175	174	5	9	6.9	4870	PASS
176	174	95	105	97.9	69248	PASS
177	176	5	10	6.8	4689	PASS

Scan 1860 (12.528 min): VD076015.D\data.ms
BFB127

m/z	Abundance
40.00	1191.0
44.00	802.0

Instrument :
MSVOA_D
ClientSampleId :
BFB127

m/z	Abundance
35.90	566.0
37.00	2255.0
38.10	2147.0
39.30	851.0
39.90	1143.0
44.00	1122.0
44.90	511.0
47.10	869.0
47.90	480.0
49.10	2499.0
50.10	11502.0
51.10	3524.0
54.90	229.0
56.00	1138.0
57.10	1954.0
60.10	633.0
61.00	3051.0
62.10	2907.0
63.10	3025.0
64.00	679.0
65.10	427.0
66.90	165.0
68.10	6378.0
69.00	6747.0
70.00	457.0
72.20	324.0
73.00	3060.0
74.10	11590.0
75.10	31584.0
76.10	2919.0
76.90	444.0
77.90	436.0
78.90	3112.0
80.00	716.0
81.00	3540.0
82.00	888.0
86.10	236.0
87.00	3361.0
88.10	3523.0
90.90	262.0
91.90	1688.0
93.00	2865.0
94.10	7433.0
95.10	65048.0
96.00	3846.0
102.70	190.0
104.10	339.0
106.00	312.0
110.80	174.0
116.90	591.0
117.80	349.0
119.00	623.0
125.00	214.0
125.80	233.0
127.90	342.0
129.80	207.0
133.20	297.0
140.90	395.0
142.90	944.0
145.00	436.0
156.70	164.0
170.90	175.0
171.90	535.0
173.00	614.0
173.90	62680.0
174.90	4428.0
176.00	61608.0
177.00	3892.0
177.80	289.0
190.80	249.0
193.00	265.0
249.10	186.0
265.10	170.0
281.00	1565.0
282.20	378.0
283.00	343.0

Instrument :
MSVOA_D
ClientSampleId :
BFB127

m/z	Abundance
36.00	403.0
37.10	3023.0
38.00	2405.0
39.10	1492.0
40.00	1259.0
44.00	1091.0
45.00	871.0
45.90	389.0
47.00	864.0
47.90	446.0
49.10	2961.0
50.00	12580.0
51.10	3679.0
52.00	163.0
55.10	182.0
56.10	1328.0
57.10	2142.0
60.00	651.0
61.00	4005.0
62.00	3280.0
63.00	3151.0
64.10	616.0
64.80	418.0
65.20	398.0
67.00	151.0
68.00	7585.0
69.00	8533.0
70.10	492.0
72.00	554.0
73.00	3792.0
74.10	13360.0
75.10	37688.0
76.00	3012.0
76.90	550.0
78.00	479.0
79.00	4098.0
79.90	945.0
80.90	3519.0
81.90	1082.0
86.00	172.0
87.00	4601.0
88.00	4031.0
91.00	392.0
92.00	2888.0
93.00	3665.0
94.10	10029.0
95.00	77632.0
96.10	5967.0
97.10	227.0
102.90	184.0
104.10	463.0
104.70	181.0
106.10	434.0
107.90	179.0
115.90	308.0
116.80	786.0
117.80	401.0
119.00	533.0
124.90	223.0
127.80	301.0
129.90	271.0
132.80	295.0
133.30	229.0
133.80	173.0
134.80	314.0
140.90	902.0
143.10	1161.0
144.90	551.0
146.00	225.0
154.90	297.0
171.00	264.0
172.00	799.0
172.90	813.0
174.00	75880.0
175.00	5606.0
176.00	76984.0
177.00	5154.0
177.80	194.0
191.00	301.0
192.90	483.0
207.00	252.0
249.00	223.0
265.20	398.0
266.90	162.0
281.10	2484.0
282.10	877.0
283.10	420.0

Instrument :
MSVOA_D
ClientSampleId :
BFB127

m/z	Abundance
35.80	245.0
37.10	2106.0
38.10	2426.0
39.00	975.0
39.90	1036.0
44.00	905.0
45.10	494.0
45.90	155.0
47.10	597.0
47.80	465.0
49.10	2663.0
50.10	11036.0
51.00	3892.0
52.10	257.0
53.90	231.0
55.00	278.0
55.90	1101.0
57.00	2124.0
60.00	869.0
61.00	3457.0
62.00	3086.0
63.00	3070.0
64.00	586.0
65.10	313.0
68.00	6440.0
69.00	7631.0
70.20	584.0
72.00	285.0
73.00	3889.0
74.10	11773.0
75.10	33176.0
76.00	2673.0
77.20	284.0
77.80	667.0
78.90	3582.0
80.10	634.0
80.90	4173.0
82.00	755.0
87.00	4354.0
88.00	4172.0
88.80	161.0
90.80	194.0
92.00	2050.0
93.00	3171.0
94.00	7927.0
95.10	69976.0
96.00	4482.0
103.90	312.0
105.90	294.0
116.80	762.0
118.00	332.0
119.00	534.0
125.00	240.0
127.70	430.0
130.00	422.0
132.90	574.0
133.40	365.0
136.70	322.0
140.90	674.0
142.90	921.0
144.90	659.0
146.00	228.0
147.90	208.0
154.80	172.0
171.00	200.0
171.90	618.0
172.90	618.0
174.00	73616.0
175.00	4576.0
176.00	69152.0
177.00	5020.0
177.90	181.0
191.10	203.0
192.80	389.0
207.10	368.0
265.10	348.0
266.00	179.0
281.10	3132.0
282.20	867.0
283.20	343.0
284.20	265.0

Instrument :
MSVOA_D
ClientSampleId :
BFB127