


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD050619\
Data File : VD062123.D
Acq On : 6 May 2019 9:44
Operator : FY/SY
Sample : BFB
Misc : 5.00µ/5mL/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D042319S.M
Title : SW846 8260
Last Update : Thu May 02 07:55:52 2019

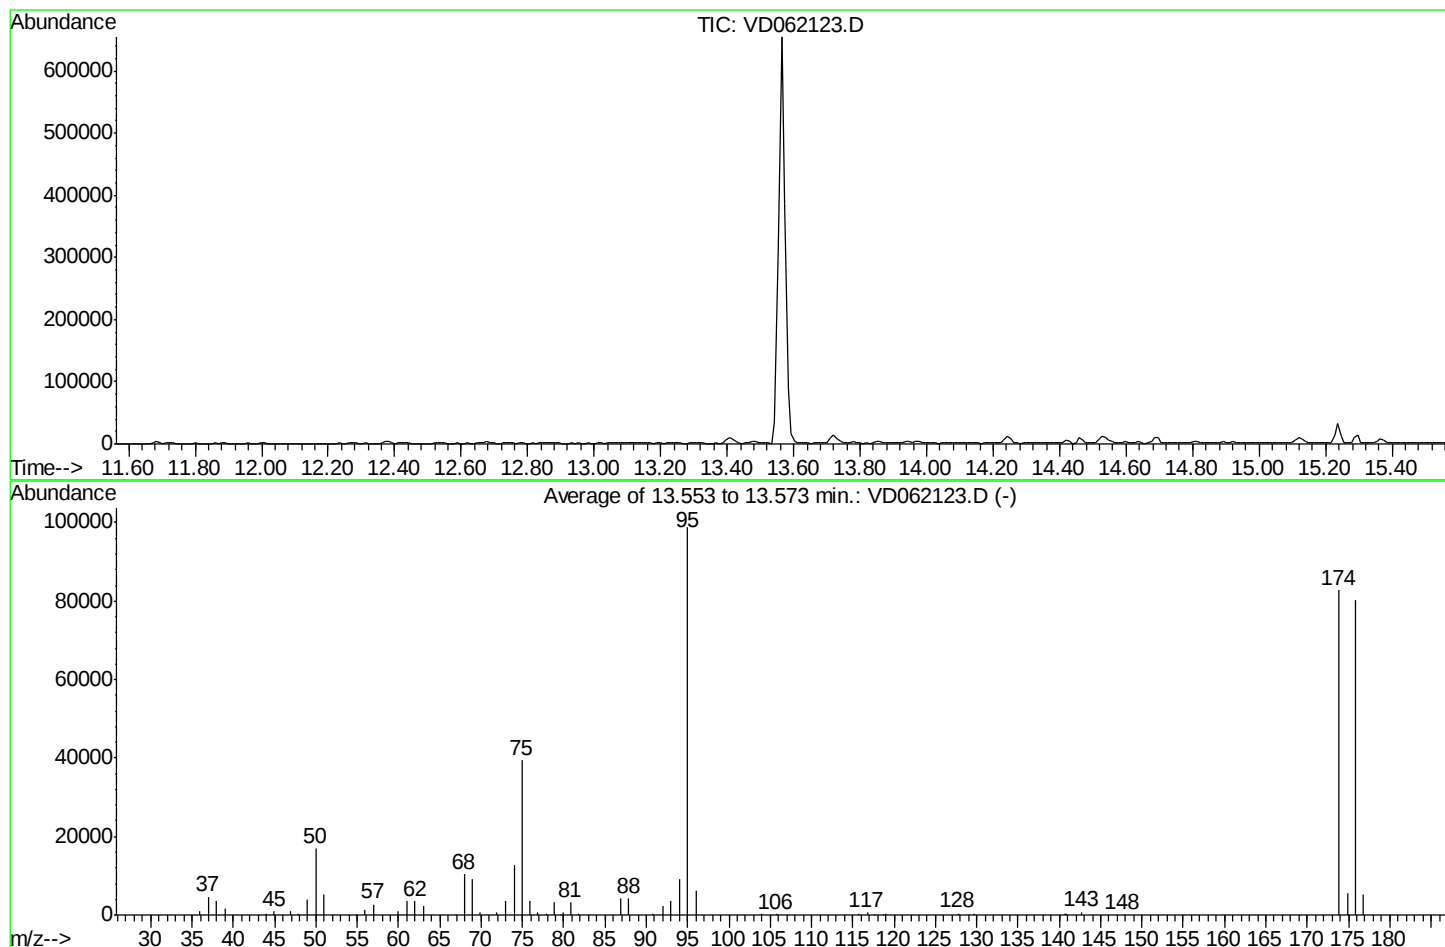

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	16905	PASS
75	95	30	60	39.9	39381	PASS
95	95	100	100	100.0	98786	PASS
96	95	5	9	6.2	6112	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.8	82765	PASS
175	174	5	9	6.7	5514	PASS
176	174	95	101	96.9	80181	PASS
177	176	5	9	6.5	5193	PASS