
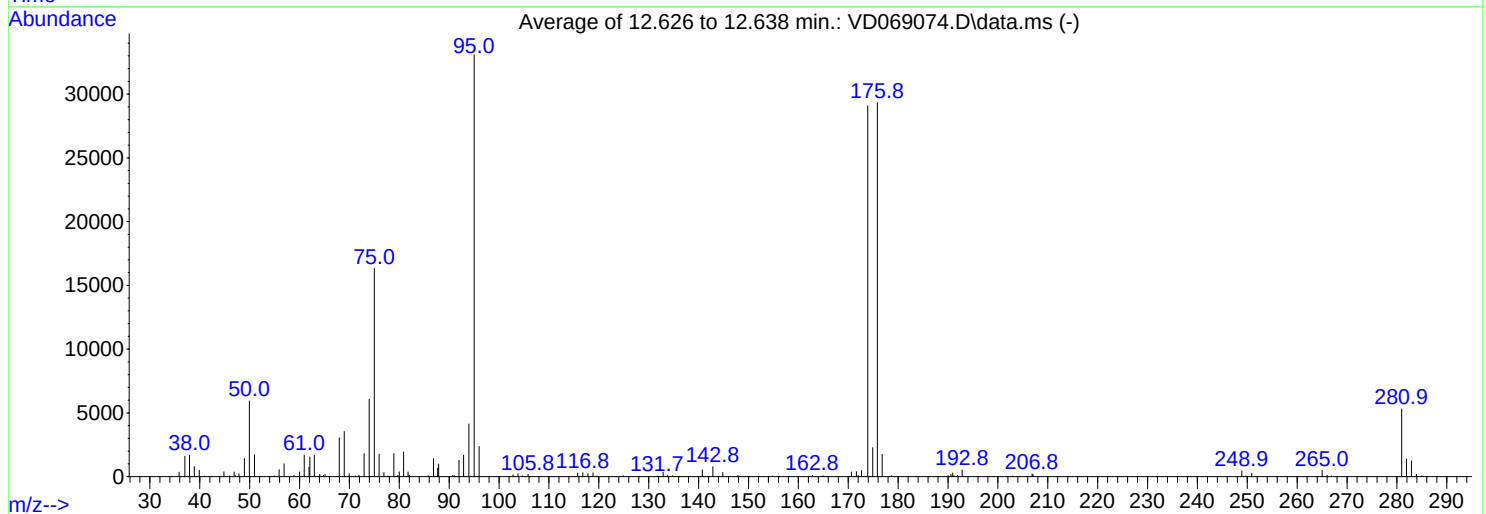


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050621\
Data File : VD069074.D
Acq On : 06 May 2021 12:42
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050421S.M
Title : SW846 8260
Last Update : Wed May 05 04:16:41 2021

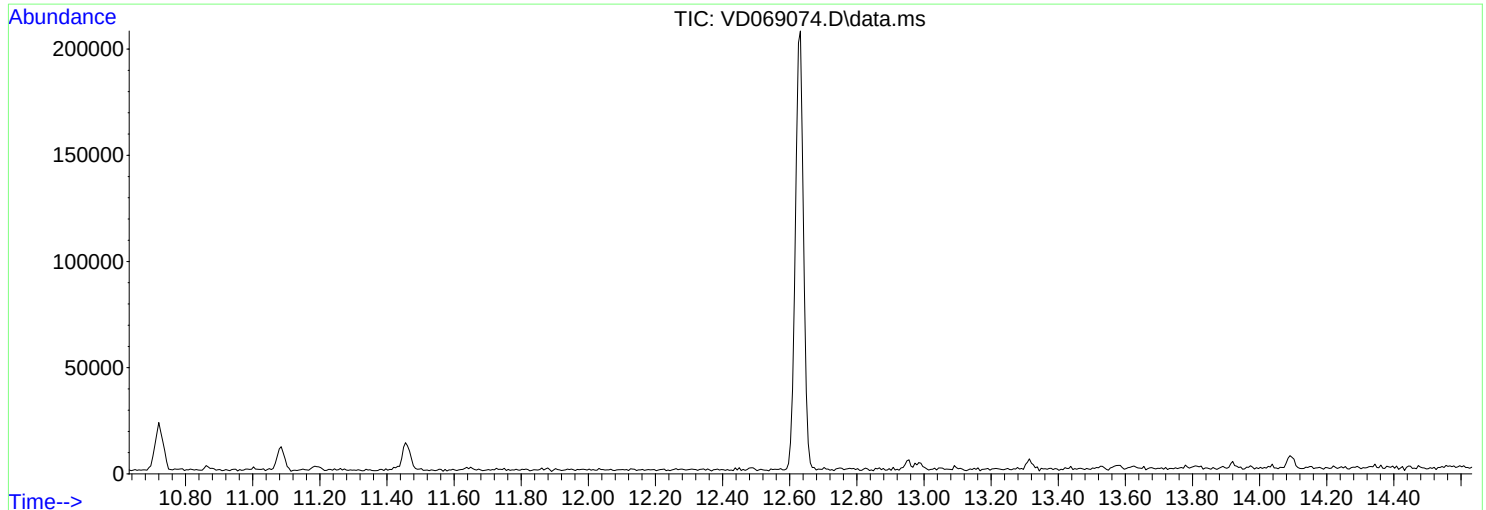

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.0	5938	PASS
75	95	30	60	49.3	16324	PASS
95	95	100	100	100.0	33080	PASS
96	95	5	9	7.1	2363	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.9	29083	PASS
175	174	5	9	7.8	2273	PASS
176	174	95	101	100.8	29323	PASS
177	176	5	9	6.0	1746	PASS