

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD050719\
 Data File : VD062153.D
 Acq On : 8 May 2019 1:55
 Operator : FY/SY
 Sample : K2673-11
 Misc : 5.02g/5mL/MSVOA D/SOIL
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-16-2.0-2.5

Quant Time: May 08 04:34:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D050719S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 07 14:26:29 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.02	168	570483	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.20	114	865975	50.00	ug/l	0.01
63) Chlorobenzene-d5	12.36	117	534303	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	14.51	152	120532	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.44	65	274565	51.79	ug/l	0.01
Spiked Amount 50.000			Recovery	=	103.58%	
35) Dibromofluoromethane	6.90	113	351316	48.90	ug/l	0.01
Spiked Amount 50.000			Recovery	=	97.80%	
50) Toluene-d8	10.39	98	617050	35.62	ug/l	0.00
Spiked Amount 50.000			Recovery	=	71.24%	
62) 4-Bromofluorobenzene	13.55	95	161815	23.26	ug/l	0.00
Spiked Amount 50.000			Recovery	=	46.52%	
Target Compounds						
					Qvalue	
5) Bromomethane	2.16	94	1125	1.239	ug/l #	12
16) Acetone	3.20	43	9792	8.807	ug/l #	86
20) Methylene Chloride	3.80	84	12054	2.597	ug/l #	94
31) Cyclohexane	7.02	56	10962	1.971	ug/l #	14
36) 1,1-Dichloropropene	7.02	75	40568	5.714	ug/l #	46
38) Carbon Tetrachloride	7.02	117	54984	5.595	ug/l #	12
81) trans-1,4-Dichloro-2-buten	13.55	75	65612	162.253	ug/l #	16
95) Naphthalene	16.11	128	23811	7.701	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD050719\
Data File : VD062153.D
Acq On : 8 May 2019 1:55
Operator : FY/SY
Sample : K2673-11
Misc : 5.02g/5mL/MSVOA D/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-16-2.0-2.5

Quant Time: May 08 04:34:10 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D050719S.M
Quant Title : SW846 8260
QLast Update : Tue May 07 14:26:29 2019
Response via : Initial Calibration

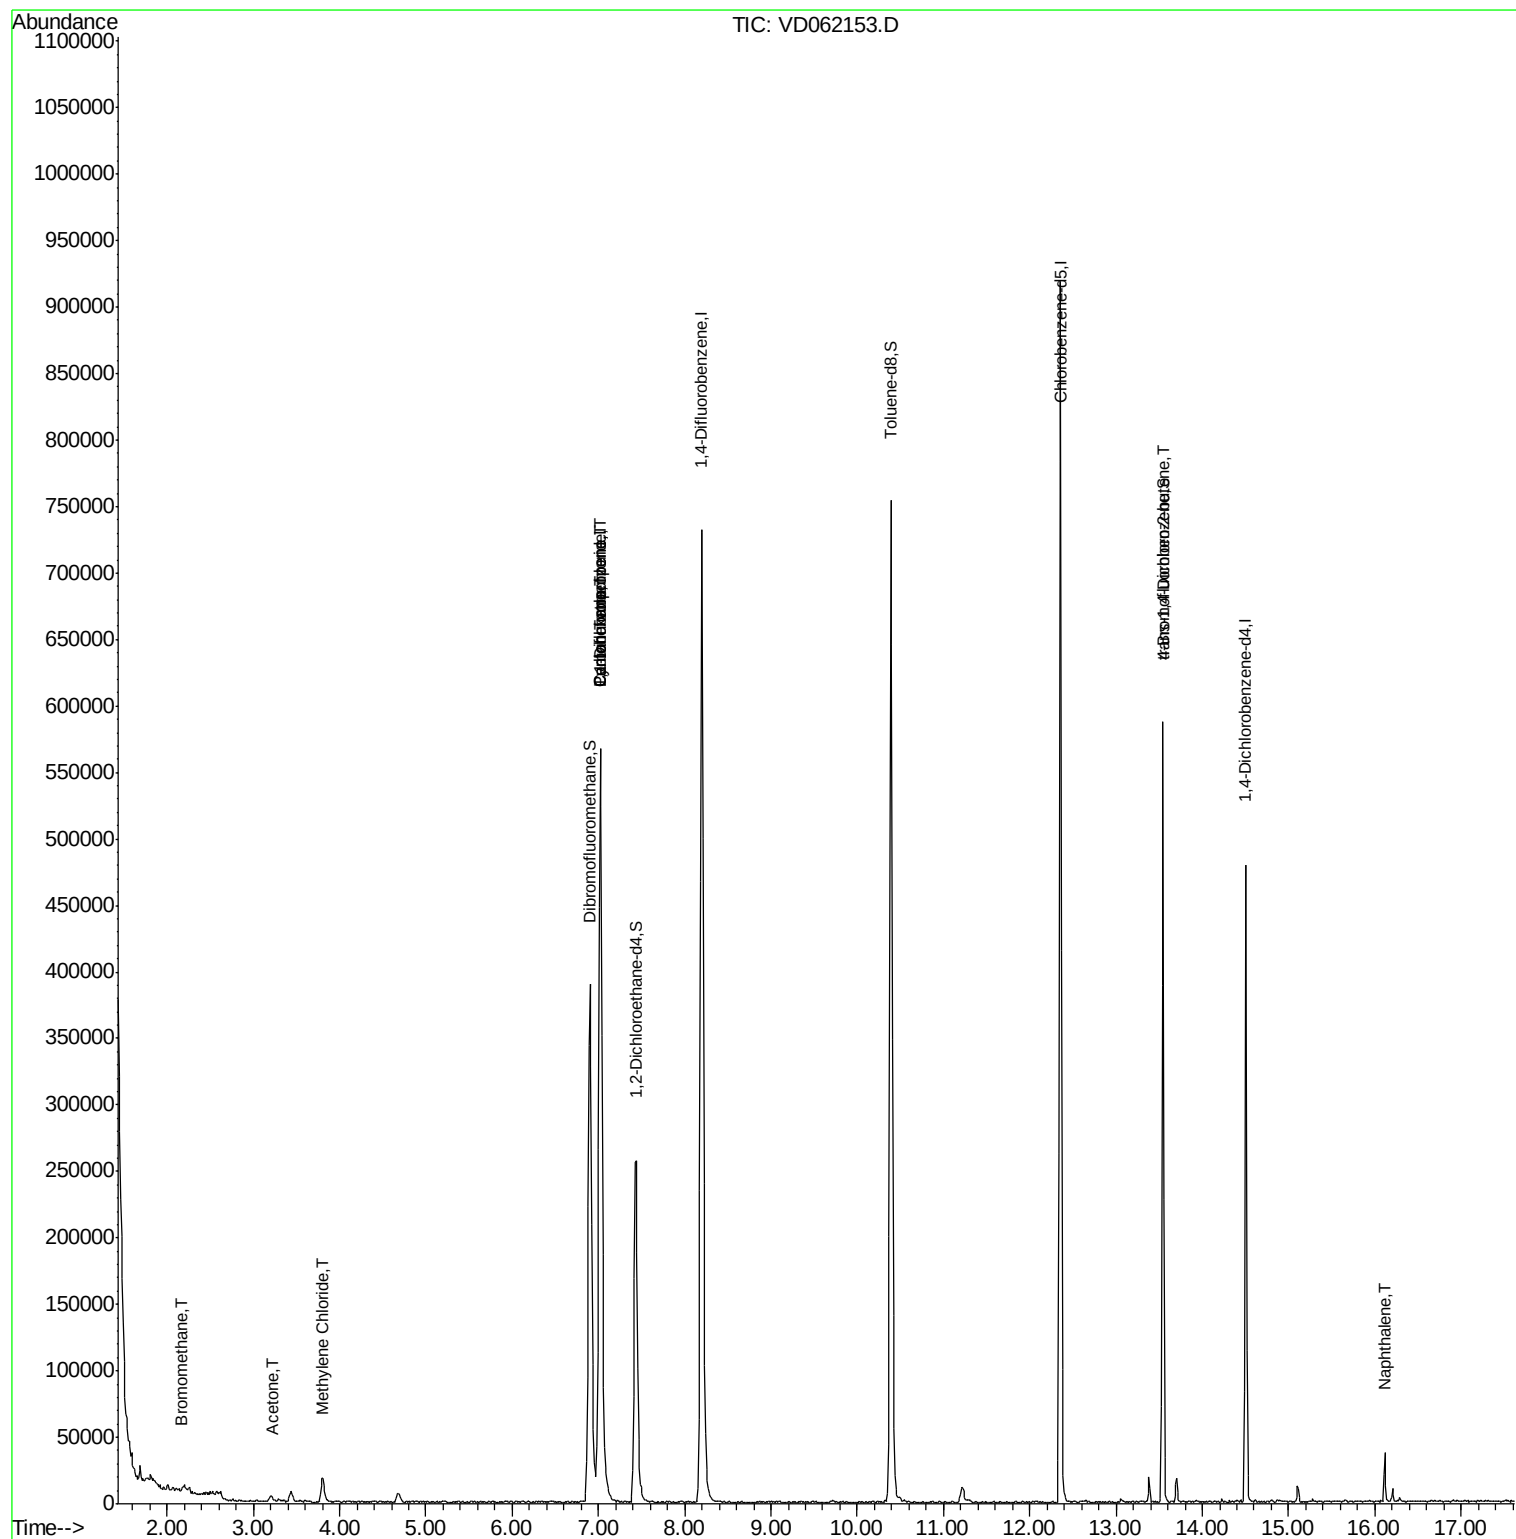

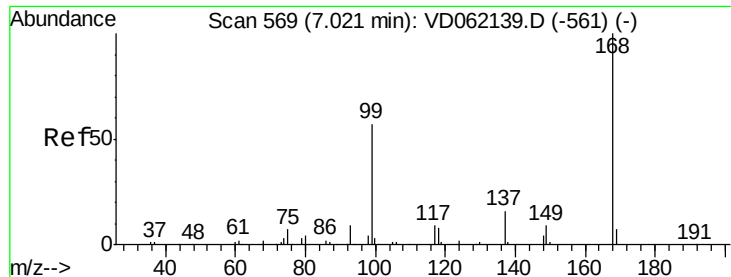

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.02 min Scan# 569

Delta R.T. 0.00 min

Lab File: VD062153.D

Acq: 8 May 2019 1:55

Instrument :

MSVOA_D

ClientSampleId :


SB-16-2.0-2.5

Tot Ion:168 Resp: 570483

Ion Ratio Lower Upper




168 100

99 60.2 46.5 69.7

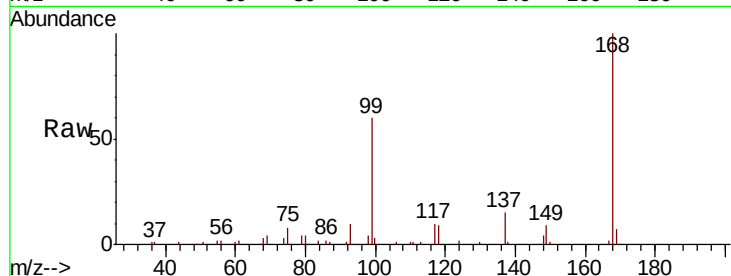

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

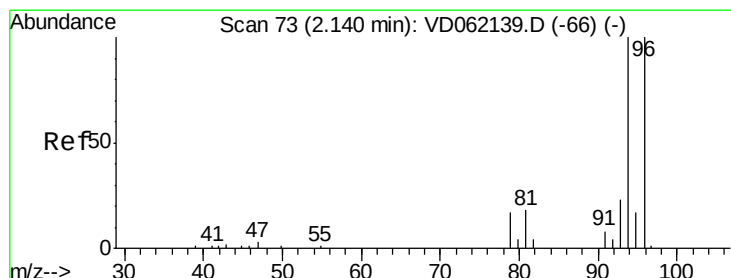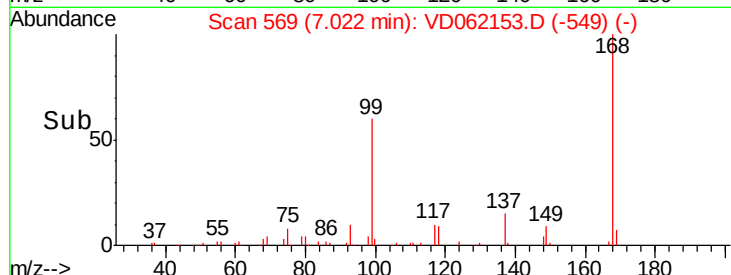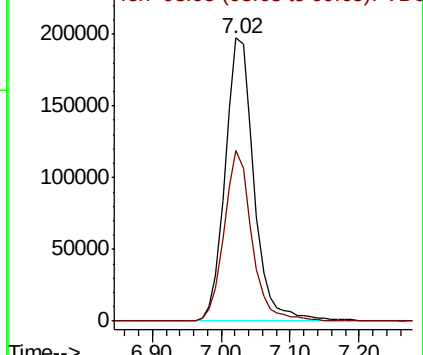

#5

Bromomethane

Concen: 1.239 ug/l

RT: 2.16 min Scan# 75

Delta R.T. 0.02 min

Lab File: VD062153.D

Acq: 8 May 2019 1:55


Tgt Ion: 94 Resp: 1125

Ion Ratio Lower Upper

94 100

96 0.0 76.6 115.0#



93 0.0 18.5 27.7#

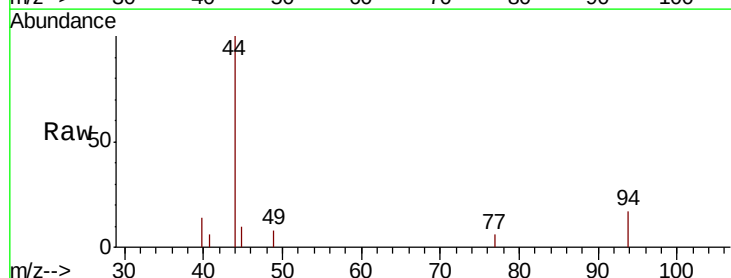


Abundance Ion 94.00 (93.70 to 94.70): VDC

Ion 96.00 (95.70 to 96.70): VDC

Ion 93.00 (92.70 to 93.70): VDC



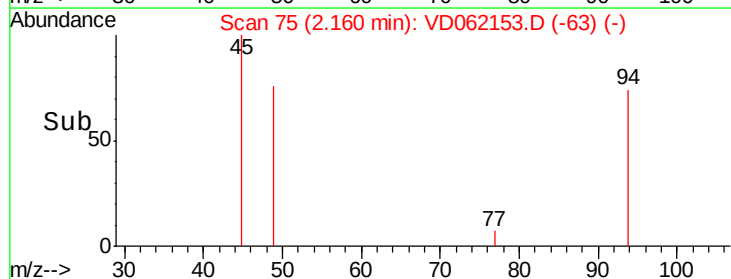
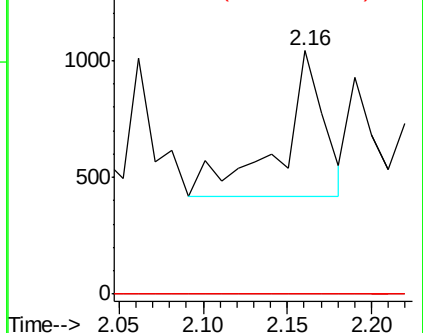


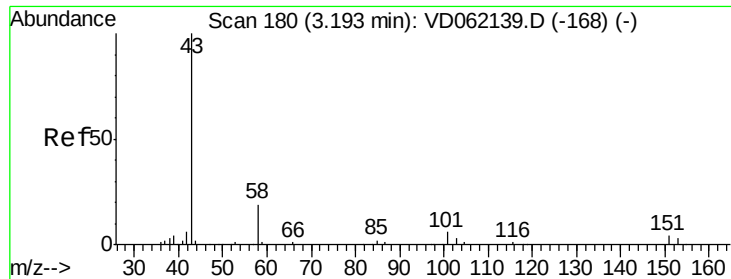

#16
Acetone
Concen: 8.807 ug/l
RT: 3.20 min Scan# 181
Delta R.T. 0.01 min
Lab File: VD062153.D
Acq: 8 May 2019 1:55




Instrument :
MSVOA_D
ClientSampleId :
SB-16-2.0-2.5


Tot Ion: 43 Resp: 9792
Ion Ratio Lower Upper
43 100
58 18.0 19.9 29.9#

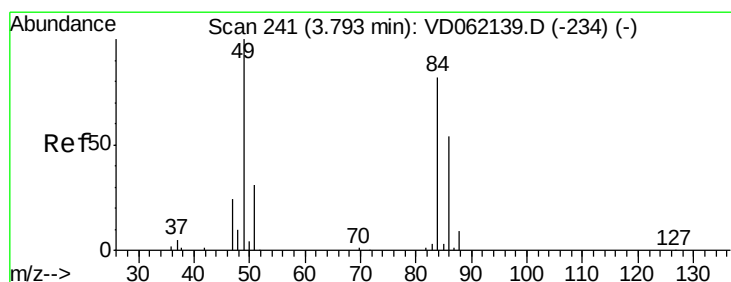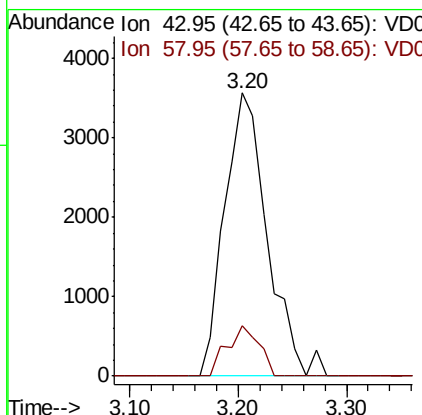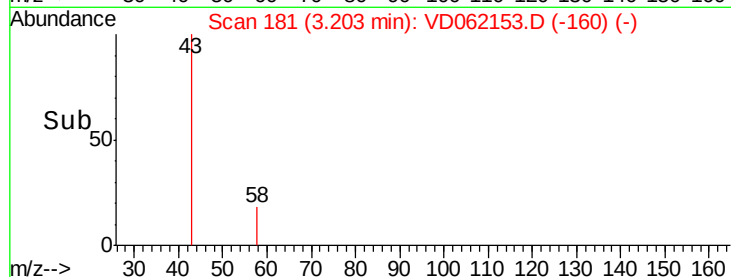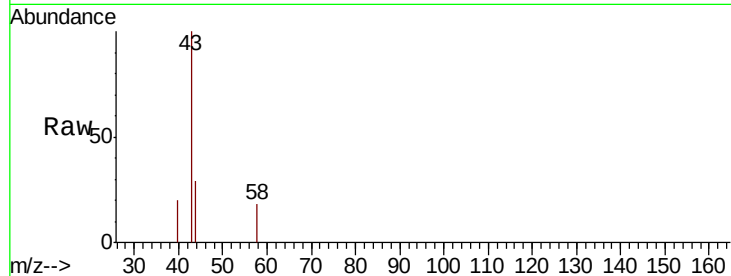

#20
Methylene Chloride
Concen: 2.597 ug/l
RT: 3.80 min Scan# 242
Delta R.T. 0.01 min
Lab File: VD062153.D
Acq: 8 May 2019 1:55

Tgt Ion: 84 Resp: 12054
Ion Ratio Lower Upper
84 100
49 121.8 94.0 141.0
51 43.9 29.0 43.4#
86 67.1 49.8 74.6


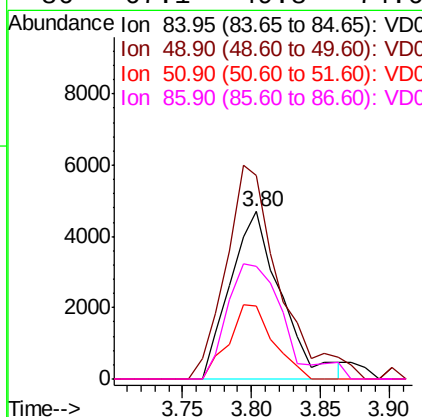
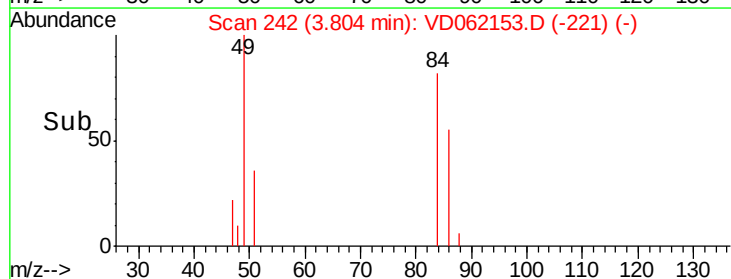
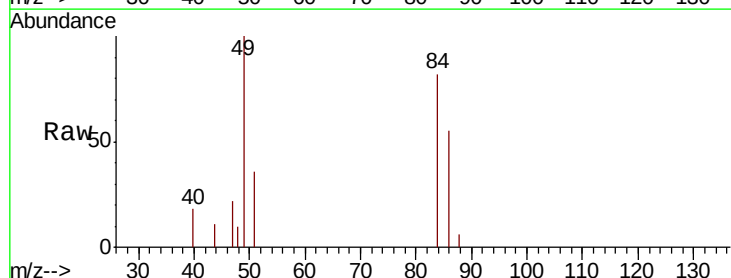




#31
Cyclohexane
Concen: 1.971 ug/l
RT: 7.02 min Scan# 569
Delta R.T. 0.09 min
Lab File: VD062153.D
Acq: 8 May 2019 1:55




Instrument :
MSVOA_D
ClientSampleId :
SB-16-2.0-2.5


Tot Ion: 56 Resp: 10962
Ion Ratio Lower Upper
56 100
69 204.0 25.8 38.6#
84 96.9 72.2 108.4

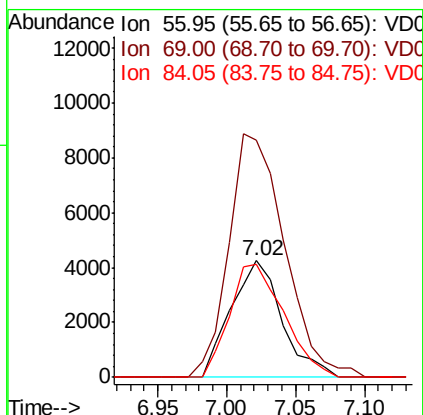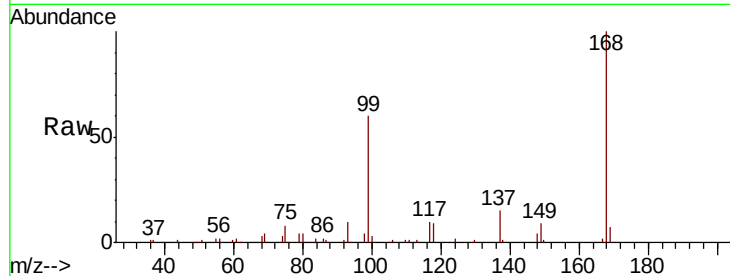

#33
1,2-Dichloroethane-d4
Concen: 51.789 ug/l
RT: 7.44 min Scan# 611
Delta R.T. 0.01 min
Lab File: VD062153.D
Acq: 8 May 2019 1:55

Tgt Ion: 65 Resp: 274565
Ion Ratio Lower Upper
65 100
67 49.3 0.0 98.0

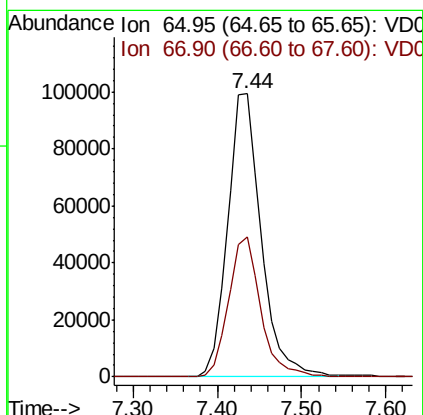


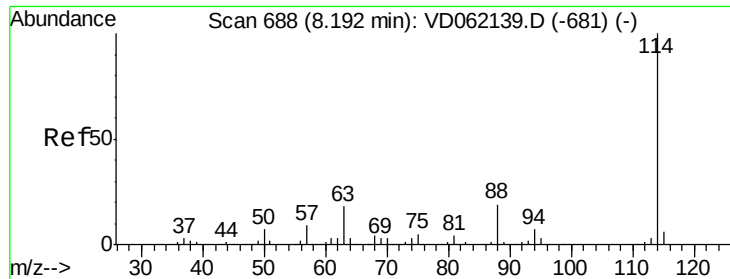




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.20 min Scan# 689
 Delta R.T. 0.01 min
 Lab File: VD062153.D
 Acq: 8 May 2019 1:55

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-16-2.0-2.5

Tot Ion:114 Resp: 865975
 Ion Ratio Lower Upper
 114 100
 63 16.7 0.0 32.4
 88 16.9 0.0 33.6

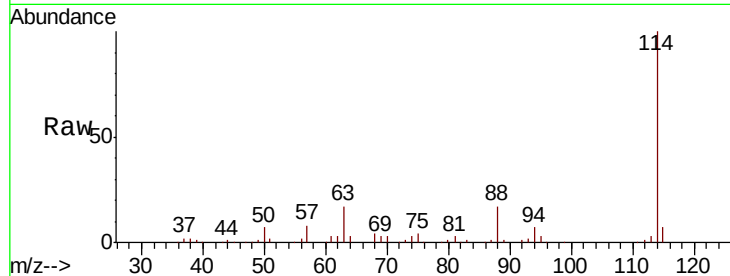


Abundance Ion 114.00 (113.70 to 114.70): V
 Ion 62.95 (62.65 to 63.65): V
 Ion 87.90 (87.60 to 88.60): V


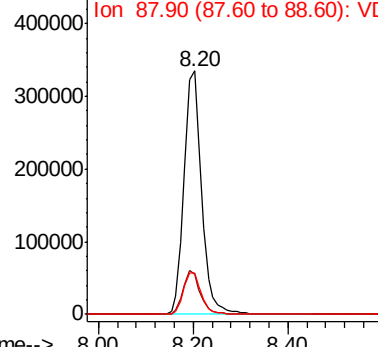



#35
 Dibromofluoromethane
 Concen: 48.895 ug/l
 RT: 6.90 min Scan# 557
 Delta R.T. 0.01 min
 Lab File: VD062153.D
 Acq: 8 May 2019 1:55

Tgt Ion:113 Resp: 351316
 Ion Ratio Lower Upper
 113 100
 111 103.5 78.5 117.7
 192 18.7 13.0 19.4



Abundance Ion 112.90 (112.60 to 113.60): V
 Ion 110.90 (110.60 to 111.60): V
 Ion 191.80 (191.50 to 192.50): V




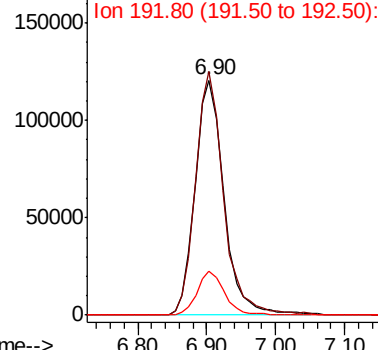


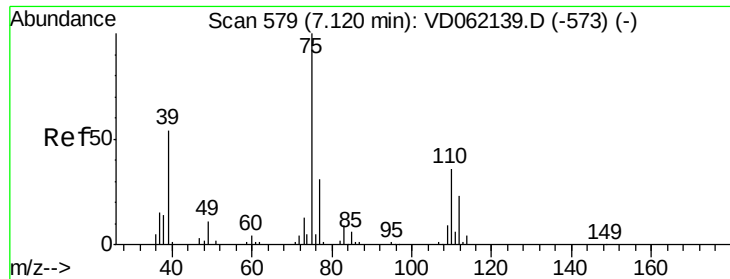

#36
 1,1-Dichloropropene
 Concen: 5.714 ug/l
 RT: 7.02 min Scan# 569
 Delta R.T. -0.10 min
 Lab File: VD062153.D
 Acq: 8 May 2019 1:55




Instrument :
 MSVOA_D
 ClientSampleId :
 SB-16-2.0-2.5


Tot Ion	Ratio	Lower	Upper
75	100		
110	7.0	19.1	57.1#
77	0.0	25.6	38.4#

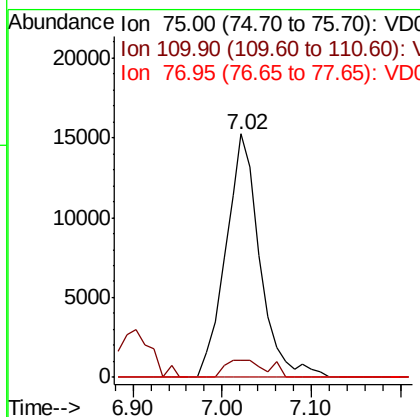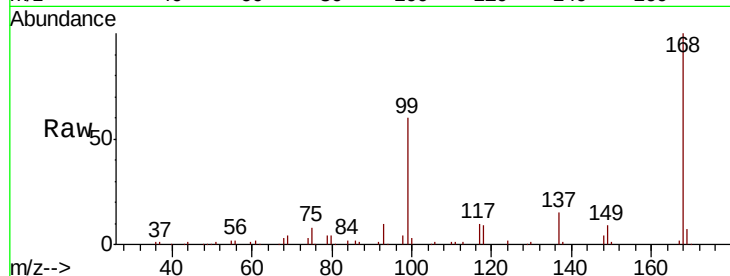

#38
 Carbon Tetrachloride
 Concen: 5.595 ug/l
 RT: 7.02 min Scan# 569
 Delta R.T. -0.07 min
 Lab File: VD062153.D
 Acq: 8 May 2019 1:55

Tgt Ion	Ratio	Lower	Upper
117	100		
119	0.0	75.8	113.8#
121	0.0	25.9	38.9#

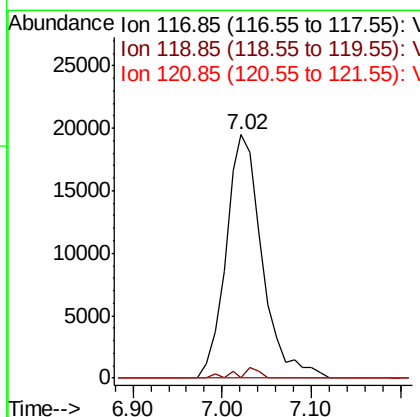

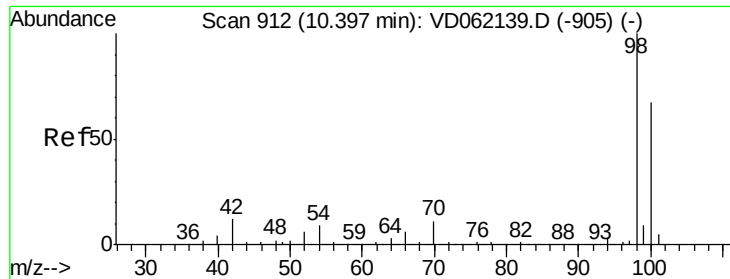

#50

Toluene-d8

Concen: 35.619 ug/l

RT: 10.39 min Scan# 911

Delta R.T. -0.01 min

Lab File: VD062153.D

Acq: 8 May 2019 1:55

Instrument :

MSVOA_D

ClientSampleId :


SB-16-2.0-2.5

Tot Ion: 98 Resp: 617050

Ion Ratio Lower Upper

98 100

100 66.7 53.8 80.8

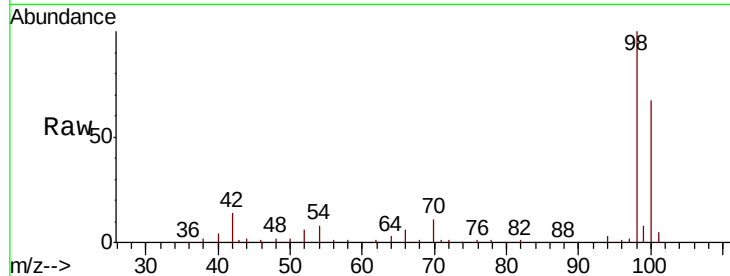

Abundance Ion 98.05 (97.75 to 98.75): VD062139.D (-905) (-)

Ion 100.05 (99.75 to 100.75): VD062139.D (-905) (-)

10.39



300000

200000

100000

0

Time-->



#62

4-Bromofluorobenzene

Concen: 23.261 ug/l

RT: 13.55 min Scan# 1232

Delta R.T. 0.00 min

Lab File: VD062153.D

Acq: 8 May 2019 1:55


Tgt Ion: 95 Resp: 161815

Ion Ratio Lower Upper

95 100

174 100.9 0.0 181.8

176 94.9 0.0 174.4



Abundance Ion 95.00 (94.70 to 95.70): VD062139.D (-1227) (-)

Ion 173.90 (173.60 to 174.60): VD062139.D (-1227) (-)

Ion 175.90 (175.60 to 176.60): VD062139.D (-1227) (-)


150000


100000

50000

0

Time-->




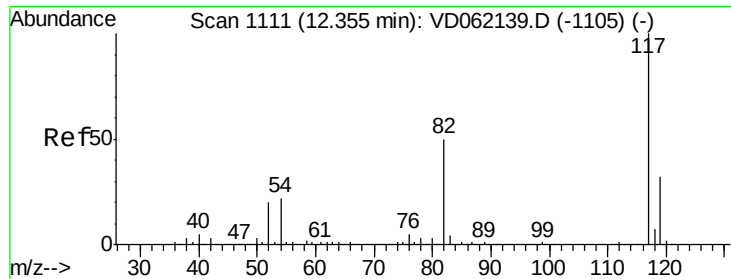




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 12.36 min Scan# 1111
Delta R.T. 0.00 min
Lab File: VD062153.D
Acq: 8 May 2019 1:55

Instrument :
MSVOA_D
ClientSampleId :
SB-16-2.0-2.5

Tot Ion:117 Resp: 534303
Ion Ratio Lower Upper
117 100
82 48.1 36.2 54.2
119 32.6 26.2 39.4

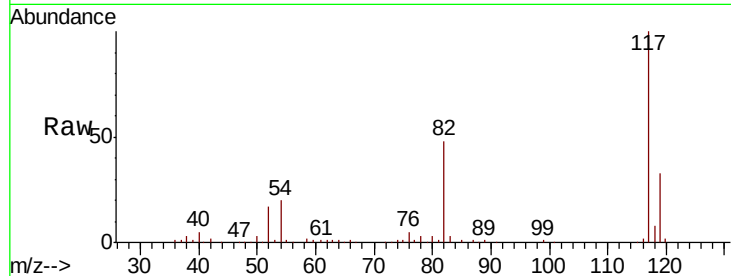


Abundance Ion 116.95 (116.65 to 117.65): V
Ion 82.05 (81.75 to 82.75): V
Ion 118.95 (118.65 to 119.65): V

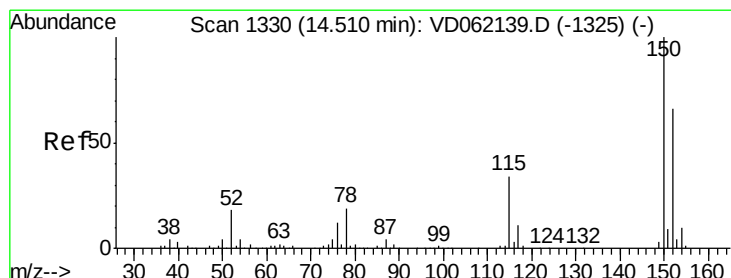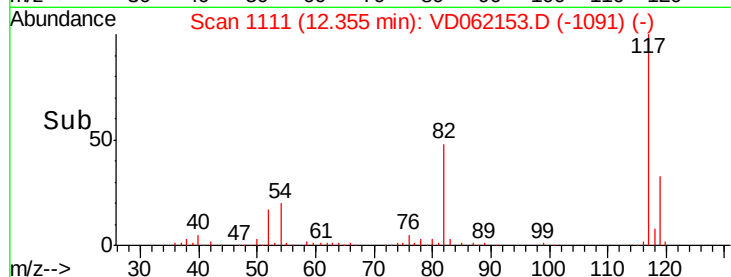
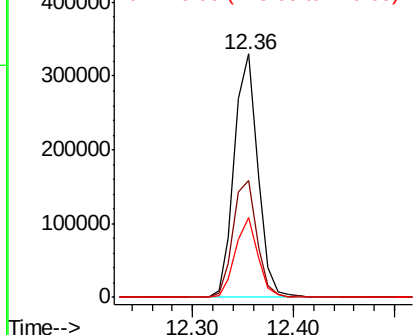



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 14.51 min Scan# 1330
Delta R.T. 0.00 min
Lab File: VD062153.D
Acq: 8 May 2019 1:55

Tgt Ion:152 Resp: 120532
Ion Ratio Lower Upper
152 100
115 51.0 30.9 92.7
150 157.6 0.0 314.8

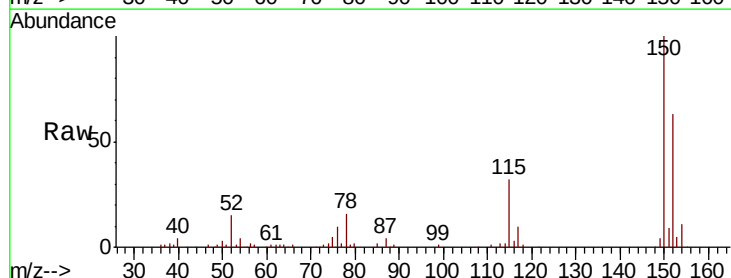

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 115.00 (114.70 to 115.70): V
Ion 149.90 (149.60 to 150.60): V

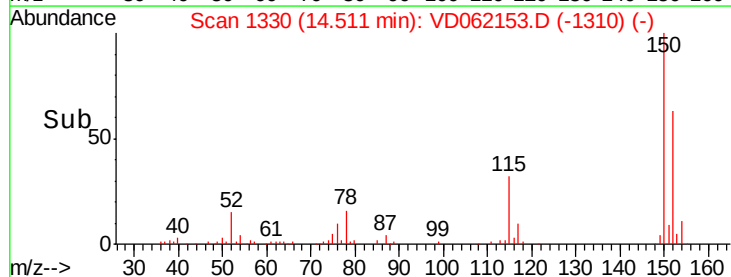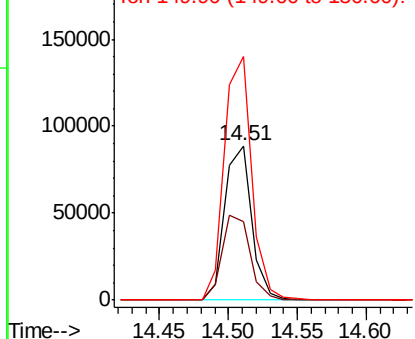







#81
trans-1,4-Dichloro-2-butene
Concen: 162.253 ug/l
RT: 13.55 min Scan# 1232
Delta R.T. 0.08 min
Lab File: VD062153.D
Acq: 8 May 2019 1:55

Instrument :
MSVOA_D
ClientSampleId :
SB-16-2.0-2.5

Tot Ion: 75 Resp: 65612
Ion Ratio Lower Upper
75 100
53 0.0 65.8 98.8#
89 0.0 35.0 52.6#




Abundance Ion 75.00 (74.70 to 75.70): VDC
Ion 53.00 (52.70 to 53.70): VDC
Ion 89.00 (88.70 to 89.70): VDC

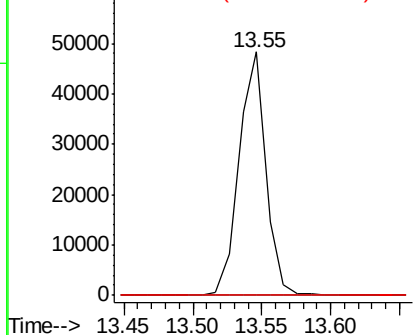

#95
Naphthalene
Concen: 7.701 ug/l
RT: 16.11 min Scan# 1493
Delta R.T. 0.00 min
Lab File: VD062153.D
Acq: 8 May 2019 1:55

Tgt Ion: 128 Resp: 23811
Ion Ratio Lower Upper
128 100
127 12.1 9.8 14.8
129 11.0 8.8 13.2



Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

