


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD050719\
Data File : VD062135.D
Acq On : 7 May 2019 9:24
Operator : FY/SY
Sample : BFB
Misc : 5.00g/5mL/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D050719S.M
Title : SW846 8260
Last Update : Tue May 07 14:26:29 2019

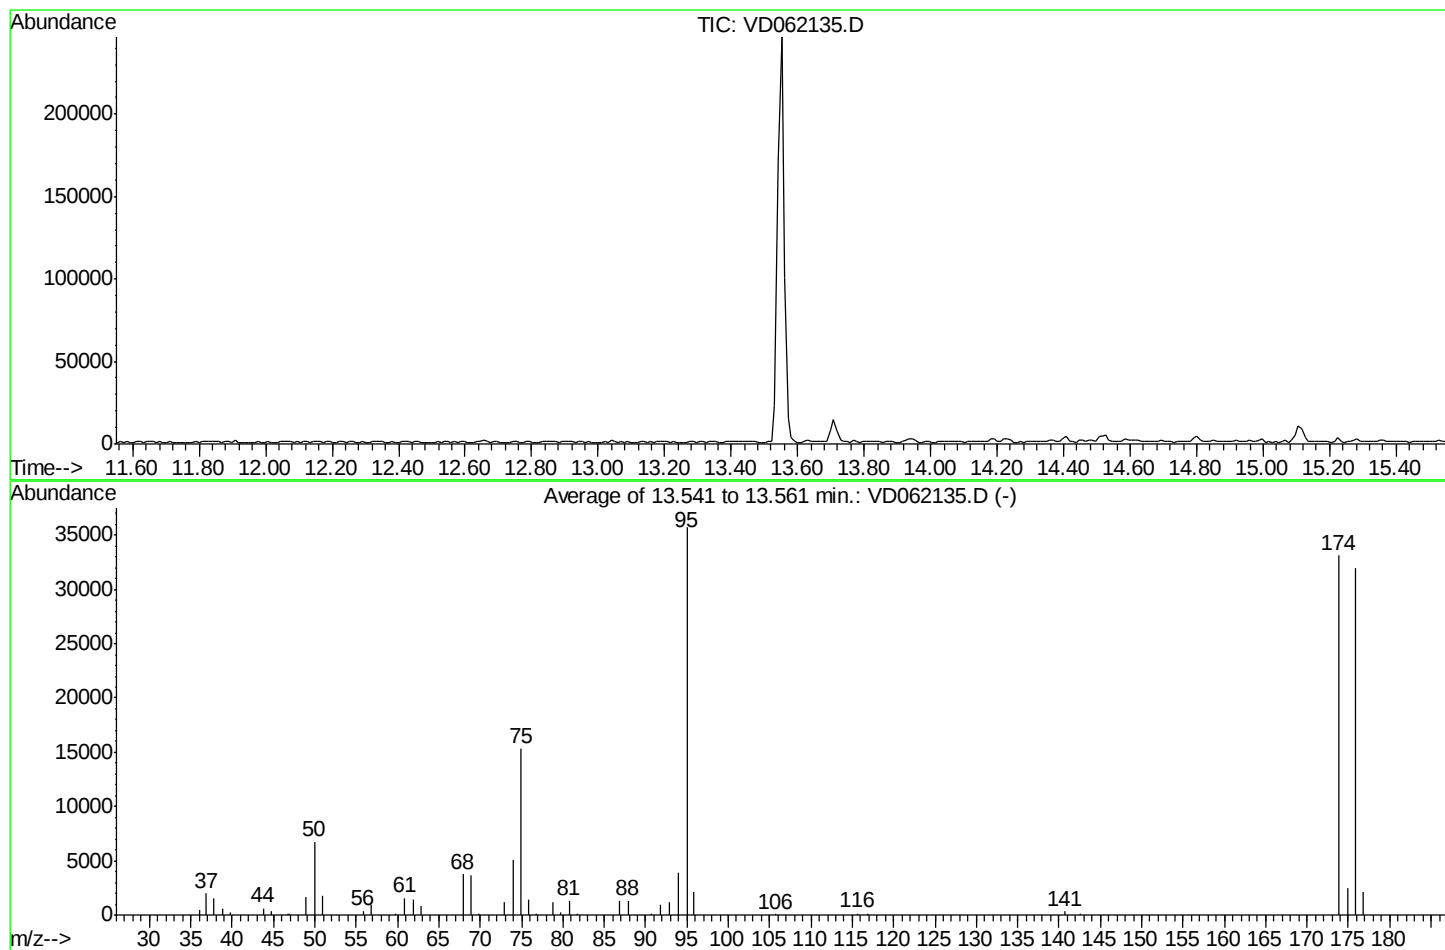

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	6781	PASS
75	95	30	60	42.8	15289	PASS
95	95	100	100	100.0	35722	PASS
96	95	5	9	6.1	2166	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.8	33136	PASS
175	174	5	9	7.6	2517	PASS
176	174	95	101	96.3	31912	PASS
177	176	5	9	6.8	2181	PASS