

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050721\
 Data File : VD069109.D
 Acq On : 07 May 2021 18:21
 Operator : VA/SY
 Sample : M2309-03
 Misc : 6.36G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 MH-TP2

Quant Time: May 08 00:09:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050421S.M
 Quant Title : SW846 8260
 QLast Update : Wed May 05 04:16:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	192710	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	378759	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.643	117	378990	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	171894	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	130805	52.67	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 105.34%	
35) Dibromofluoromethane	7.914	113	140090	53.93	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 107.86%	
50) Toluene-d8	10.338	98	483530	50.43	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 100.86%	
62) 4-Bromofluorobenzene	12.626	95	155454	49.29	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 98.58%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050721\
Data File : VD069109.D
Acq On : 07 May 2021 18:21
Operator : VA/SY
Sample : M2309-03
Misc : 6.36G/5.00ml/MSVOA_D/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
MH-TP2

Quant Time: May 08 00:09:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050421S.M
Quant Title : SW846 8260
QLast Update : Wed May 05 04:16:41 2021
Response via : Initial Calibration




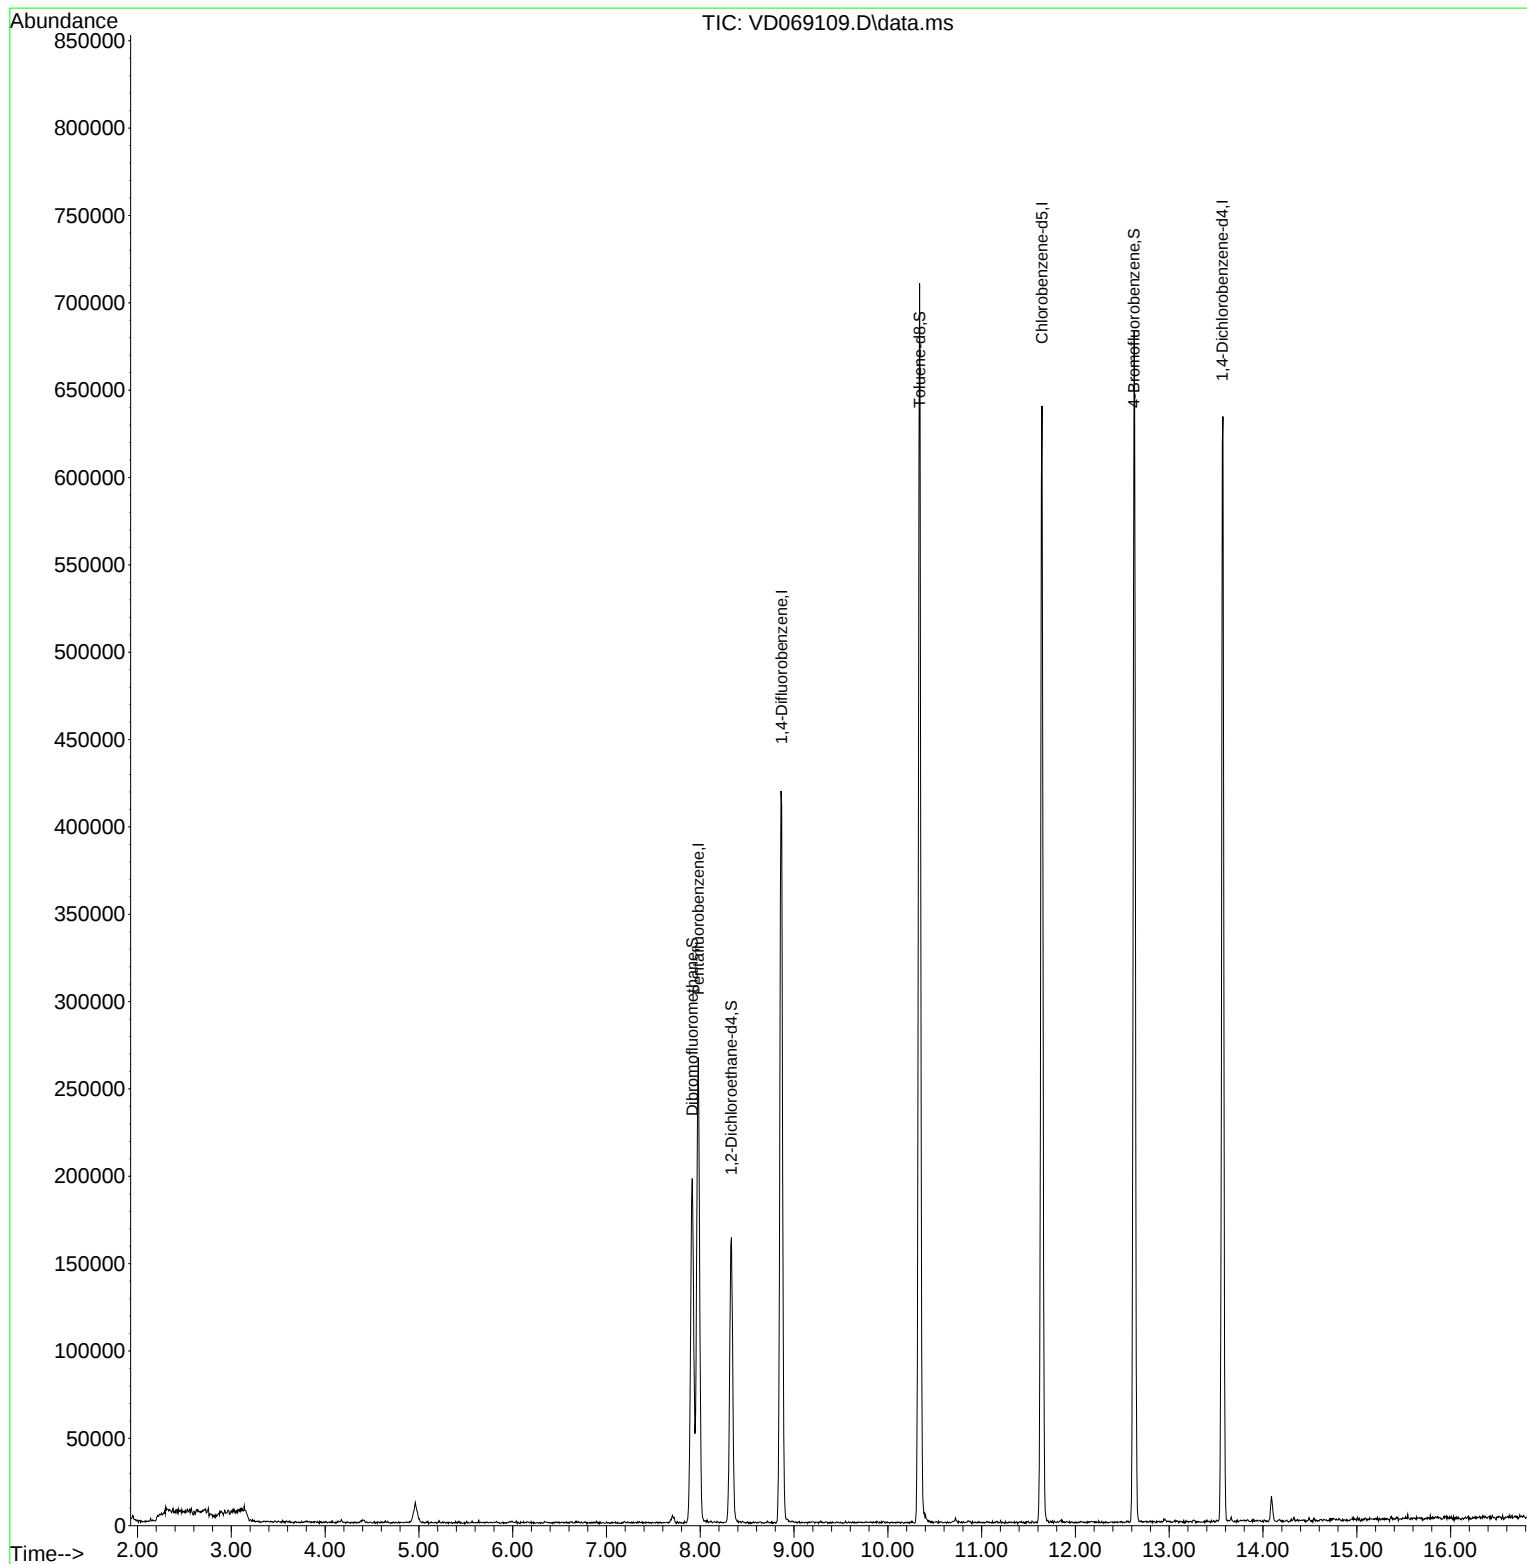


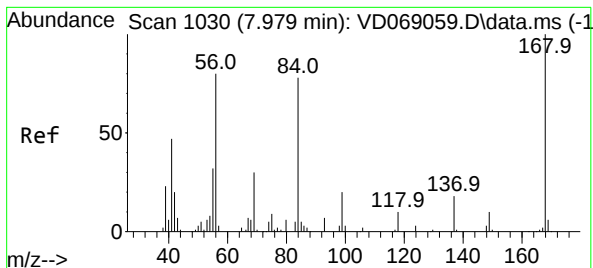

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.000 min
Lab File: VD069109.D
Acq: 07 May 2021 18:21




Instrument :
MSVOA_D
ClientSampleId :
MH-TP2


Tgt Ion:168 Resp: 192710
Ion Ratio Lower Upper
168 100
99 57.3 52.6 78.8

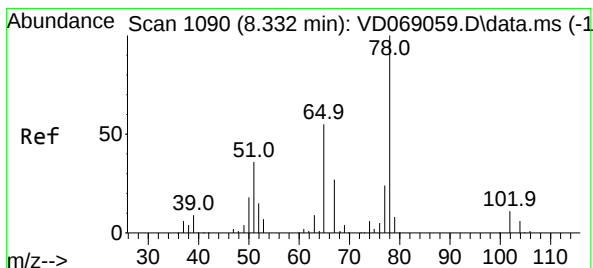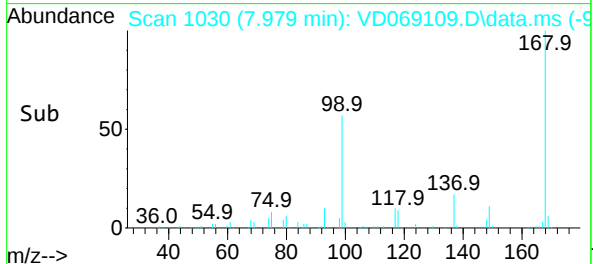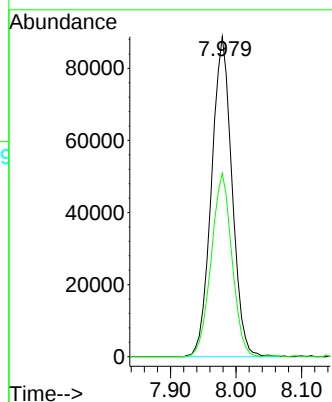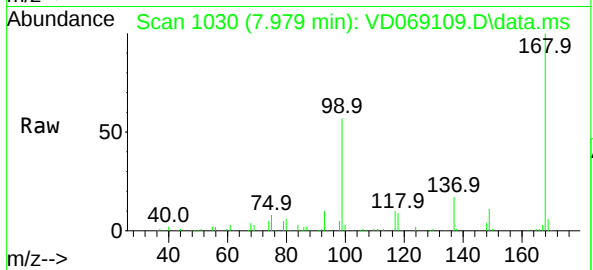

#33
1,2-Dichloroethane-d4
Concen: 52.67 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. -0.000 min
Lab File: VD069109.D
Acq: 07 May 2021 18:21

Tgt Ion: 65 Resp: 130805
Ion Ratio Lower Upper
65 100
67 51.5 0.0 103.4

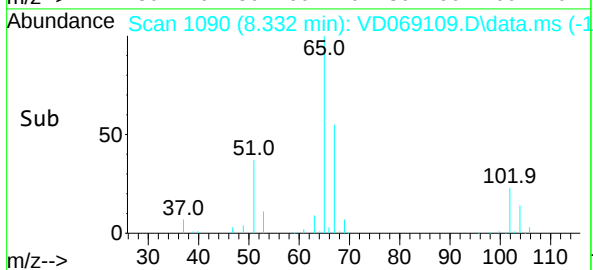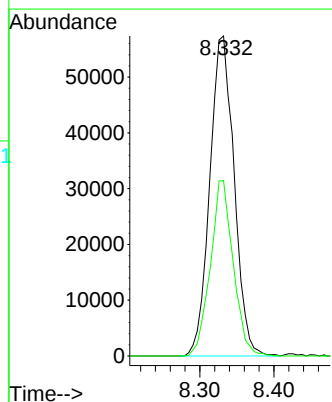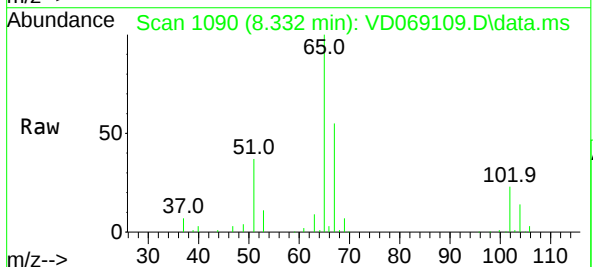

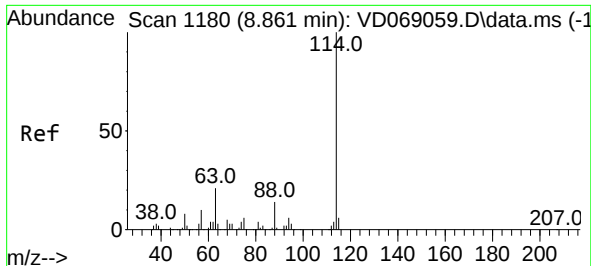

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 8.867 min Scan# 1181

Delta R.T. 0.006 min

Lab File: VD069109.D

Acq: 07 May 2021 18:21





Tgt Ion:114 Resp: 378759

Ion Ratio Lower Upper

114 100

63 17.7 0.0 41.4

88 13.7 0.0 27.8

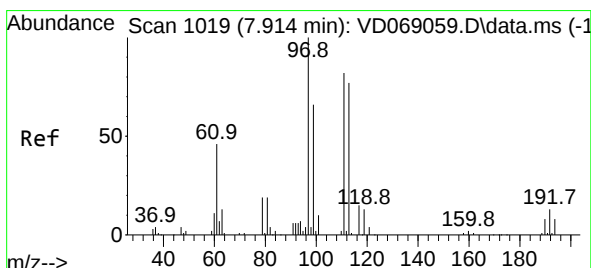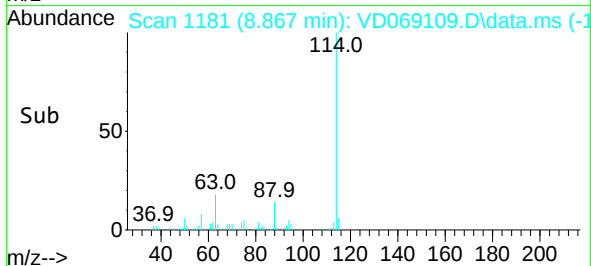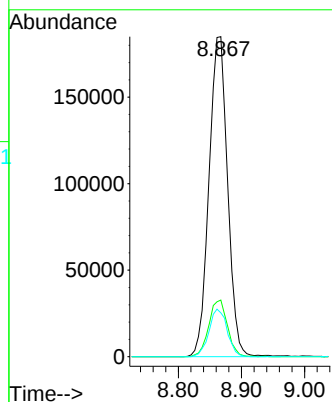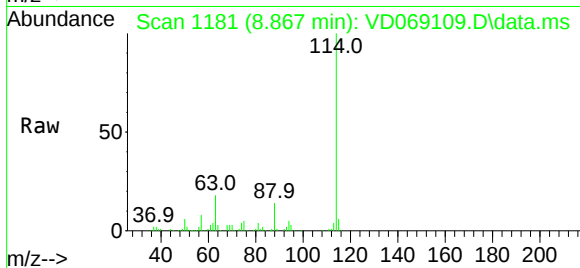

#35

Dibromofluoromethane

Concen: 53.93 ug/l

RT: 7.914 min Scan# 1019

Delta R.T. -0.000 min

Lab File: VD069109.D

Acq: 07 May 2021 18:21




Tgt Ion:113 Resp: 140090


Ion Ratio Lower Upper

113 100

111 102.9 84.6 126.8

192 17.6 13.5 20.3


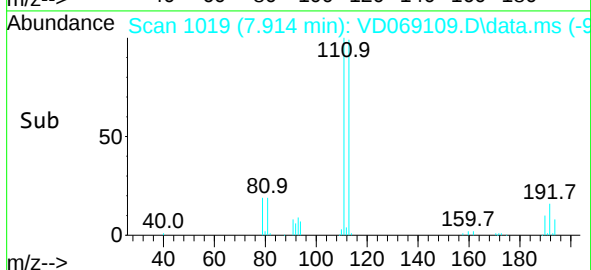
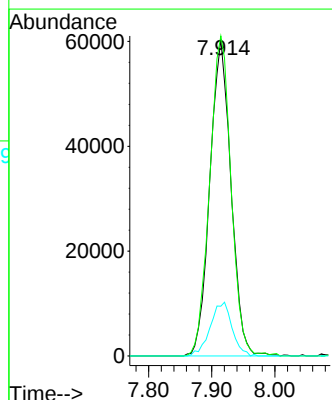
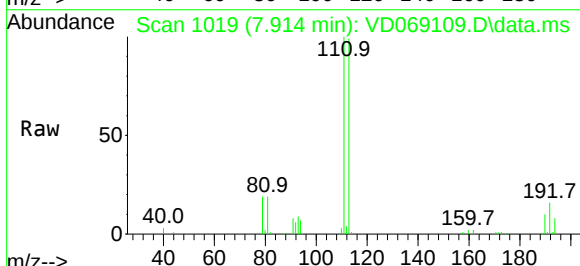


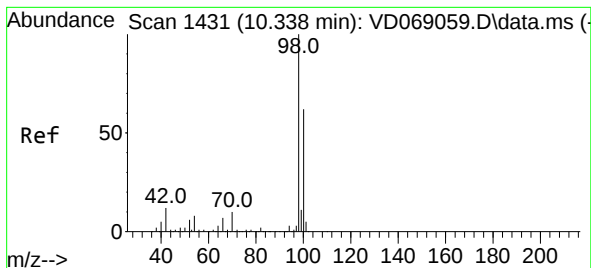

#50
Toluene-d8
Concen: 50.43 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.000 min
Lab File: VD069109.D
Acq: 07 May 2021 18:21




Instrument :
MSVOA_D
ClientSampleId :
MH-TP2


Tgt Ion: 98 Resp: 483530
Ion Ratio Lower Upper
98 100
100 64.1 51.6 77.4

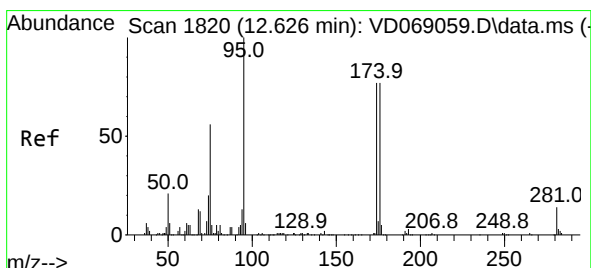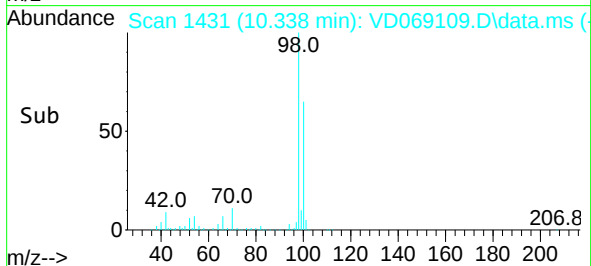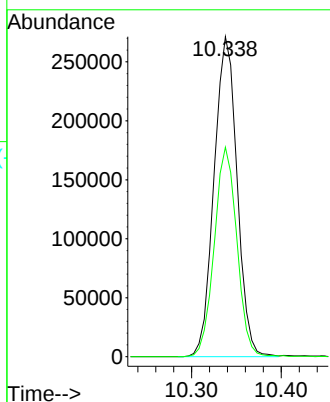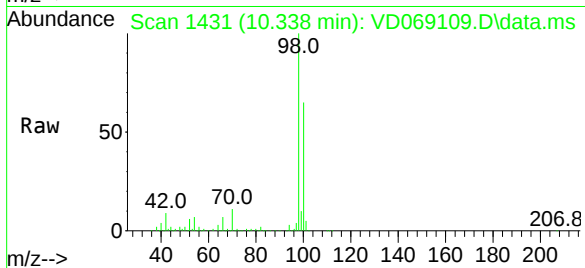

#62
4-Bromofluorobenzene
Concen: 49.29 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.000 min
Lab File: VD069109.D
Acq: 07 May 2021 18:21

Tgt Ion: 95 Resp: 155454
Ion Ratio Lower Upper
95 100
174 86.6 0.0 156.0
176 84.7 0.0 149.4


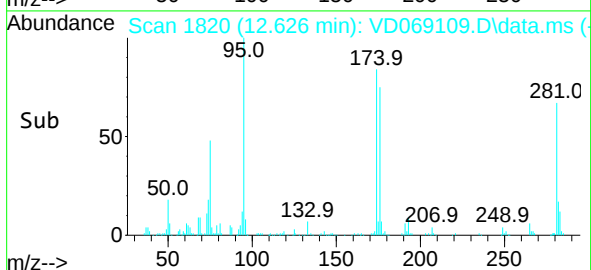
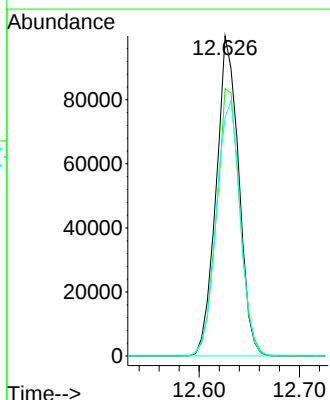
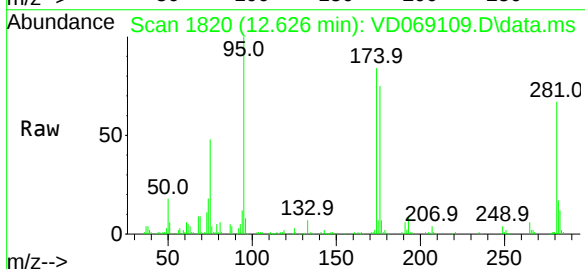


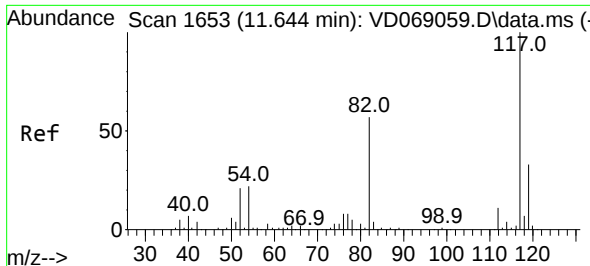

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.643 min Scan# 1653
Delta R.T. -0.000 min
Lab File: VD069109.D
Acq: 07 May 2021 18:21

Instrument :
MSVOA_D
ClientSampleId :
MH-TP2

Tgt Ion:117 Resp: 378990
Ion Ratio Lower Upper
117 100
82 52.8 45.4 68.2
119 31.4 26.8 40.2

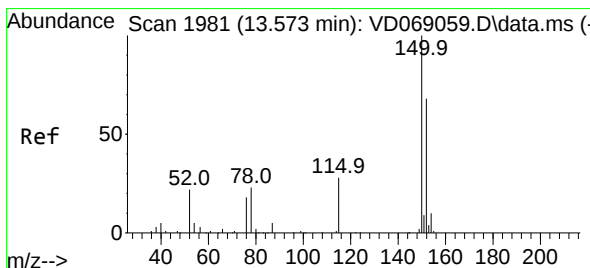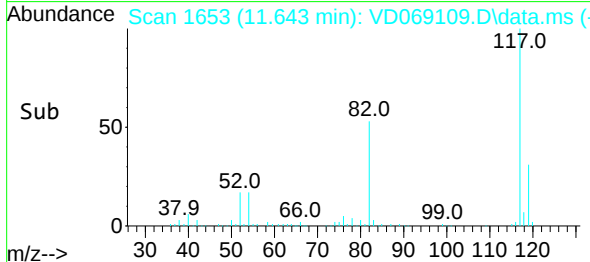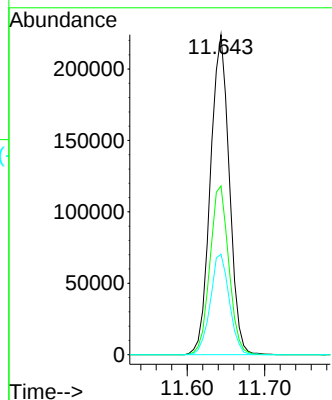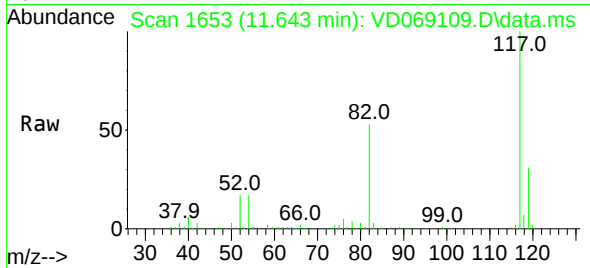

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. -0.006 min
Lab File: VD069109.D
Acq: 07 May 2021 18:21

Tgt Ion:152 Resp: 171894
Ion Ratio Lower Upper
152 100
115 58.4 30.5 91.5
150 157.2 0.0 340.8

