
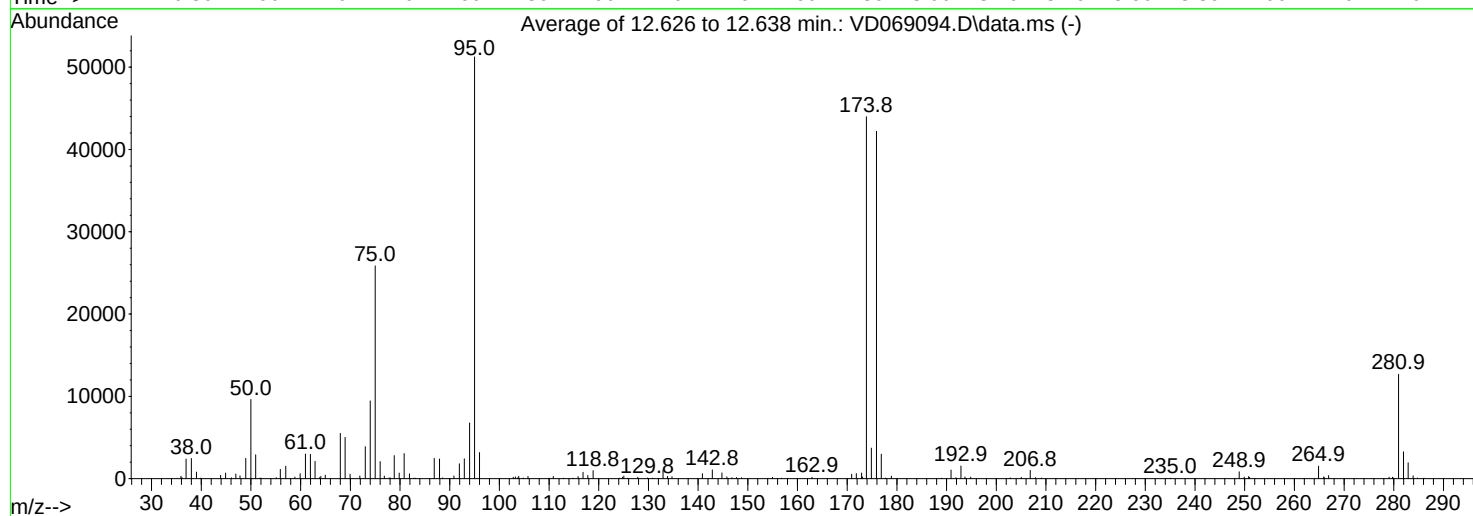


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050721\
Data File : VD069094.D
Acq On : 07 May 2021 10:39
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050421S.M
Title : SW846 8260
Last Update : Wed May 05 04:16:41 2021

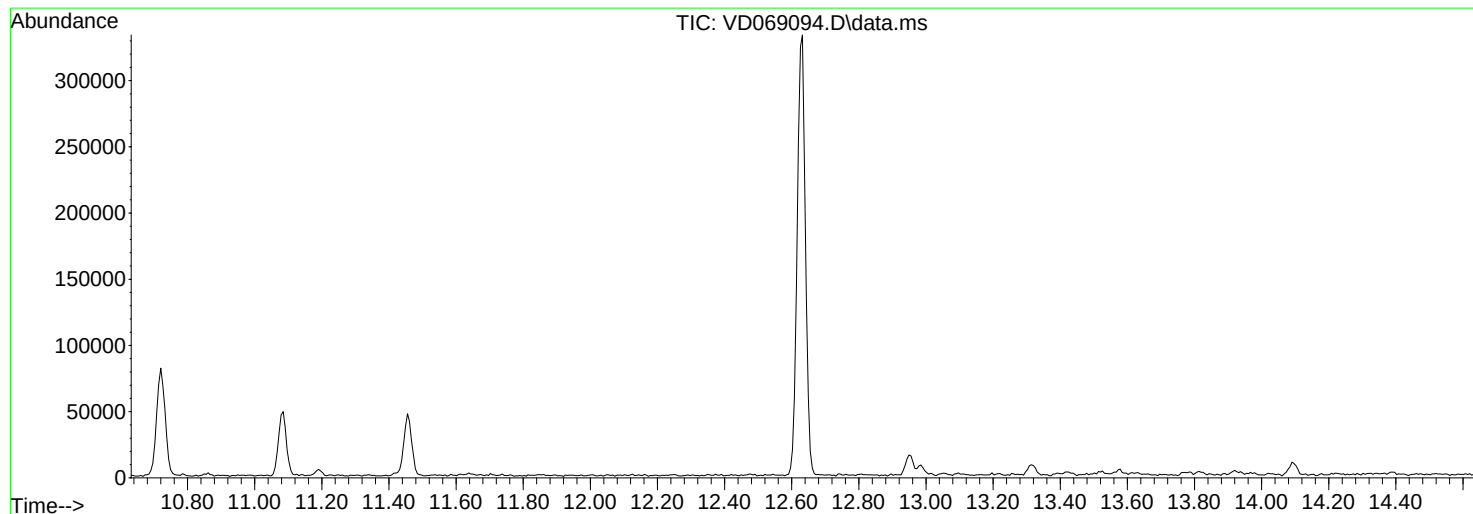

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	9623	PASS
75	95	30	60	50.5	25859	PASS
95	95	100	100	100.0	51256	PASS
96	95	5	9	6.2	3163	PASS
173	174	0.00	2	1.5	677	PASS
174	95	50	100	85.8	43979	PASS
175	174	5	9	8.4	3713	PASS
176	174	95	101	96.0	42213	PASS
177	176	5	9	7.1	2978	PASS