


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD050820\
Data File : VD065716.D
Acq On : 08 May 2020 10:43
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D050620S.M
Title : SW846 8260
Last Update : Wed May 06 17:01:16 2020

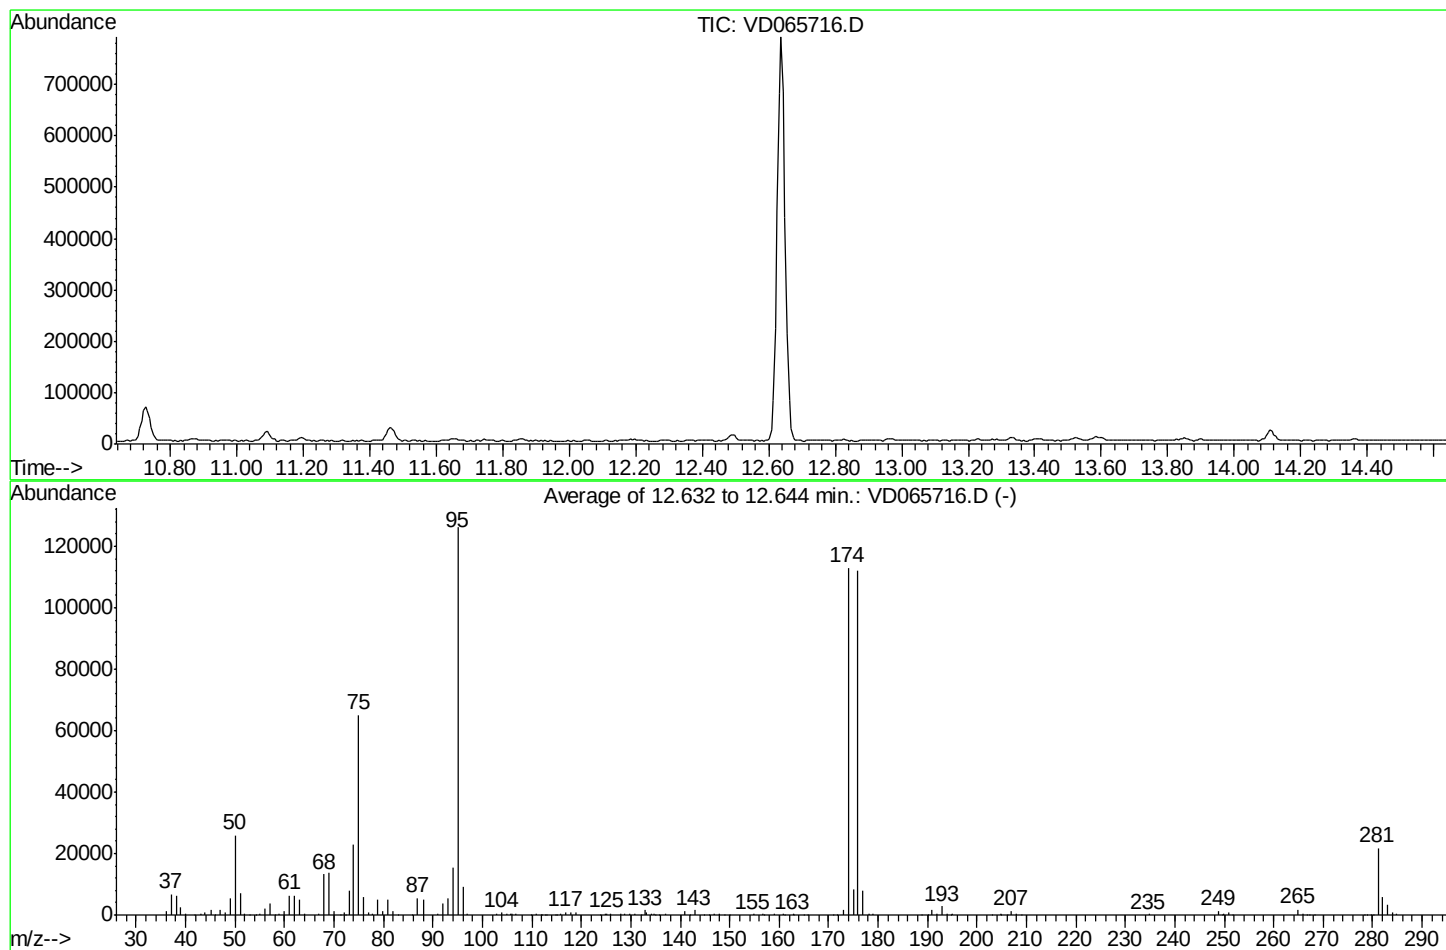

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	25968	PASS
75	95	30	60	51.5	65032	PASS
95	95	100	100	100.0	126173	PASS
96	95	5	9	7.1	9001	PASS
173	174	0.00	2	1.3	1515	PASS
174	95	50	100	89.5	112906	PASS
175	174	5	9	7.5	8484	PASS
176	174	95	101	99.1	111938	PASS
177	176	5	9	7.0	7844	PASS