

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051021\
 Data File : VD069121.D
 Acq On : 10 May 2021 14:20
 Operator : VA/SY
 Sample : M2330-01RE
 Misc : 6.69G/5.00ml/MSVOA_D/soil
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 CFOS-SOILRE

Quant Time: May 10 16:11:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050421S.M
 Quant Title : SW846 8260
 QLast Update : Wed May 05 04:16:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	192813	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	401587	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	293815	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	57497	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	141675	57.01	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 114.02%			
35) Dibromofluoromethane	7.914	113	141982	51.56	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 103.12%			
50) Toluene-d8	10.338	98	430354	42.33	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery = 84.66%			
62) 4-Bromofluorobenzene	12.626	95	97770	29.24	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 58.48%			
Target Compounds					Qvalue	
10) Methyl Iodide	4.297	142	493	3.40	ug/l #	49
11) Tert butyl alcohol	5.232	59	13989	39.74	ug/l #	95
16) Acetone	4.156	43	158381	476.29	ug/l	97
17) Carbon Disulfide	4.403	76	9866	1.44	ug/l #	78
20) Methylene Chloride	4.956	84	14489	Below Cal	#	77
25) 2-Butanone	7.220	43	31787	59.84	ug/l	99
31) Cyclohexane	7.985	56	6038	1.68	ug/l #	41
37) Ethyl Acetate	7.220	43	31787	19.96	ug/l #	69
40) Benzene	8.350	78	18113	1.55	ug/l	100
41) Methacrylonitrile	7.550	41	1057	1.14	ug/l #	15
43) Isopropyl Acetate	8.508	43	20675	6.92	ug/l #	49
48) Methyl methacrylate	9.479	41	3363	2.28	ug/l #	52
51) 4-Methyl-2-Pentanone	10.226	43	8957	5.86	ug/l	96
52) Toluene	10.402	92	20805	2.80	ug/l	98
56) Ethyl methacrylate	10.667	69	534	2.56	ug/l #	26
59) 2-Hexanone	10.985	43	7951	7.71	ug/l	99
67) Ethyl Benzene	11.744	91	40083	3.77	ug/l	95
68) m/p-Xylenes	11.849	106	21374	5.35	ug/l	88
69) o-Xylene	12.179	106	12591	3.51	ug/l	91
73) Isopropylbenzene	12.473	105	12499	3.14	ug/l	91
74) N-amyl acetate	12.249	43	9565	11.45	ug/l #	45
76) 1,2,3-Trichloropropane	12.632	75	51916	103.72	ug/l #	100
78) n-propylbenzene	12.820	91	25825	5.28	ug/l	95
80) 1,3,5-Trimethylbenzene	12.955	105	9674	2.86	ug/l	93
81) trans-1,4-Dichloro-2-b...	12.632	75	51916	225.69	ug/l #	11
82) 4-Chlorotoluene	12.820	91	25825	8.85	ug/l #	40
83) tert-Butylbenzene	13.220	119	207068	75.00	ug/l	99
84) 1,2,4-Trimethylbenzene	13.261	105	24725	7.30	ug/l	95
85) sec-Butylbenzene	13.391	105	11041	2.76	ug/l	96
86) p-Isopropyltoluene	13.508	119	5442	1.48	ug/l #	75
89) n-Butylbenzene	13.838	91	14745	4.21	ug/l	96
90) Hexachloroethane	14.114	117	2592	3.42	ug/l #	23
95) Naphthalene	15.396	128	6529	5.98	ug/l #	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

MSVOA_D


ClientSampleId :


CFOS-SOILRE

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051021\
 Data File : VD069121.D
 Acq On : 10 May 2021 14:20
 Operator : VA/SY
 Sample : M2330-01RE
 Misc : 6.69G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 CFOS-SOILRE

Quant Time: May 10 16:11:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050421S.M
 Quant Title : SW846 8260
 QLast Update : Wed May 05 04:16:41 2021
 Response via : Initial Calibration




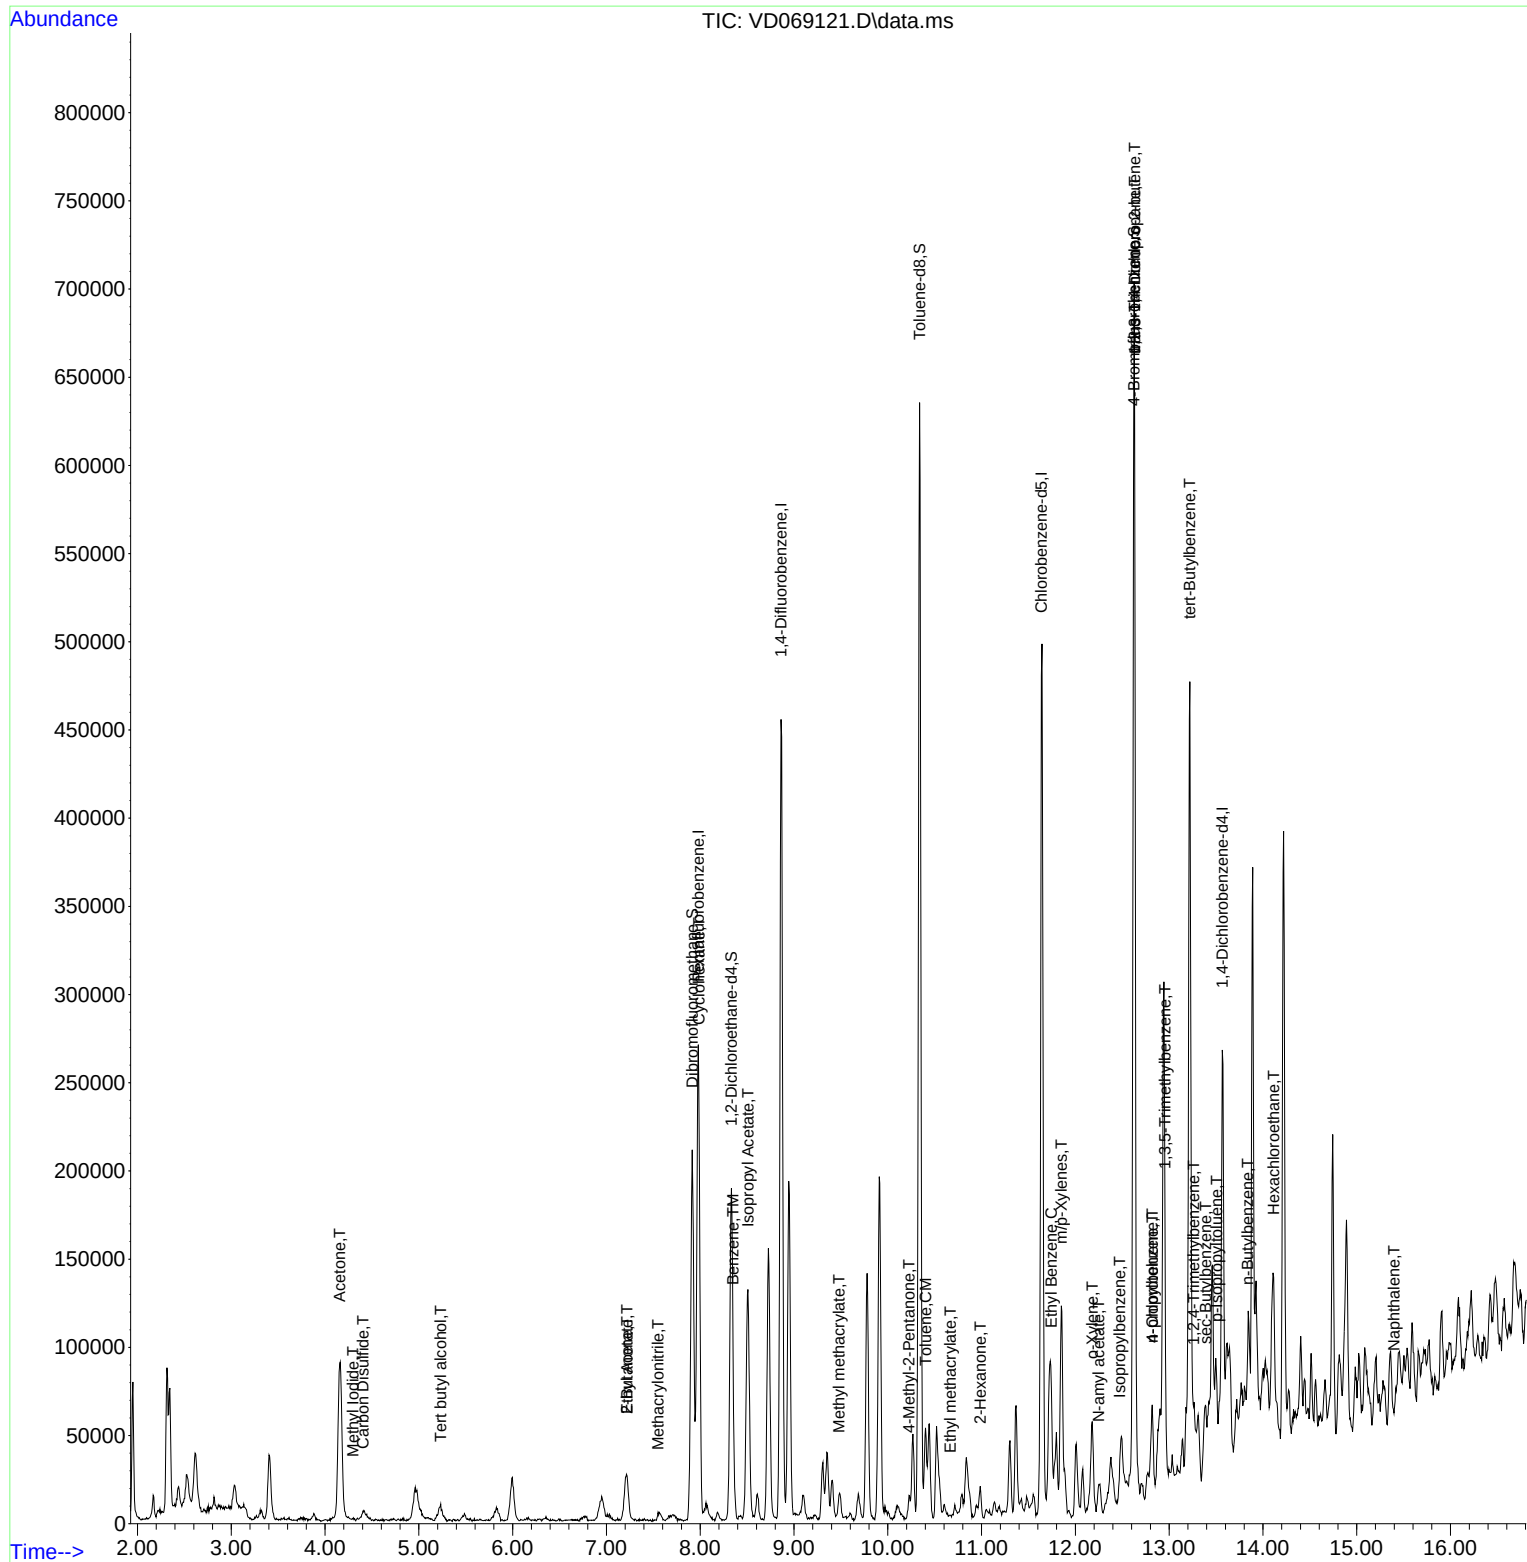


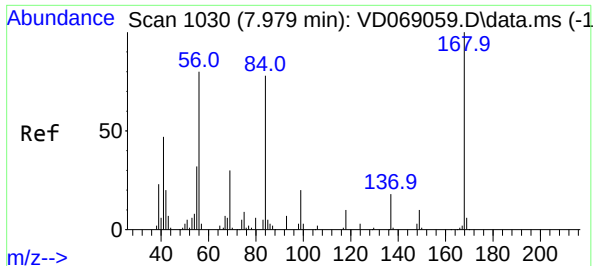

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20




Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE


Tgt Ion:168 Resp: 192813
Ion Ratio Lower Upper
168 100
99 59.3 52.6 78.8

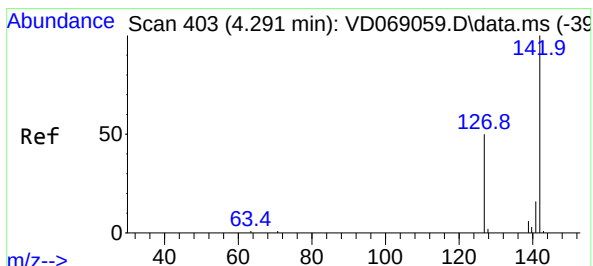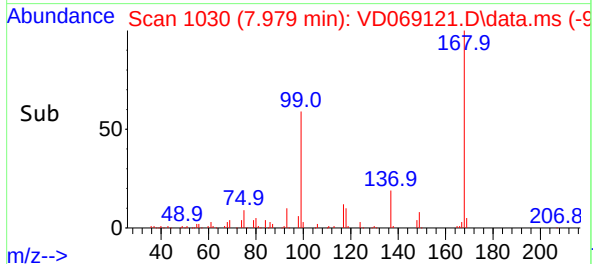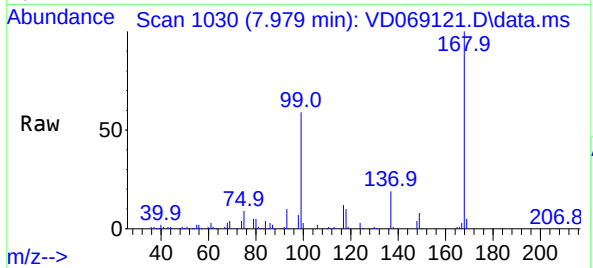

#10
Methyl Iodide
Concen: 3.40 ug/l
RT: 4.297 min Scan# 404
Delta R.T. 0.006 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion:142 Resp: 493
Ion Ratio Lower Upper
142 100
127 13.4 41.6 62.4#
141 0.0 12.2 18.4#

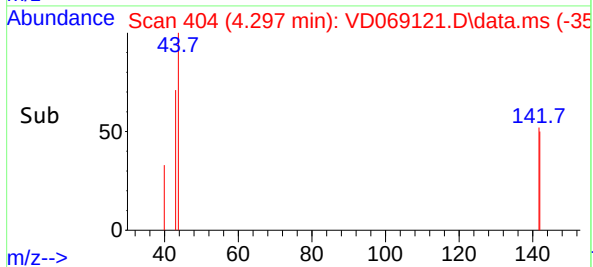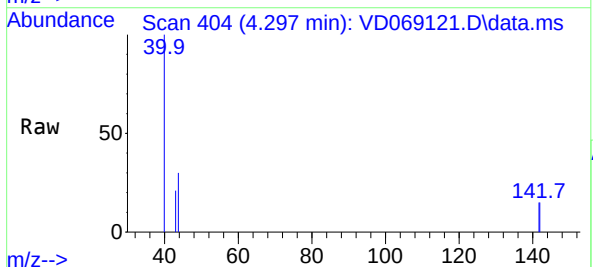







#11

Tert butyl alcohol
Concen: 39.74 ug/l
RT: 5.232 min Scan# 563
Delta R.T. 0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE




Tgt Ion: 59 Resp: 13989
Ion Ratio Lower Upper
59 100
57 8.2 5.3 7.9#

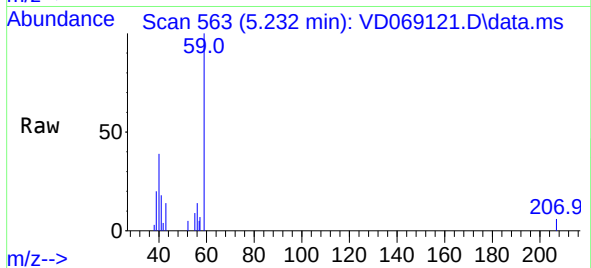


#16

Acetone
Concen: 476.29 ug/l
RT: 4.156 min Scan# 380
Delta R.T. -0.006 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion: 43 Resp: 158381
Ion Ratio Lower Upper
43 100
58 32.3 24.5 36.7


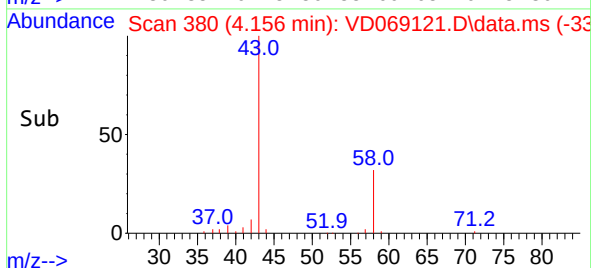
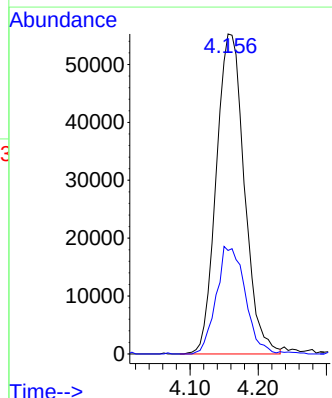





#17
Carbon Disulfide
Concen: 1.44 ug/l
RT: 4.403 min Scan# 422
Delta R.T. -0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20




Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE


Tgt Ion: 76 Resp: 9866
Ion Ratio Lower Upper
76 100
78 17.3 7.4 11.2#

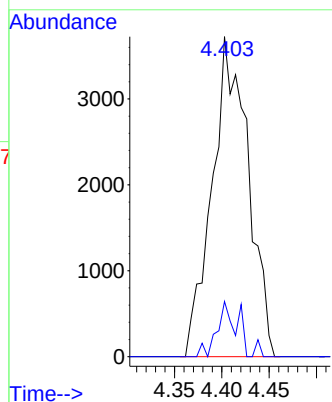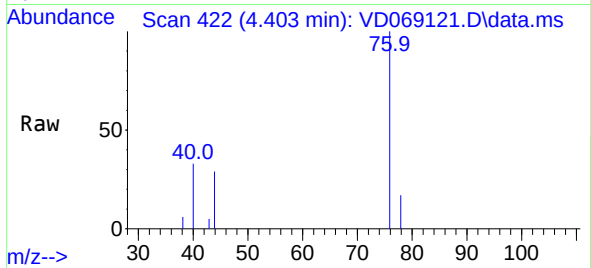

#25
2-Butanone
Concen: 59.84 ug/l
RT: 7.220 min Scan# 901
Delta R.T. 0.006 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion: 43 Resp: 31787
Ion Ratio Lower Upper
43 100
72 29.1 23.0 34.4

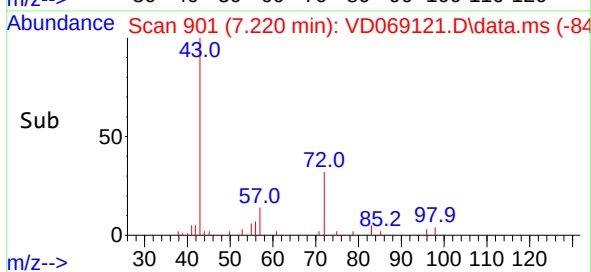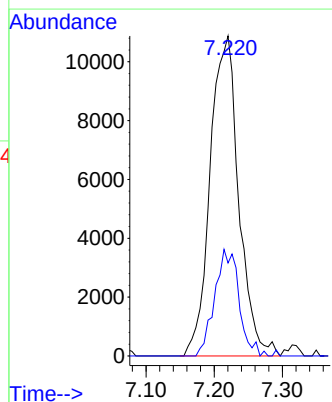

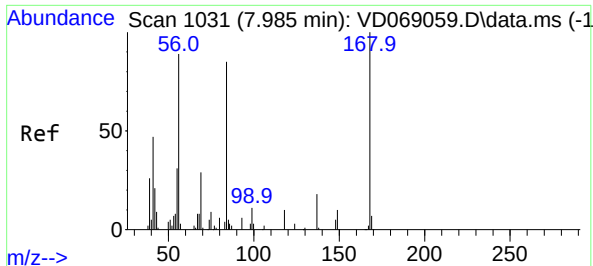

#31

Cyclohexane

Concen: 1.68 ug/l

RT: 7.985 min Scan# 1031





Delta R.T. -0.000 min

Lab File: VD069121.D

Acq: 10 May 2021 14:20

Tgt Ion: 56 Resp: 6038

Ion	Ratio	Lower	Upper
56	100		
69	134.1	26.3	39.5#
84	111.8	75.9	113.9

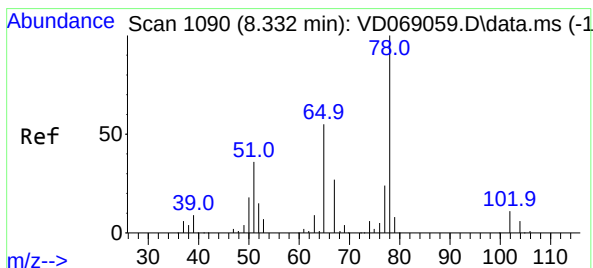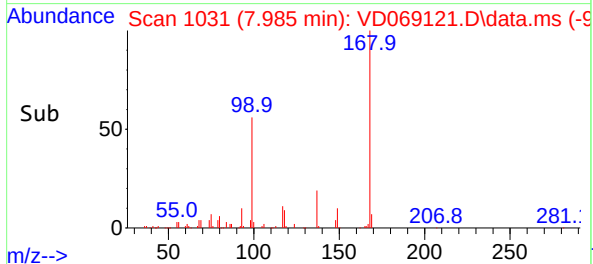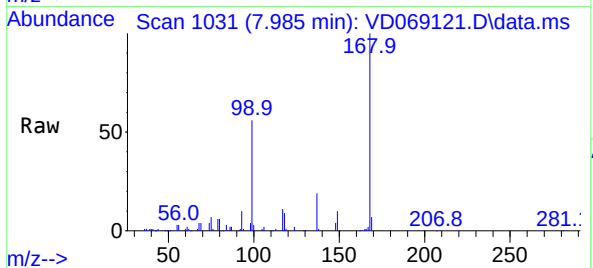

#33

1,2-Dichloroethane-d4

Concen: 57.01 ug/l

RT: 8.332 min Scan# 1090




Delta R.T. -0.000 min

Lab File: VD069121.D

Acq: 10 May 2021 14:20

Tgt Ion: 65 Resp: 141675

Ion	Ratio	Lower	Upper
65	100		
67	52.7	0.0	103.4

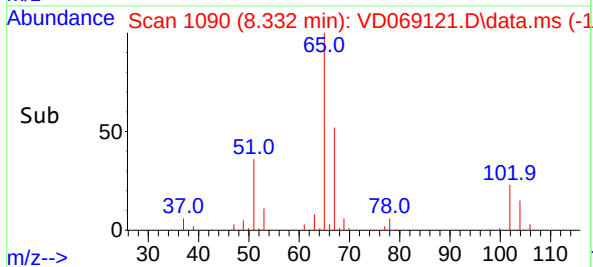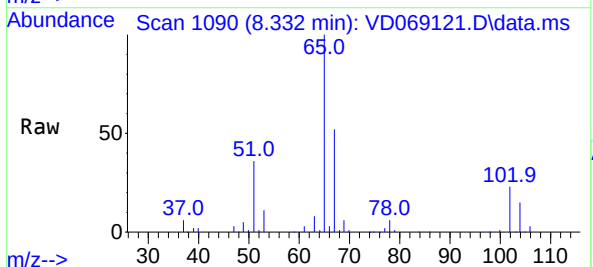


Instrument :

MSVOA_D

ClientSampleId :

CFOS-SOILRE




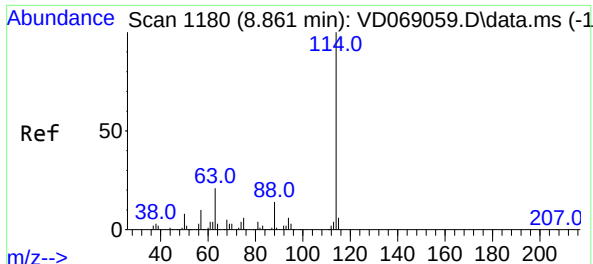


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. 0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE




Tgt Ion:114	Resp:	401587
Ion Ratio	Lower	Upper
114	100	
63	19.9	0.0 41.4
88	14.2	0.0 27.8

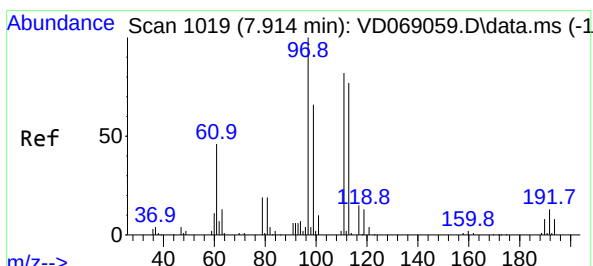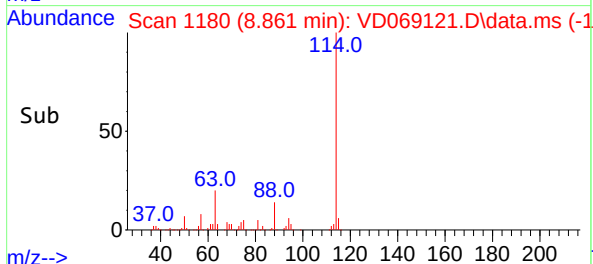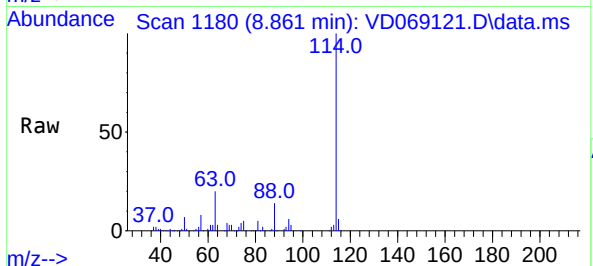


#35

Dibromofluoromethane
Concen: 51.56 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. -0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion:113	Resp:	141982
Ion Ratio	Lower	Upper
113	100	
111	104.8	84.6 126.8
192	18.9	13.5 20.3


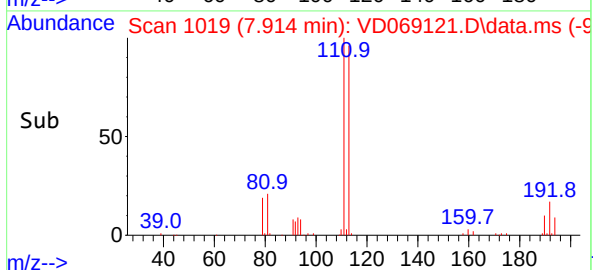

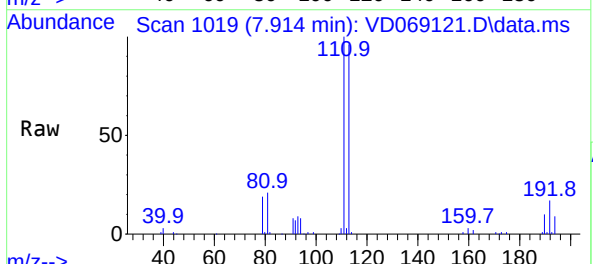




#37
Ethyl Acetate
Concen: 19.96 ug/l
RT: 7.220 min Scan# 901
Delta R.T. -0.077 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20




Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE


Tgt Ion: 43 Resp: 31787
Ion Ratio Lower Upper
43 100
61 0.0 11.0 16.4#
70 0.2 8.5 12.7#

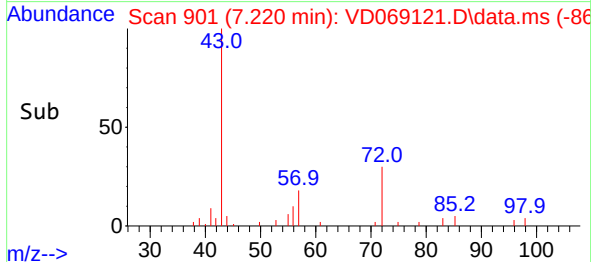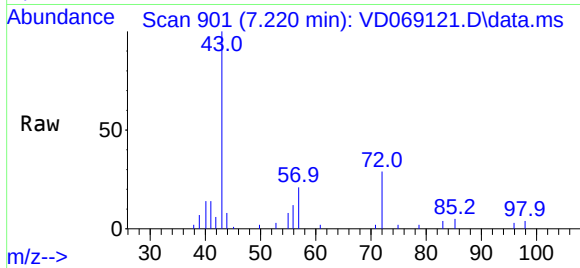

#40
Benzene
Concen: 1.55 ug/l
RT: 8.350 min Scan# 1093
Delta R.T. -0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion: 78 Resp: 18113
Ion Ratio Lower Upper
78 100
77 25.5 20.5 30.7


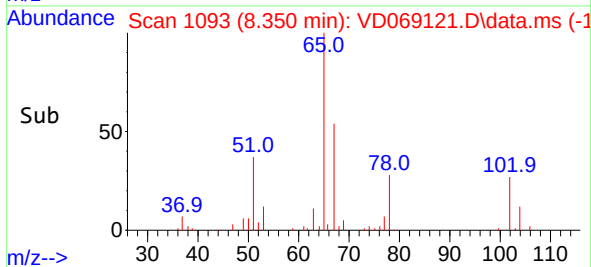

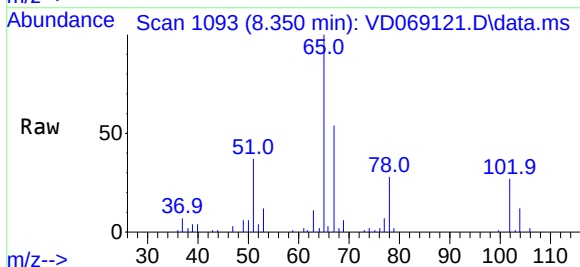




#41
Methacrylonitrile
Concen: 1.14 ug/l
RT: 7.550 min Scan# 957
Delta R.T. 0.006 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20




Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE


Tgt Ion: 41 Resp: 1057
Ion Ratio Lower Upper
41 100
39 0.0 55.4 83.2#
67 8.8 0.0 0.0#
52 0.0 0.0 0.0

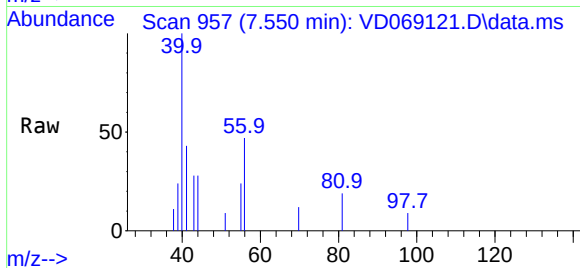

#43
Isopropyl Acetate
Concen: 6.92 ug/l
RT: 8.508 min Scan# 1120
Delta R.T. 0.059 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion: 43 Resp: 20675
Ion Ratio Lower Upper
43 100
61 0.0 26.1 39.1#
87 0.0 11.7 17.5#


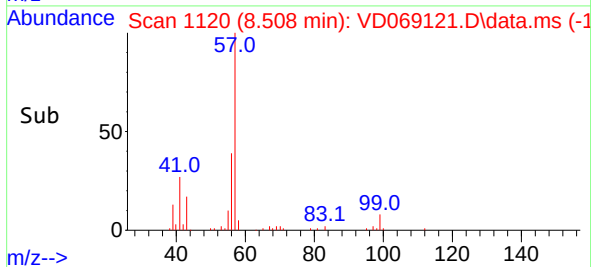

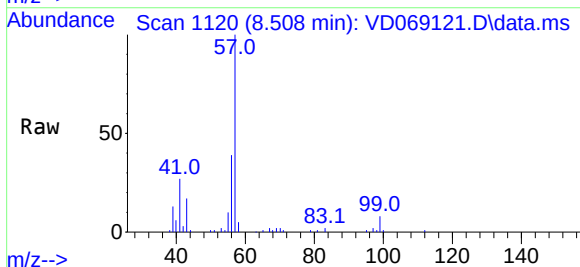


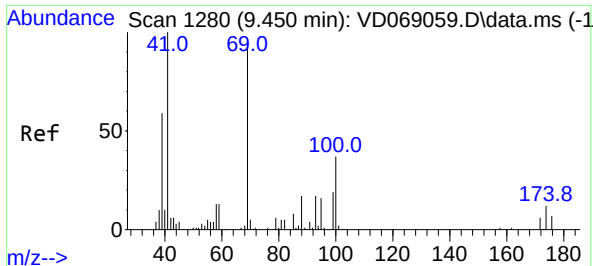

#48
Methyl methacrylate
Concen: 2.28 ug/l
RT: 9.479 min Scan# 1285
Delta R.T. 0.029 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20




Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE


Tgt Ion: 41 Resp: 3363
Ion Ratio Lower Upper
41 100
69 17.3 73.9 110.9#
39 60.7 51.0 76.4

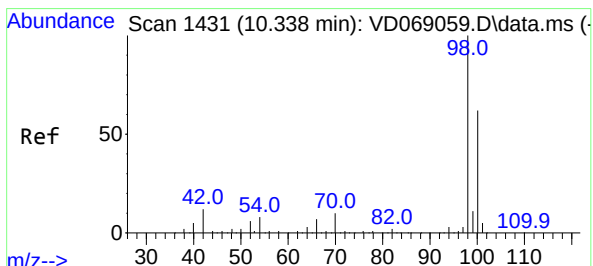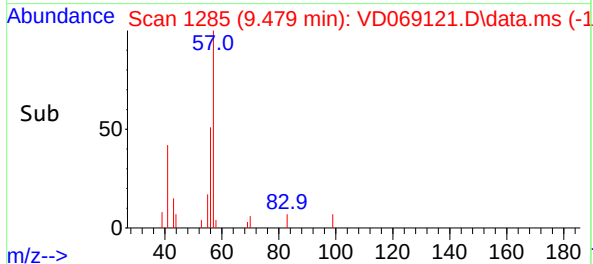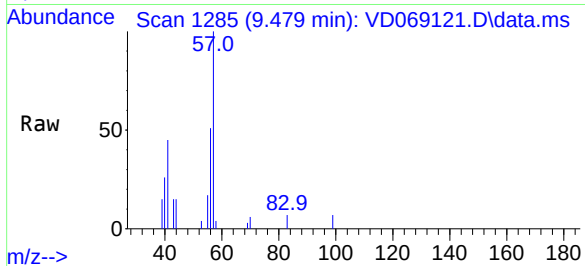

#50
Toluene-d8
Concen: 42.33 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion: 98 Resp: 430354
Ion Ratio Lower Upper
98 100
100 64.6 51.6 77.4


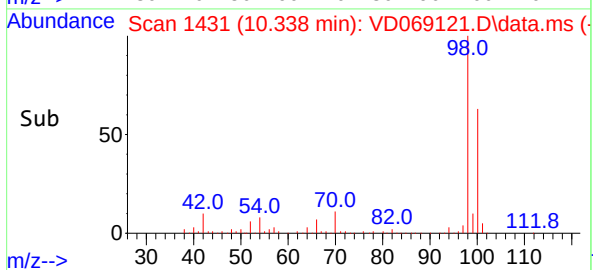

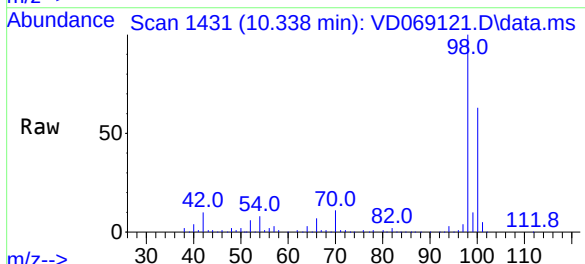




#51
4-Methyl-2-Pentanone
Concen: 5.86 ug/l
RT: 10.226 min Scan# 1412
Delta R.T. -0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20




Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE


Tgt Ion: 43 Resp: 8957
Ion Ratio Lower Upper
43 100
58 38.6 32.7 49.1

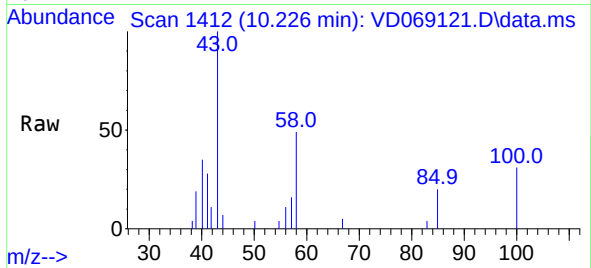

#52
Toluene
Concen: 2.80 ug/l
RT: 10.402 min Scan# 1442
Delta R.T. -0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion: 92 Resp: 20805
Ion Ratio Lower Upper
92 100
91 175.7 138.2 207.2


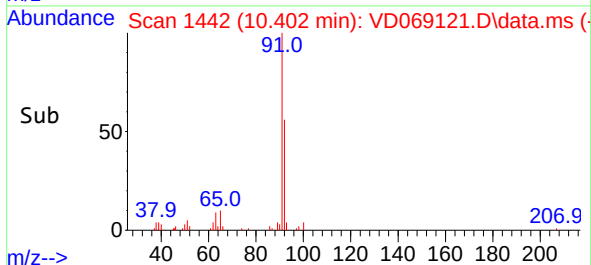

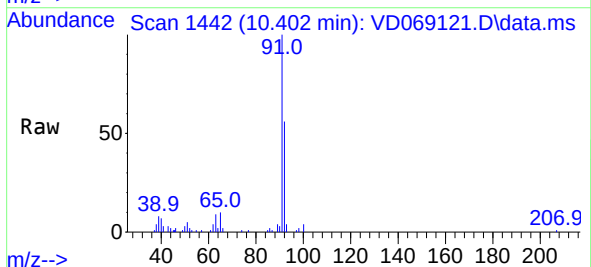




#56
Ethyl methacrylate
Concen: 2.56 ug/l
RT: 10.667 min Scan# 1487
Delta R.T. 0.006 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20




Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE


Tgt Ion: 69 Resp: 534
Ion Ratio Lower Upper
69 100
41 0.0 49.2 73.8#
39 0.0 29.8 44.6#

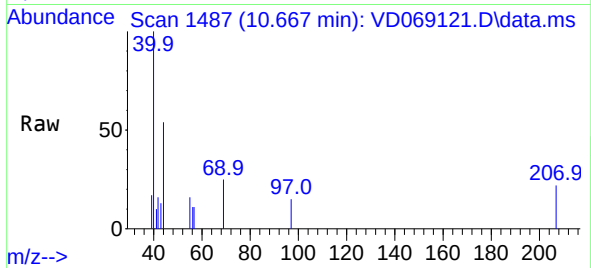

#59
2-Hexanone
Concen: 7.71 ug/l
RT: 10.985 min Scan# 1541
Delta R.T. 0.006 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion: 43 Resp: 7951
Ion Ratio Lower Upper
43 100
58 55.2 27.9 83.6


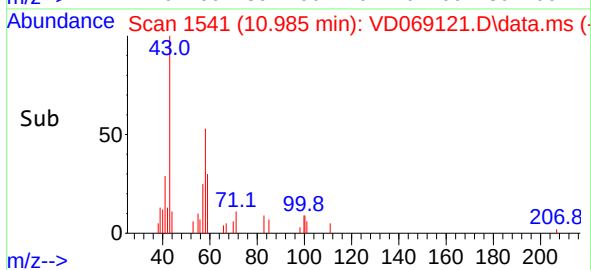

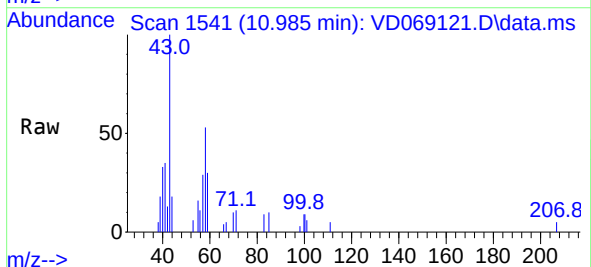




#62
4-Bromofluorobenzene
Concen: 29.24 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20




Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE


Tgt Ion: 95 Resp: 97770
Ion Ratio Lower Upper
95 100
174 84.2 0.0 156.0
176 83.4 0.0 149.4

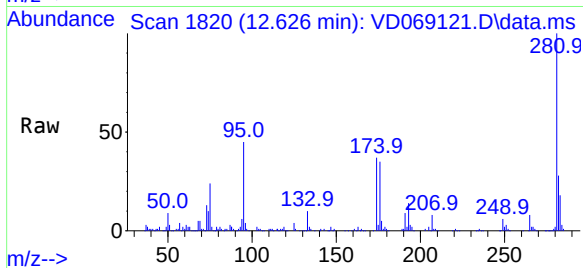

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. -0.006 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion: 117 Resp: 293815
Ion Ratio Lower Upper
117 100
82 49.0 45.4 68.2
119 29.6 26.8 40.2


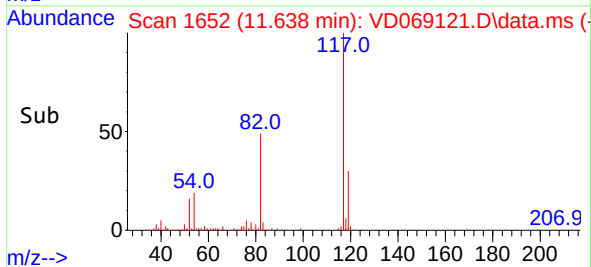

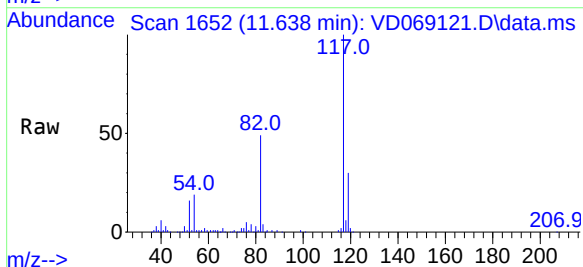




#67
Ethyl Benzene
Concen: 3.77 ug/l
RT: 11.744 min Scan# 1670
Delta R.T. -0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20




Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE


Tgt Ion: 91 Resp: 40083
Ion Ratio Lower Upper
91 100
106 28.9 25.5 38.3

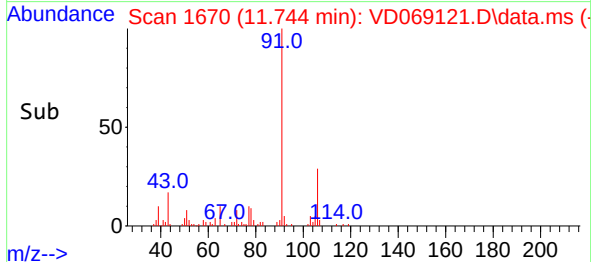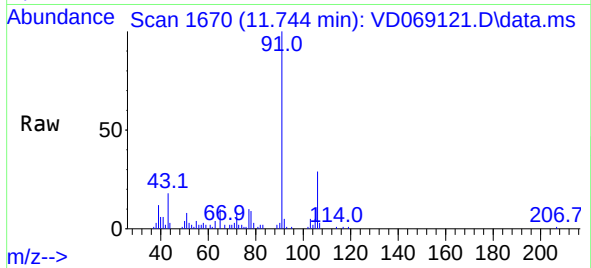

#68
m/p-Xylenes
Concen: 5.35 ug/l
RT: 11.849 min Scan# 1688
Delta R.T. -0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion:106 Resp: 21374
Ion Ratio Lower Upper
106 100
91 186.5 164.6 246.8


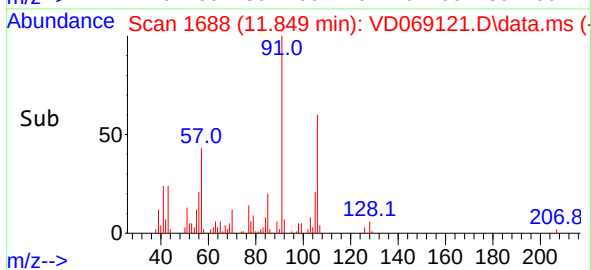






#69
o-Xylene
Concen: 3.51 ug/l
RT: 12.179 min Scan# 1744
Delta R.T. -0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20




Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE


Tgt Ion:106 Resp: 12591
Ion Ratio Lower Upper
106 100
91 199.3 107.1 321.4

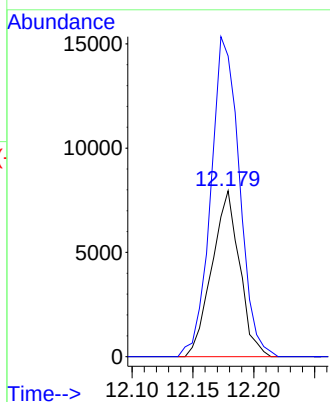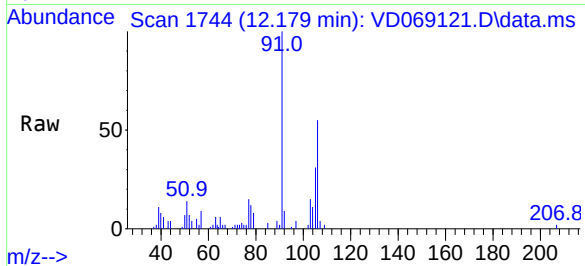

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. -0.006 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion:152 Resp: 57497
Ion Ratio Lower Upper
152 100
115 57.7 30.5 91.5
150 153.1 0.0 340.8


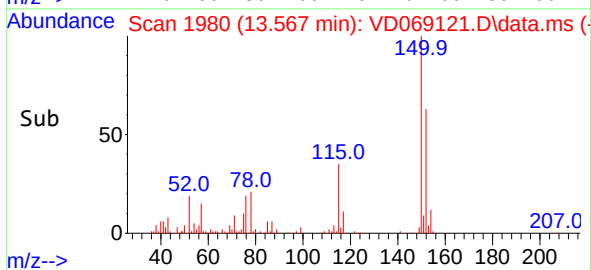

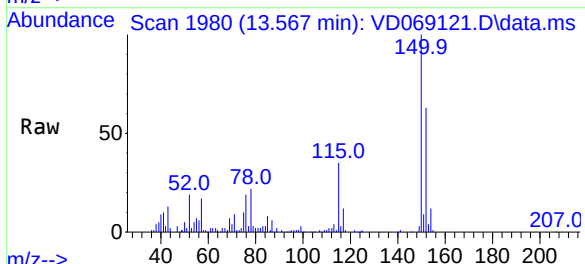




#73
Isopropylbenzene
Concen: 3.14 ug/l
RT: 12.473 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20




Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE


Tgt Ion:105 Resp: 12499
Ion Ratio Lower Upper
105 100
120 30.9 13.1 39.1

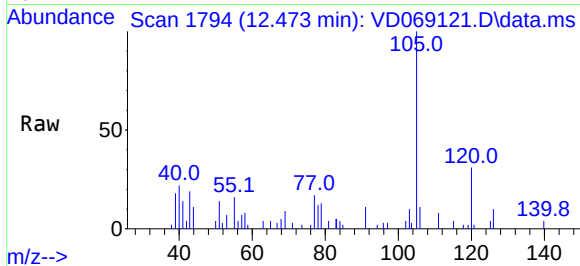

#74
N-ethyl acetate
Concen: 11.45 ug/l
RT: 12.249 min Scan# 1756
Delta R.T. -0.035 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion: 43 Resp: 9565
Ion Ratio Lower Upper
43 100
70 0.0 36.4 54.6#
55 7.6 21.8 32.8#
61 0.0 19.8 29.6#


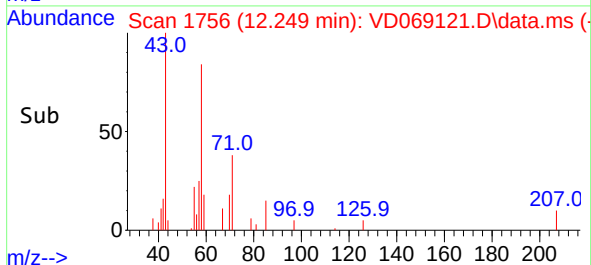
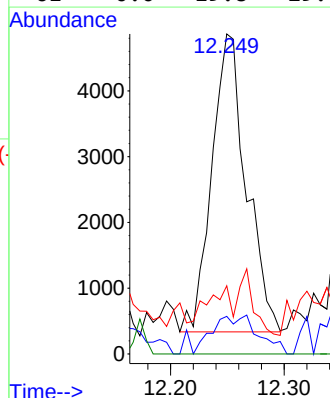
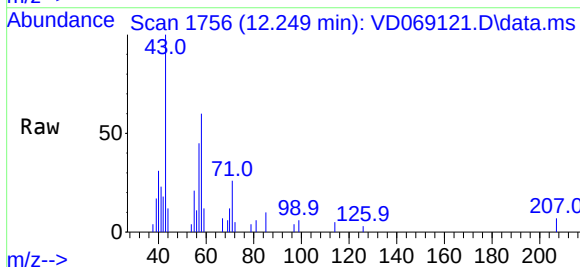




#76
1,2,3-Trichloropropane
Concen: 103.72 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. -0.147 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20




Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE


Tgt Ion: 75 Resp: 51916
Ion Ratio Lower Upper
75 100
77 2.5 0.0 0.0#

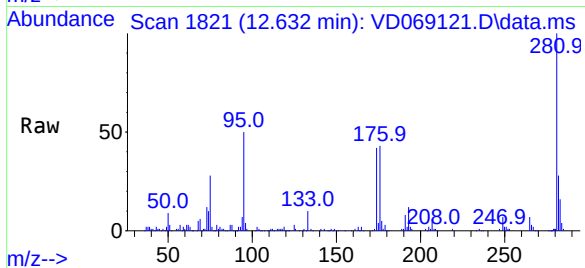

#78
n-propylbenzene
Concen: 5.28 ug/l
RT: 12.820 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion: 91 Resp: 25825
Ion Ratio Lower Upper
91 100
120 24.9 11.3 33.8


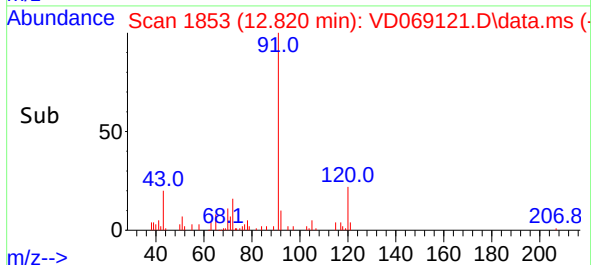

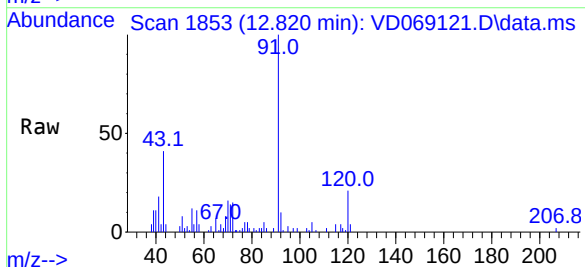




#80
1,3,5-Trimethylbenzene
Concen: 2.86 ug/l
RT: 12.955 min Scan# 1876
Delta R.T. -0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20




Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE


Tgt Ion:105 Resp: 9674
Ion Ratio Lower Upper
105 100
120 53.3 24.2 72.6

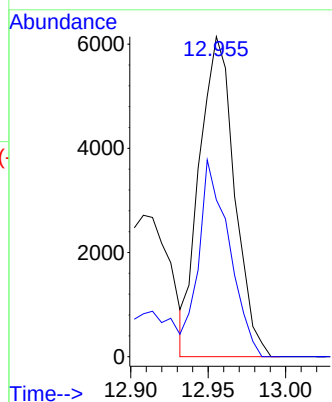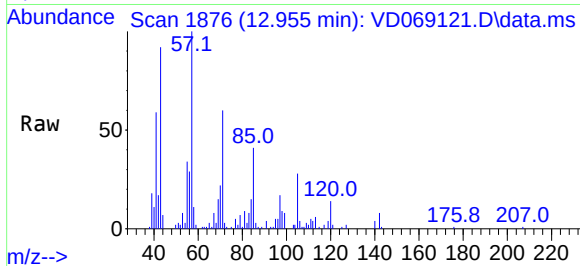

#81
trans-1,4-Dichloro-2-butene
Concen: 225.69 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.106 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion: 75 Resp: 51916
Ion Ratio Lower Upper
75 100
53 0.0 80.4 120.6#
89 2.7 37.8 56.8#


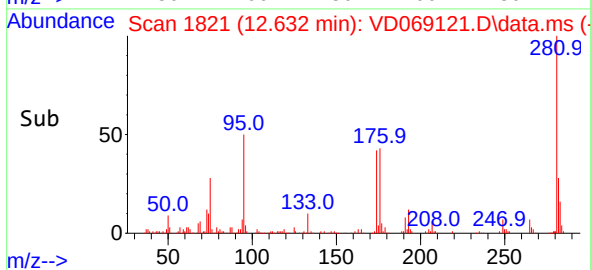

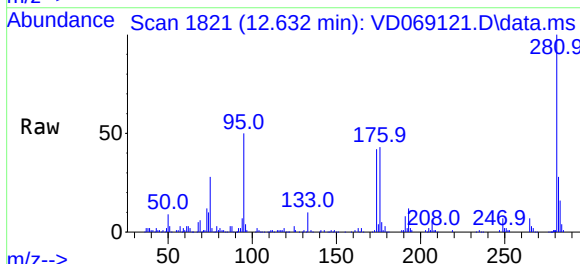


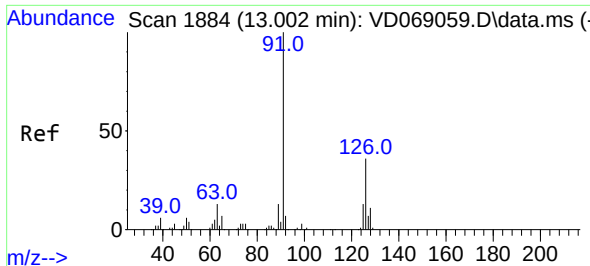

#82
4-Chlorotoluene
Concen: 8.85 ug/l
RT: 12.820 min Scan# 1853
Delta R.T. -0.182 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20




Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE


Tgt Ion: 91 Resp: 25825
Ion Ratio Lower Upper
91 100
126 0.0 17.3 51.7#

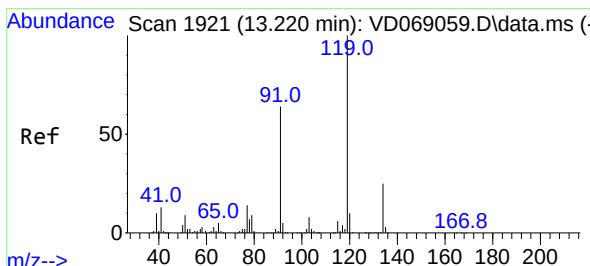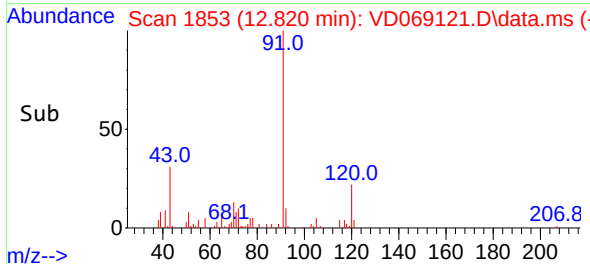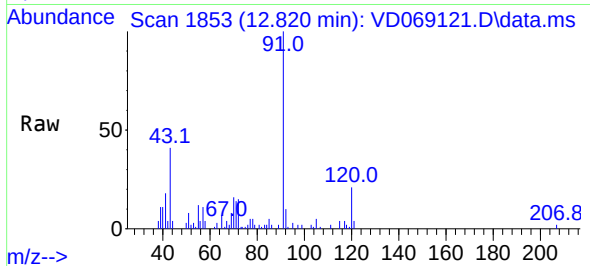

#83
tert-Butylbenzene
Concen: 75.00 ug/l
RT: 13.220 min Scan# 1921
Delta R.T. -0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion: 119 Resp: 207068
Ion Ratio Lower Upper
119 100
91 66.9 32.8 98.3
134 25.0 12.6 37.8


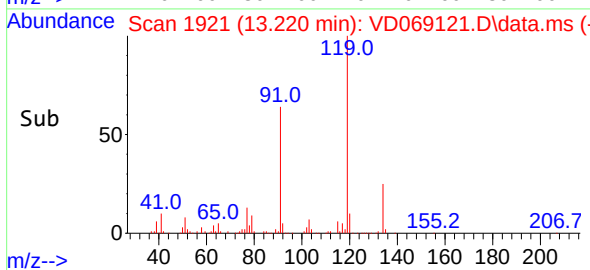

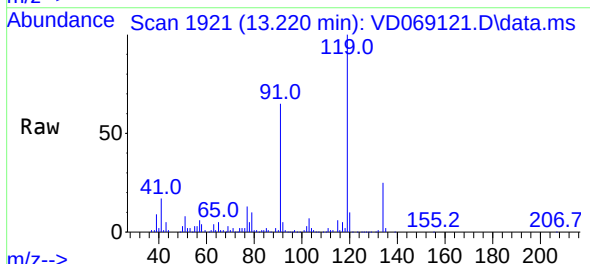




#84
1,2,4-Trimethylbenzene
Concen: 7.30 ug/l
RT: 13.261 min Scan# 1928
Delta R.T. -0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20




Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE


Tgt Ion:105 Resp: 24725
Ion Ratio Lower Upper
105 100
120 41.9 22.5 67.5

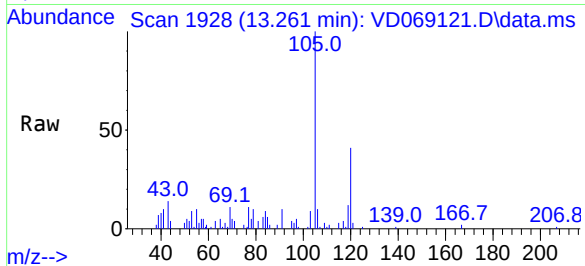

#85
sec-Butylbenzene
Concen: 2.76 ug/l
RT: 13.391 min Scan# 1950
Delta R.T. -0.006 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion:105 Resp: 11041
Ion Ratio Lower Upper
105 100
134 21.3 9.8 29.4


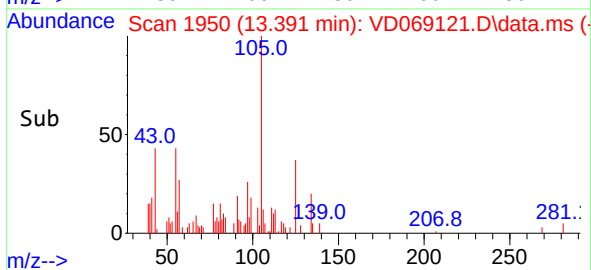

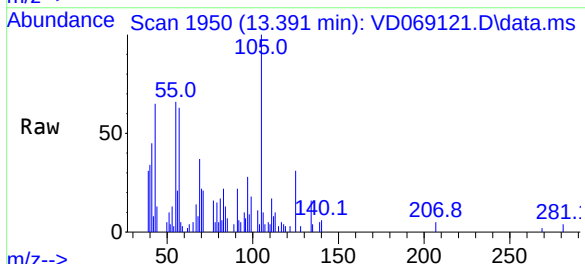


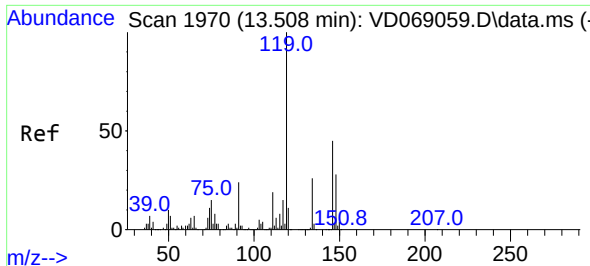

#86
p-Isopropyltoluene
Concen: 1.48 ug/l
RT: 13.508 min Scan# 1970
Delta R.T. -0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20




Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE


Tgt Ion:119 Resp: 5442
Ion Ratio Lower Upper
119 100
134 24.7 12.9 38.7
91 0.0 12.3 36.9#

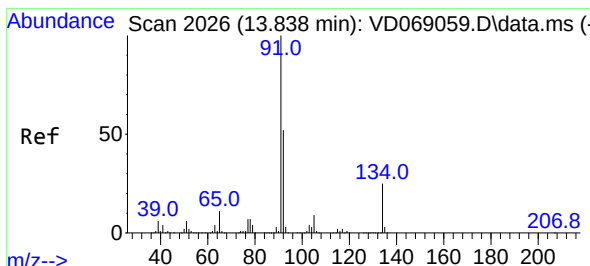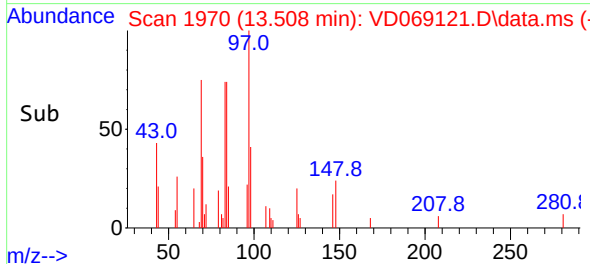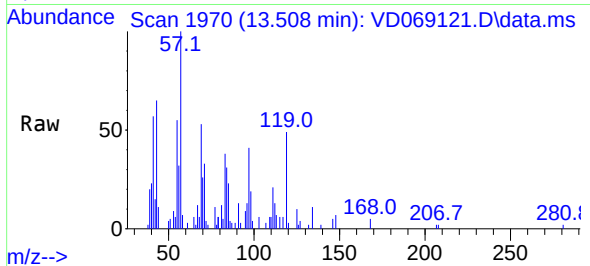

#89
n-Butylbenzene
Concen: 4.21 ug/l
RT: 13.838 min Scan# 2026
Delta R.T. -0.000 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion: 91 Resp: 14745
Ion Ratio Lower Upper
91 100
92 52.7 26.2 78.5
134 19.2 12.1 36.3


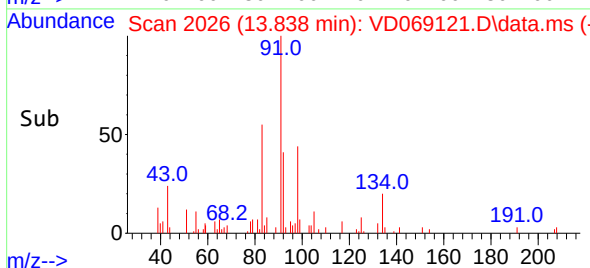
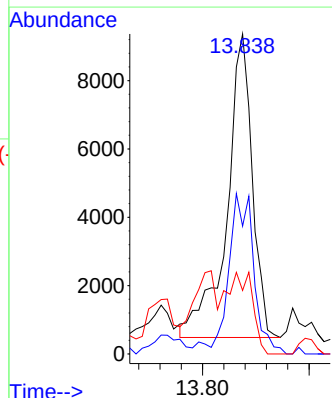
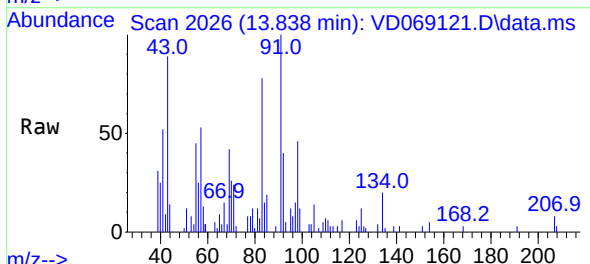


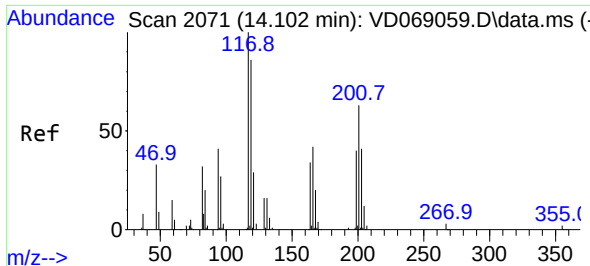

#90
Hexachloroethane
Concen: 3.42 ug/l
RT: 14.114 min Scan# 2073
Delta R.T. 0.012 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Instrument :
MSVOA_D
ClientSampleId :
CFOS-SOILRE

Tgt Ion:117 Resp: 2592
Ion Ratio Lower Upper
117 100
201 4.6 32.6 97.8#

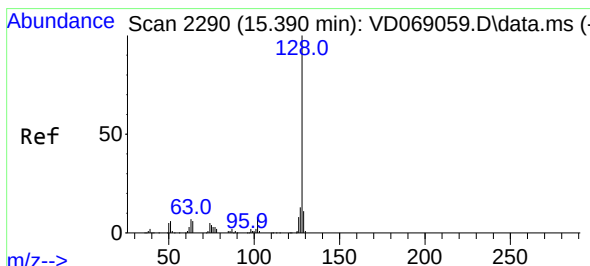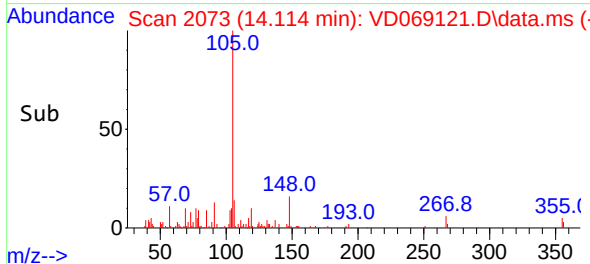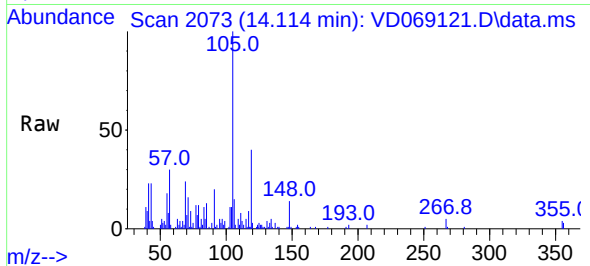

#95
Naphthalene
Concen: 5.98 ug/l
RT: 15.396 min Scan# 2291
Delta R.T. 0.006 min
Lab File: VD069121.D
Acq: 10 May 2021 14:20

Tgt Ion:128 Resp: 6529
Ion Ratio Lower Upper
128 100
127 0.0 10.7 16.1#
129 13.6 8.5 12.7#

