
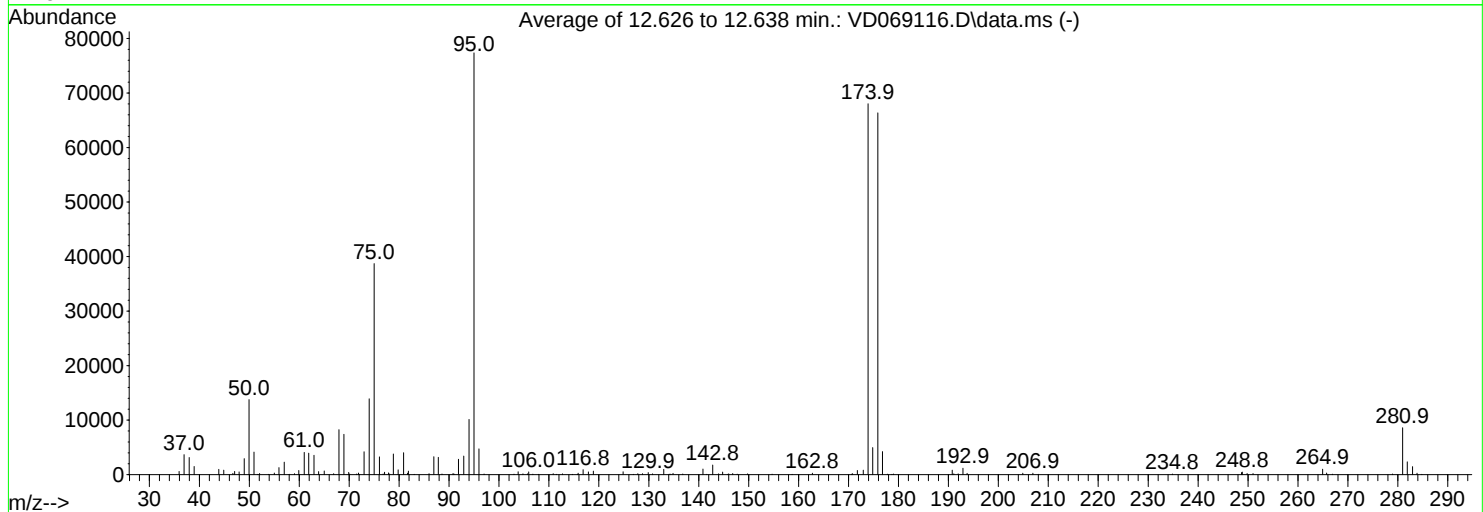


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051021\
Data File : VD069116.D
Acq On : 10 May 2021 10:49
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050421S.M
Title : SW846 8260
Last Update : Wed May 05 04:16:41 2021

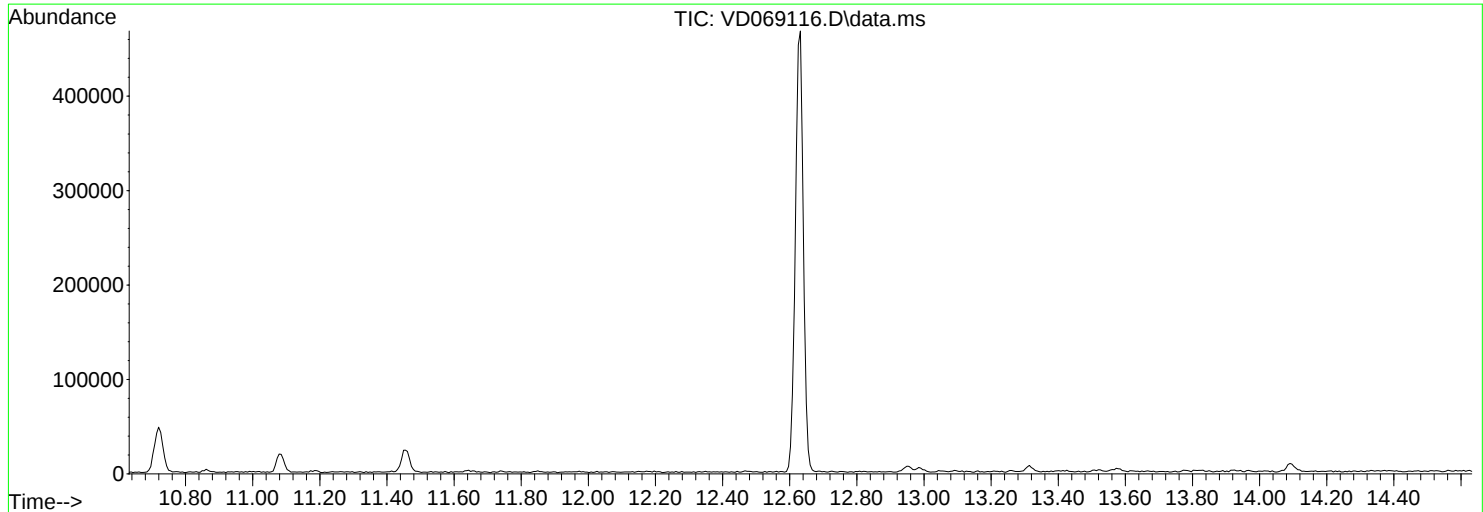

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	13755	PASS
75	95	30	60	50.0	38704	PASS
95	95	100	100	100.0	77368	PASS
96	95	5	9	6.1	4730	PASS
173	174	0.00	2	1.2	829	PASS
174	95	50	100	87.9	68016	PASS
175	174	5	9	7.3	4951	PASS
176	174	95	101	97.6	66355	PASS
177	176	5	9	6.4	4226	PASS