


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_D\DATA\VD051119\
Data File : VD062227.D
Acq On : 11 May 2019 9:34
Operator : FY/SY
Sample : BFB
Misc : 5.00g/5mL/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D050719S.M
Title : SW846 8260
Last Update : Tue May 07 14:26:29 2019

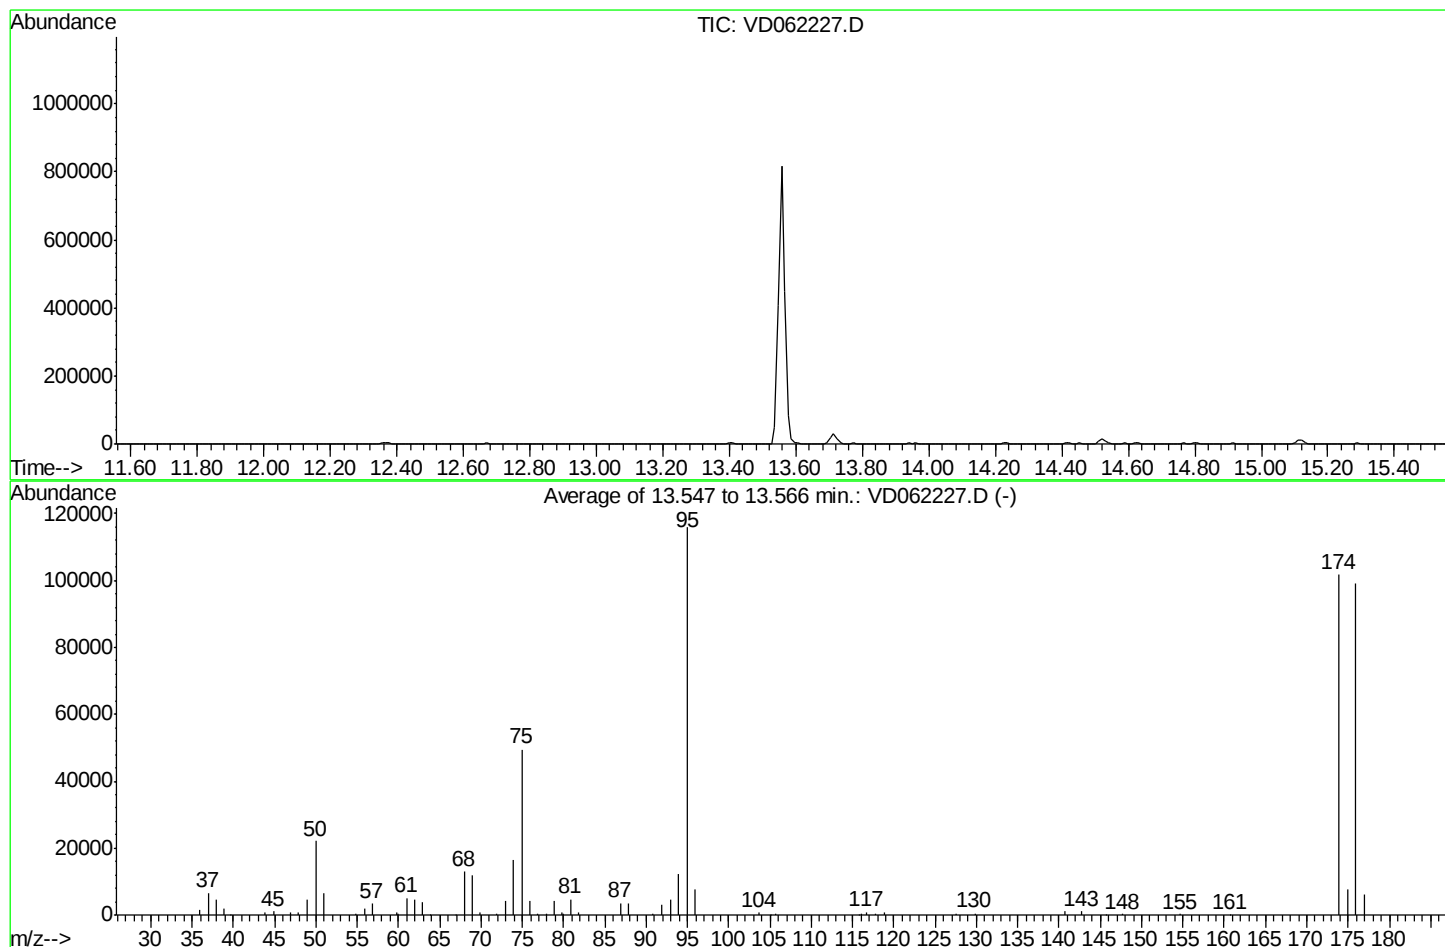

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	22073	PASS
75	95	30	60	42.7	49461	PASS
95	95	100	100	100.0	115901	PASS
96	95	5	9	6.6	7639	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.8	101736	PASS
175	174	5	9	7.7	7844	PASS
176	174	95	101	97.4	99125	PASS
177	176	5	9	6.2	6192	PASS