




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051123\
 Data File : VD076083.D
 Acq On : 11 May 2023 16:30
 Operator : KP/SY
 Sample : 02591-37
 Misc : 6.04G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 JREA8

Manual IntegrationsAPPROVED

Quant Time: May 12 03:05:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 12 02:22:21 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 05/12/2023
 Supervised By :Mahesh Dadoda 05/12/2023

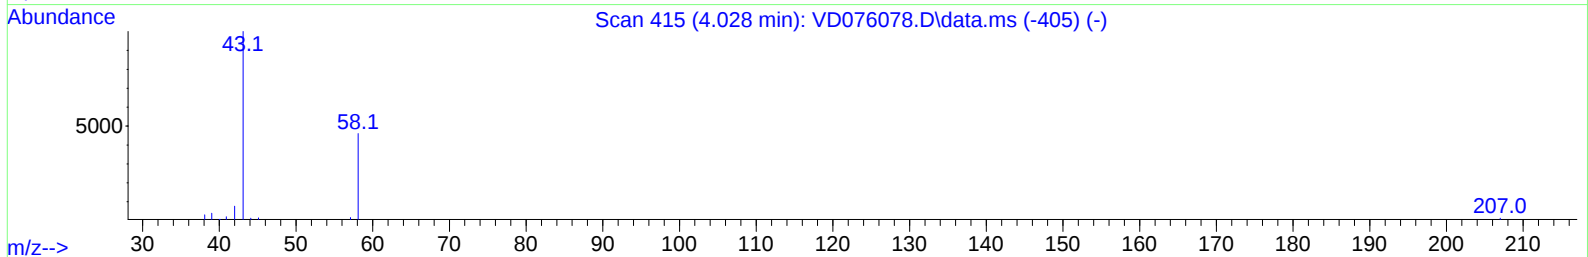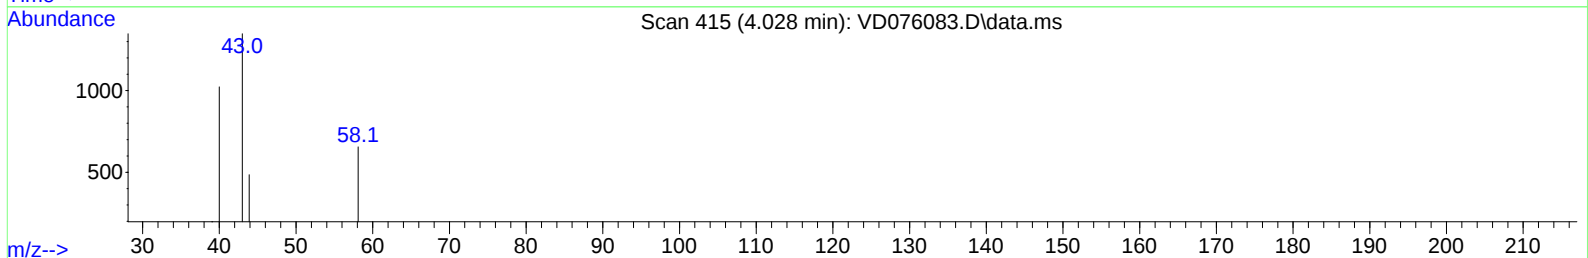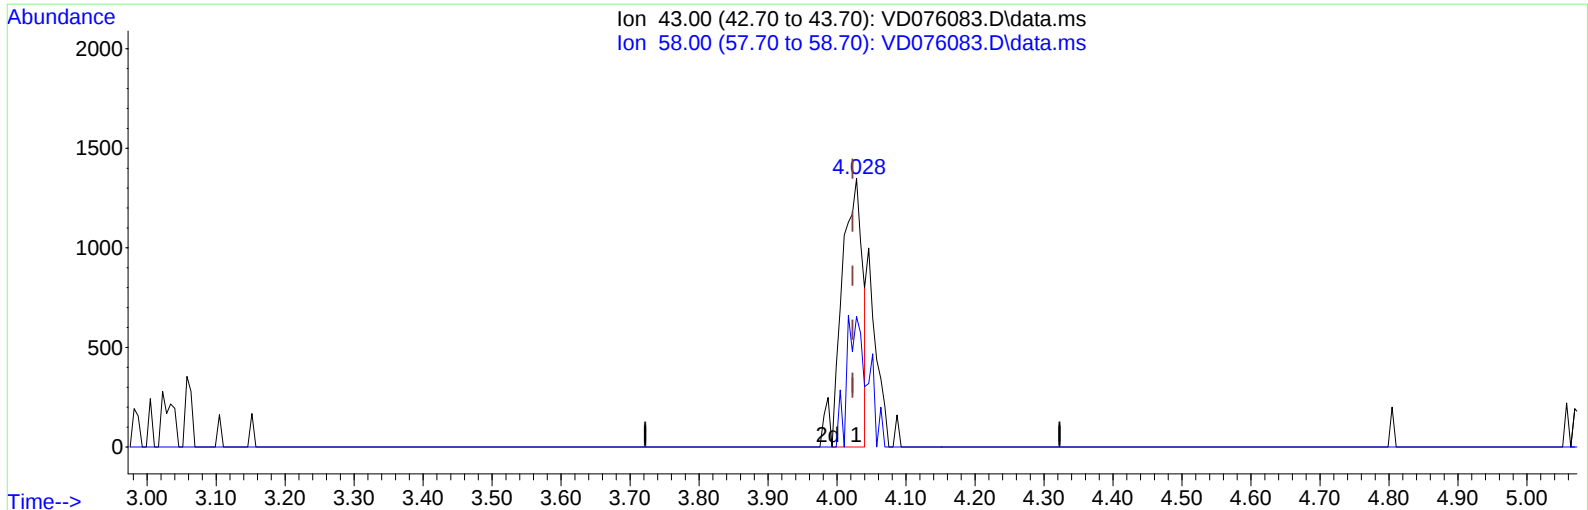

TIC: VD076083.D\data.ms

(13) Acetone (T)

4.028min (+ 0.006) 4.17 ug/L

response 2697

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	20.02
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051123\
Data File : VD076083.D
Acq On : 11 May 2023 16:30
Operator : KP/SY
Sample : 02591-37
Misc : 6.04G/10.00ml/MSVOA_D/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
JREA8

Manual IntegrationsAPPROVED

Quant Time: May 12 03:05:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 12 02:22:21 2023
Response via : Initial Calibration

Reviewed By :John Carlone 05/12/2023
Supervised By :Mahesh Dadoda 05/12/2023

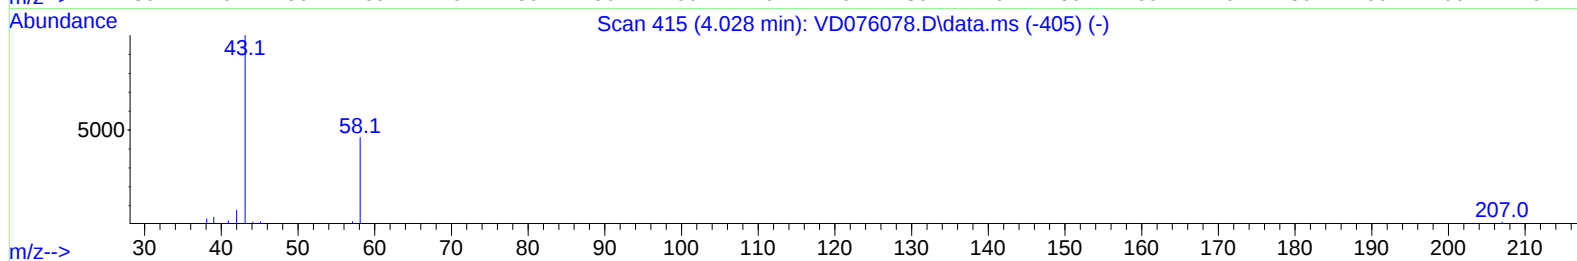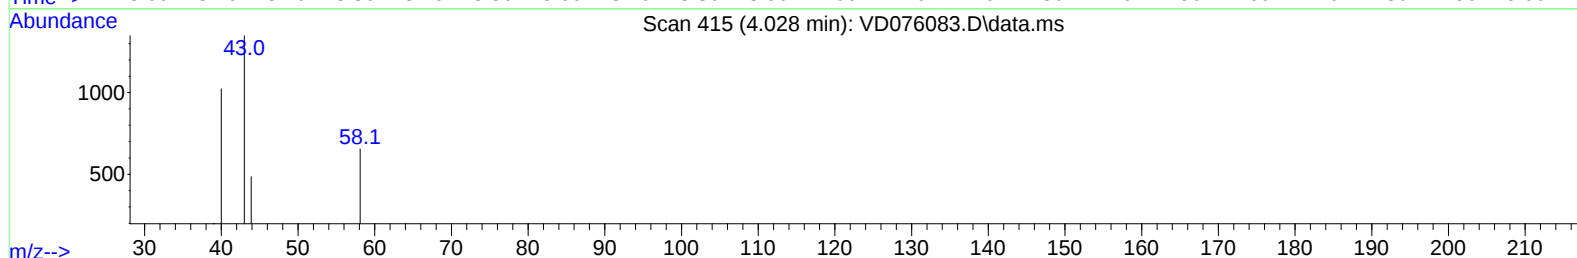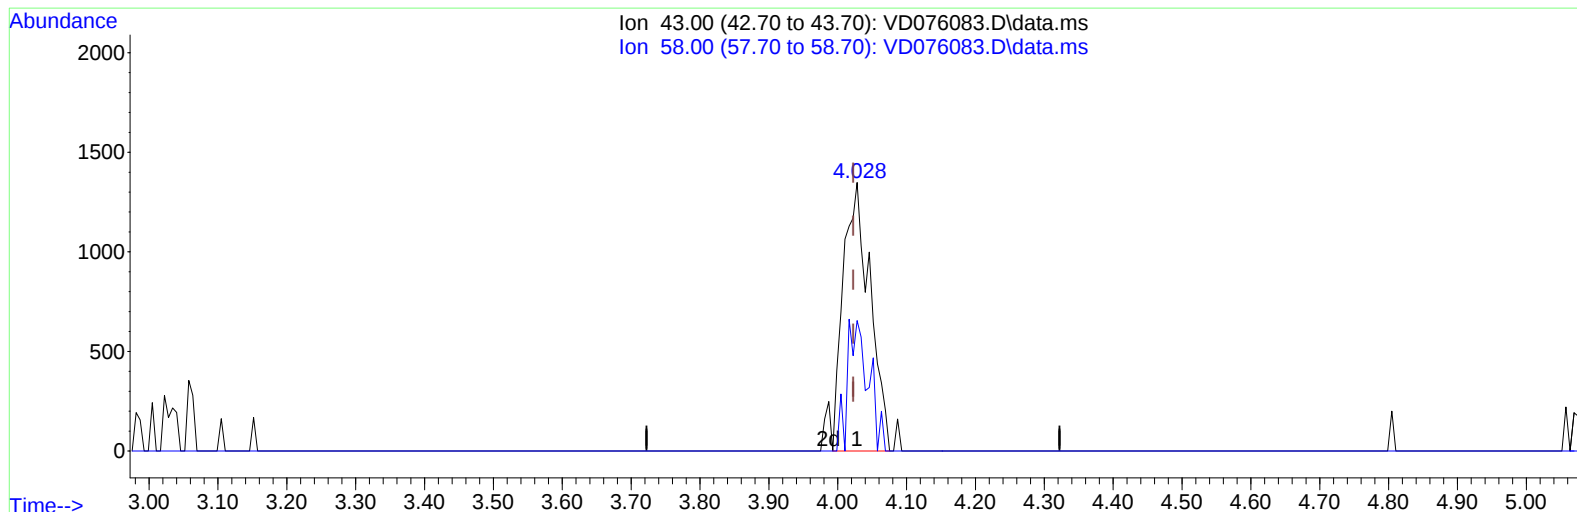

TIC: VD076083.D\data.ms

(13) Acetone (T)

4.028min (+ 0.006) 5.61 ug/L m

response 3626

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	14.89
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051123\
 Data File : VD076083.D
 Acq On : 11 May 2023 16:30
 Operator : KP/SY
 Sample : 02591-37
 Misc : 6.04G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 JREA8

Manual IntegrationsAPPROVED

Quant Time: May 12 03:05:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 12 02:22:21 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 05/12/2023
 Supervised By :Mahesh Dadoda 05/12/2023

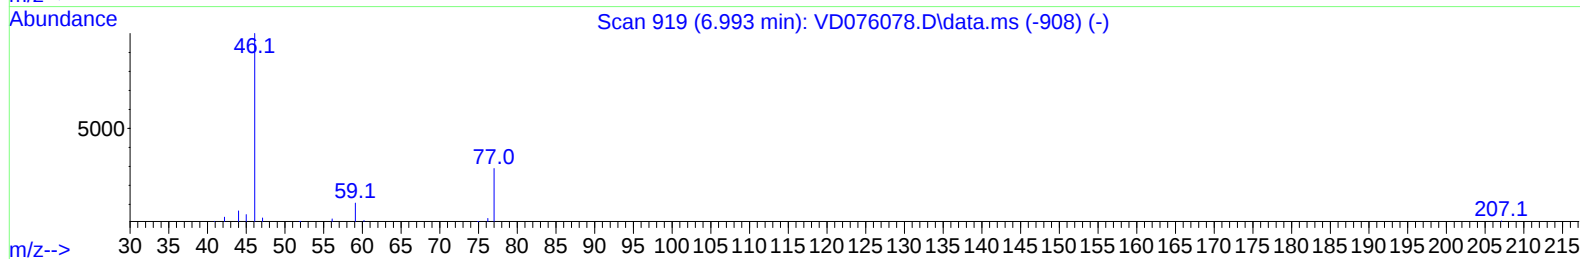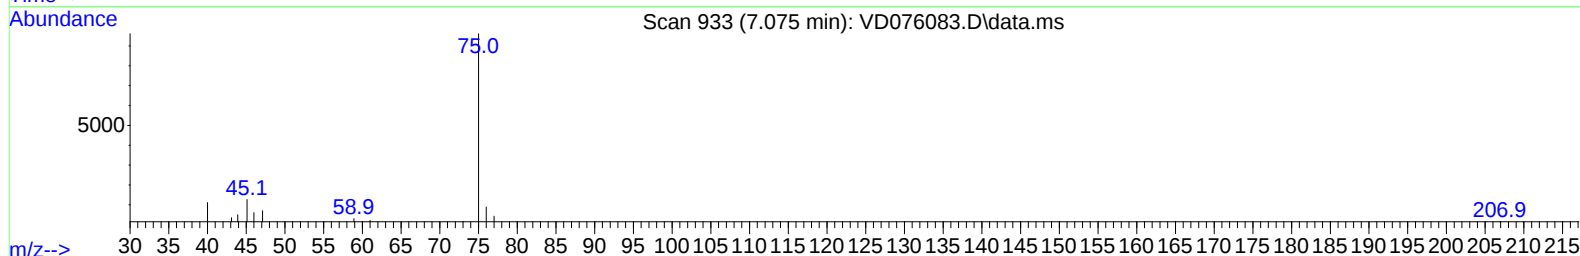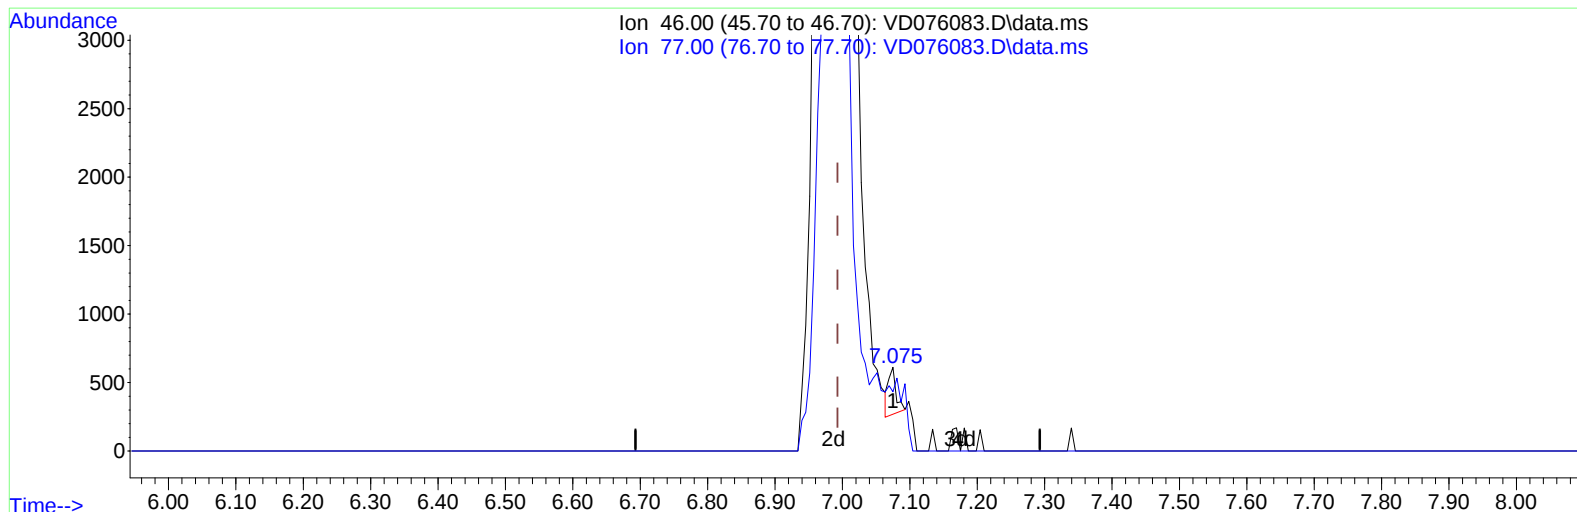

TIC: VD076083.D\data.ms

(21) 2-Butanone-d5 (S)

7.075min (+ 0.082) 0.38 ug/L

response 276

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	33.50	31.88
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051123\
 Data File : VD076083.D
 Acq On : 11 May 2023 16:30
 Operator : KP/SY
 Sample : 02591-37
 Misc : 6.04G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 JREA8

Manual IntegrationsAPPROVED

Quant Time: May 12 03:05:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 12 02:22:21 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 05/12/2023
 Supervised By :Mahesh Dadoda 05/12/2023

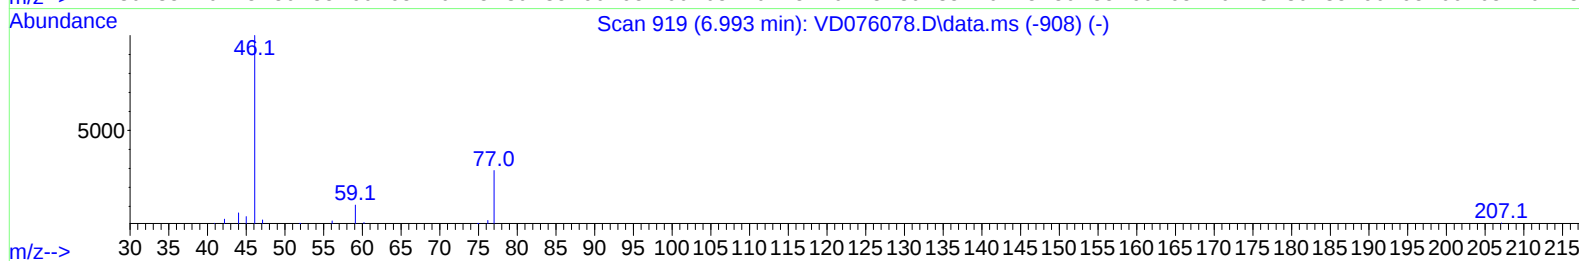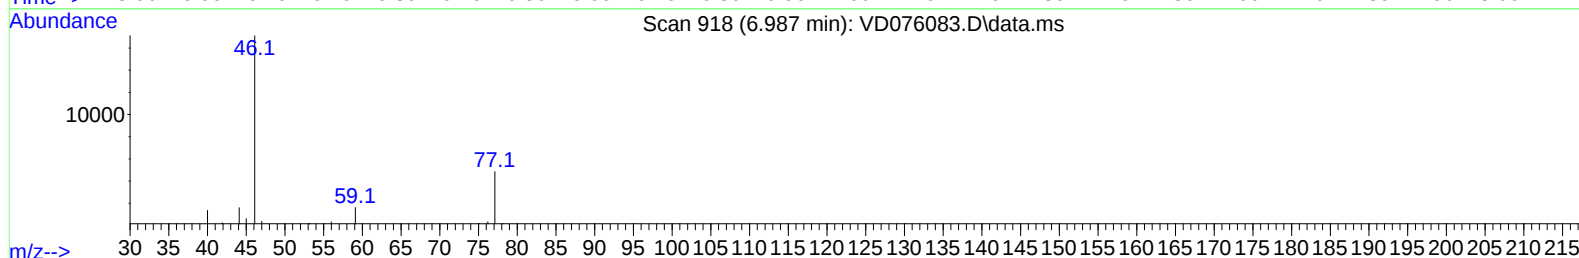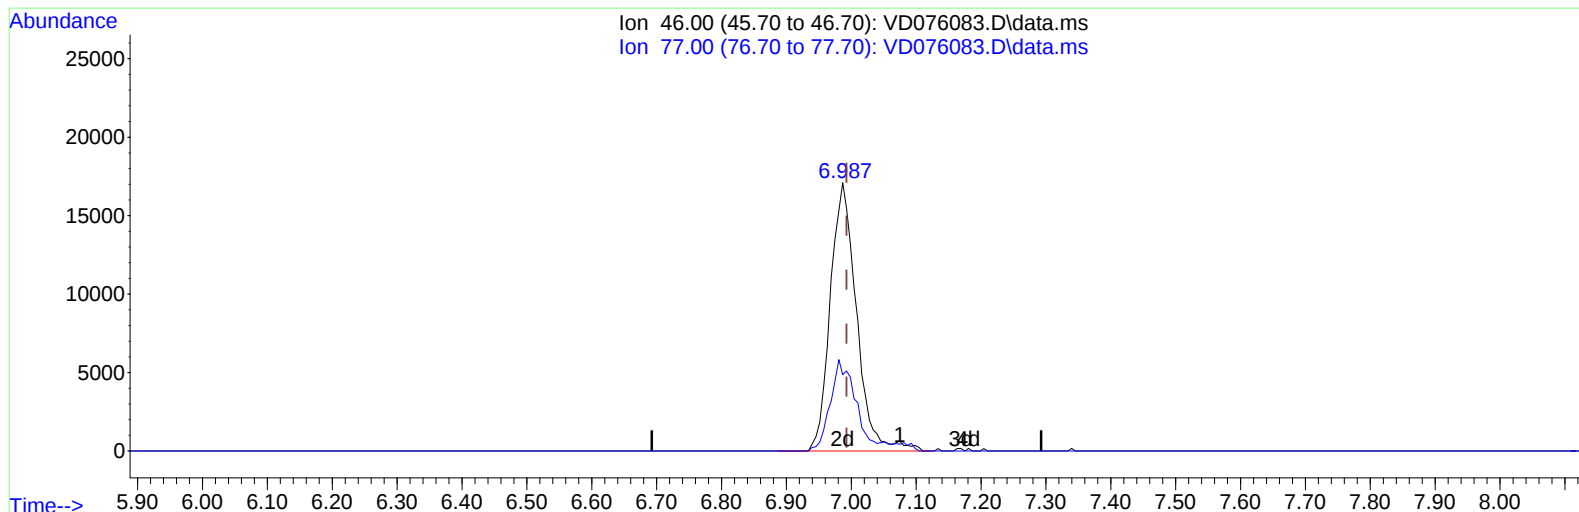

TIC: VD076083.D\data.ms

(21) 2-Butanone-d5 (S)

6.987min (-0.006) 66.12 ug/L m

response 47991

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	33.50	0.18#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051123\
 Data File : VD076083.D
 Acq On : 11 May 2023 16:30
 Operator : KP/SY
 Sample : 02591-37
 Misc : 6.04G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 JREA8

Manual IntegrationsAPPROVED

Quant Time: May 12 03:05:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 12 02:22:21 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 05/12/2023
 Supervised By :Mahesh Dadoda 05/12/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	352369	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	217492	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	42582	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.269	65	80144	14.868	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	59.480%		
7) Chloroethane-d5	2.793	69	87671	17.716	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	70.880%		
11) 1,1-Dichloroethene-d2	3.910	65	18788	13.845	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	55.400%		
21) 2-Butanone-d5	6.987	46	47991m	66.124	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	132.240%		
24) Chloroform-d	7.569	84	154595	20.942	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	83.760%		
26) 1,2-Dichloroethane-d4	8.228	65	71932	22.167	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	88.680%		
32) Benzene-d6	8.198	84	240334	24.510	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	98.040%		
36) 1,2-Dichloropropane-d6	9.210	67	93385	30.908	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	123.640%#		
41) Toluene-d8	10.269	98	151795	17.371	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	69.480%		
43) trans-1,3-Dichloroprop...	10.528	79	28853	25.440	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	101.760%		
47) 2-Hexanone-d5	10.881	63	33904	76.628	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	153.260%#		
56) 1,1,2,2-Tetrachloroeth...	12.651	84	69054	26.540	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	106.160%		
66) 1,2-Dichlorobenzene-d4	13.816	152	25302	20.800	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	83.200%		
Target Compounds						Qvalue
13) Acetone	4.028	43	3626m	5.608	ug/L	
16) Methylene chloride	4.793	84	30947	5.401	ug/L	98
42) Toluene	10.334	91	8962	0.694	ug/L	85
53) m,p-Xylene	11.787	106	3132	0.600	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051123\
Data File : VD076083.D
Acq On : 11 May 2023 16:30
Operator : KP/SY
Sample : 02591-37
Misc : 6.04G/10.00ml/MSVOA_D/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
JREA8

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 05/12/2023
Supervised By :Mahesh Dadoda 05/12/2023

Quant Time: May 12 03:05:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 12 02:22:21 2023
Response via : Initial Calibration

