

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051123\
 Data File : VD076090.D
 Acq On : 11 May 2023 20:02
 Operator : KP/SY
 Sample : 02591-24
 Misc : 4.16G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 JREB4

Quant Time: May 12 03:06:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 12 02:22:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	679389	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	576273	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	189708	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.269	65	103525	9.961	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	39.840%
7) Chloroethane-d5	2.793	69	116743	12.235	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	48.960%
11) 1,1-Dichloroethene-d2	3.905	65	26201	10.014	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	40.040%#
21) 2-Butanone-d5	6.981	46	68017	48.607	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.220%
24) Chloroform-d	7.563	84	234871	16.501	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	66.000%
26) 1,2-Dichloroethane-d4	8.228	65	108713	17.376	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	69.520%#
32) Benzene-d6	8.199	84	369466	14.221	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	56.880%
36) 1,2-Dichloropropane-d6	9.210	67	150008	18.738	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	74.960%
41) Toluene-d8	10.269	98	296600	12.810	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	51.240%
43) trans-1,3-Dichloroprop...	10.522	79	45250	15.058	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	60.240%
47) 2-Hexanone-d5	10.875	63	46525	39.686	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.380%
56) 1,1,2,2-Tetrachloroeth...	12.651	84	155525	22.560	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.240%
66) 1,2-Dichlorobenzene-d4	13.816	152	106500	19.652	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	78.600%
Target Compounds						
16) Methylene chloride	4.799	84	28062	2.540	ug/L	Qvalue 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051123\
Data File : VD076090.D
Acq On : 11 May 2023 20:02
Operator : KP/SY
Sample : 02591-24
Misc : 4.16G/10.00ml/MSVOA_D/SOIL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
JREB4

Quant Time: May 12 03:06:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 12 02:22:21 2023
Response via : Initial Calibration

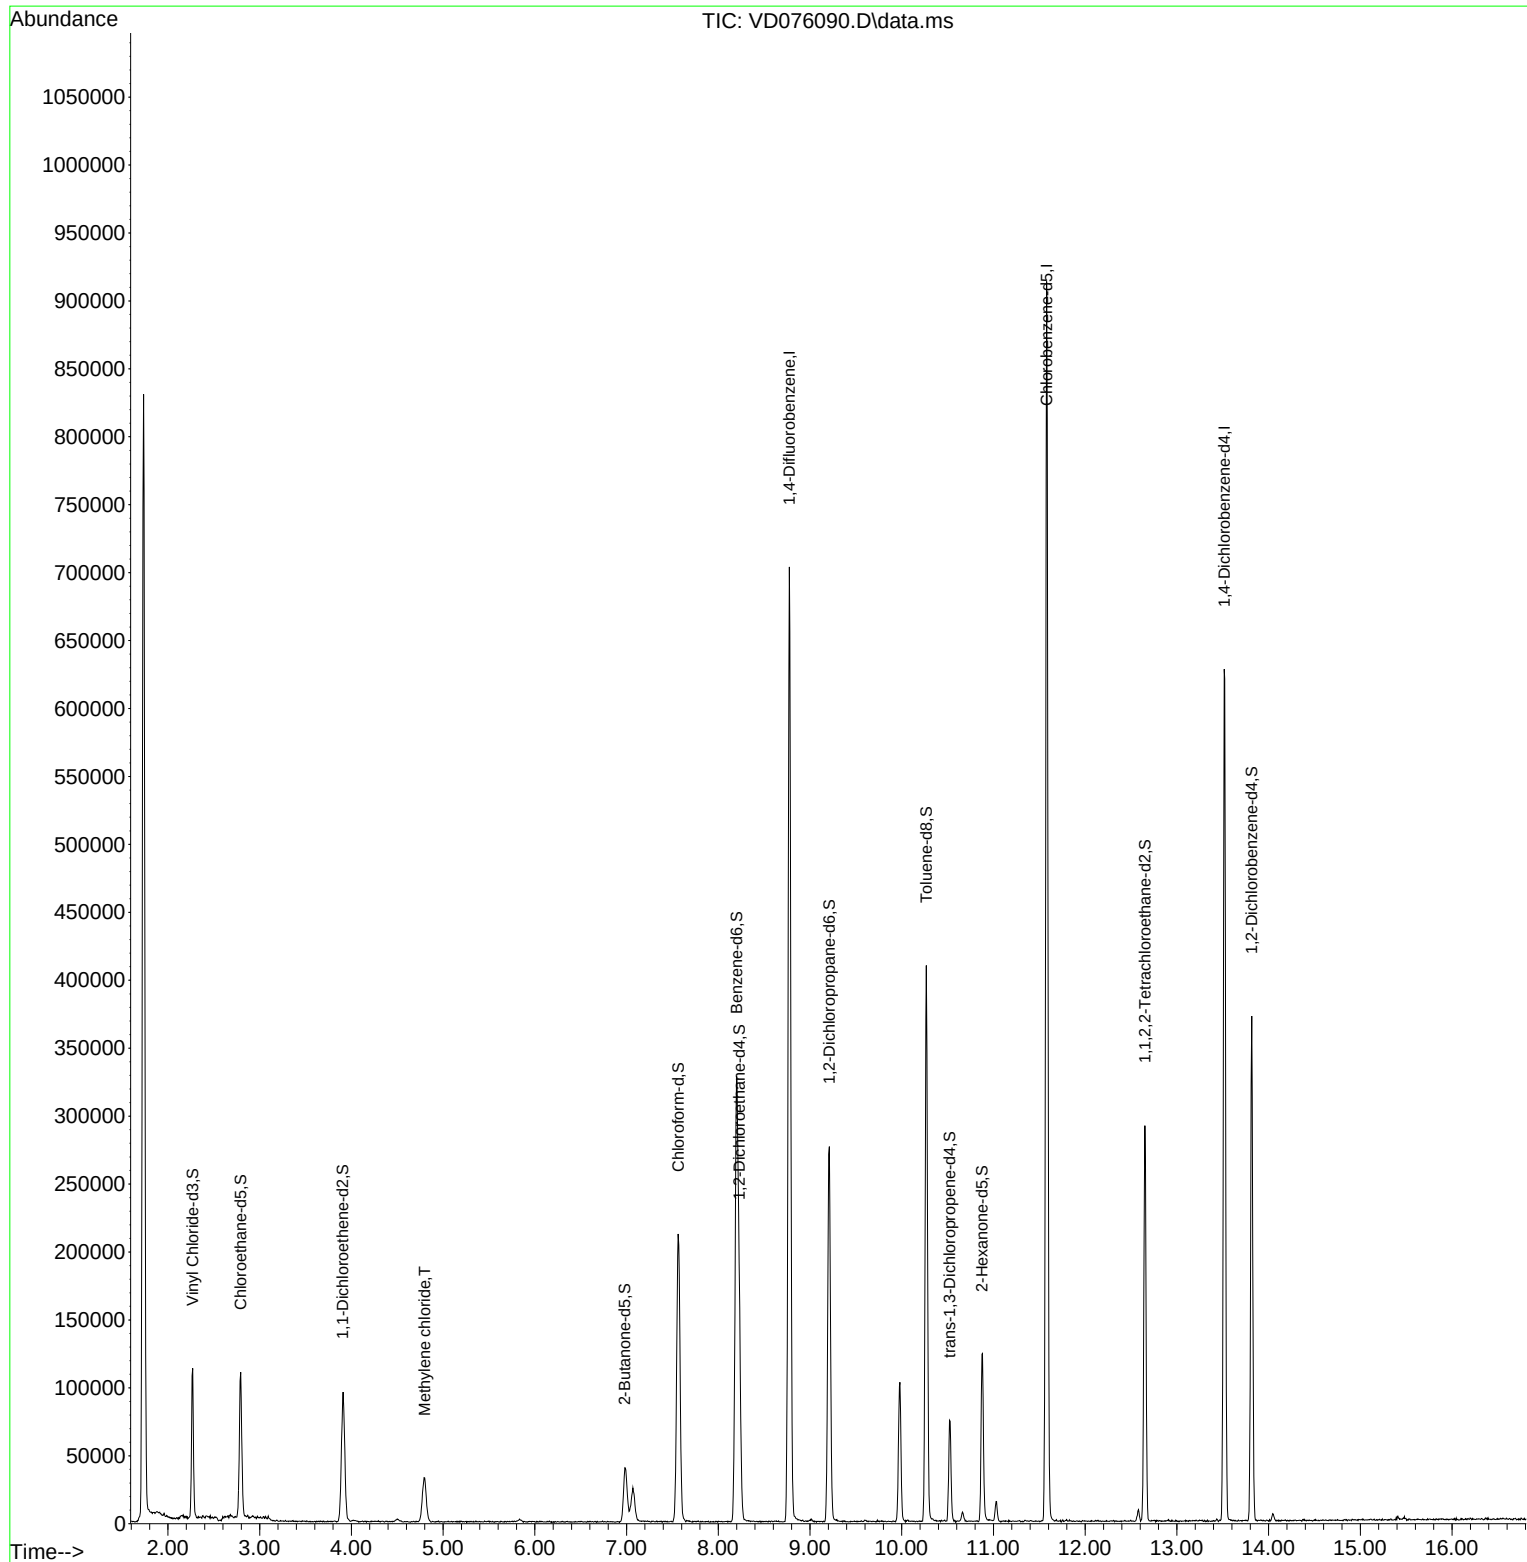

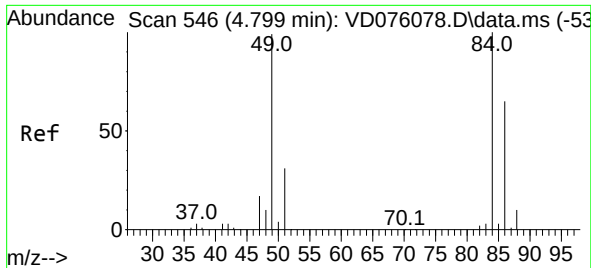

#16
Methylene chloride
Concen: 2.540 ug/L
RT: 4.799 min Scan# 54
Delta R.T. 0.000 min
Lab File: VD076090.D
Acq: 11 May 2023 20:02

Instrument :
MSVOA_D
ClientSampleId :
JREB4

Tgt Ion: 84 Resp: 28062
Ion Ratio Lower Upper
84 100
86 57.7 45.8 85.2
49 107.4 60.8 112.8

