
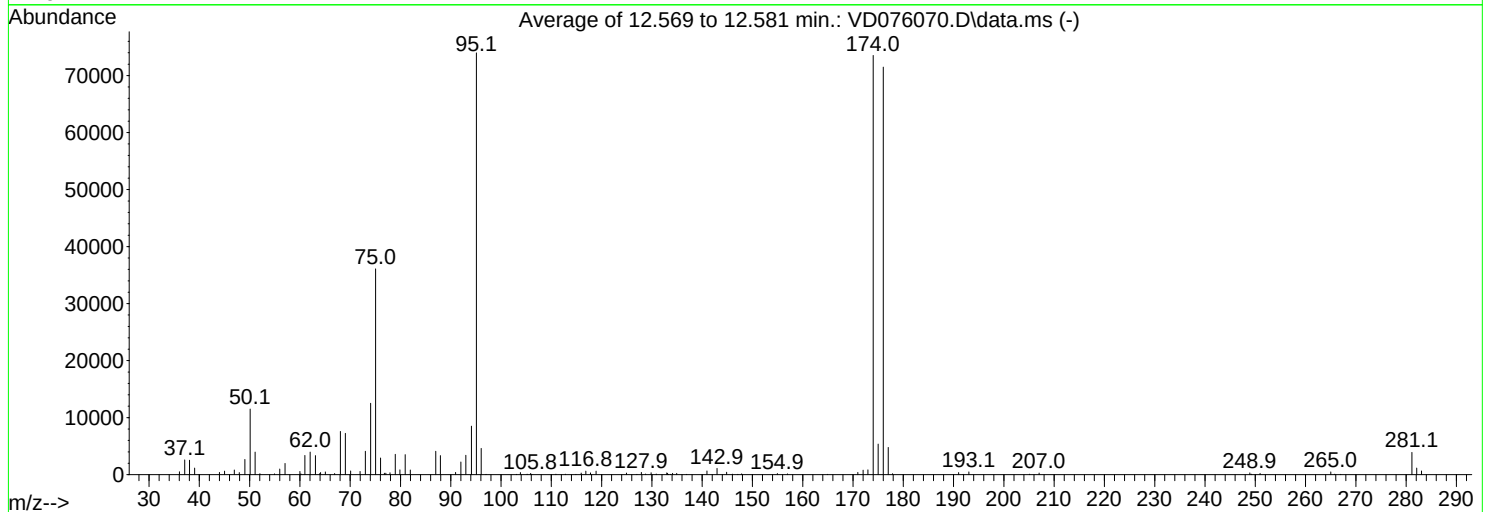


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051123\
Data File : VD076070.D
Acq On : 11 May 2023 09:33
Operator : KP/SY
Sample : BFB131
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB131

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051123SMA.M
Title : SFAM01.0
Last Update : Sun May 14 23:54:23 2023

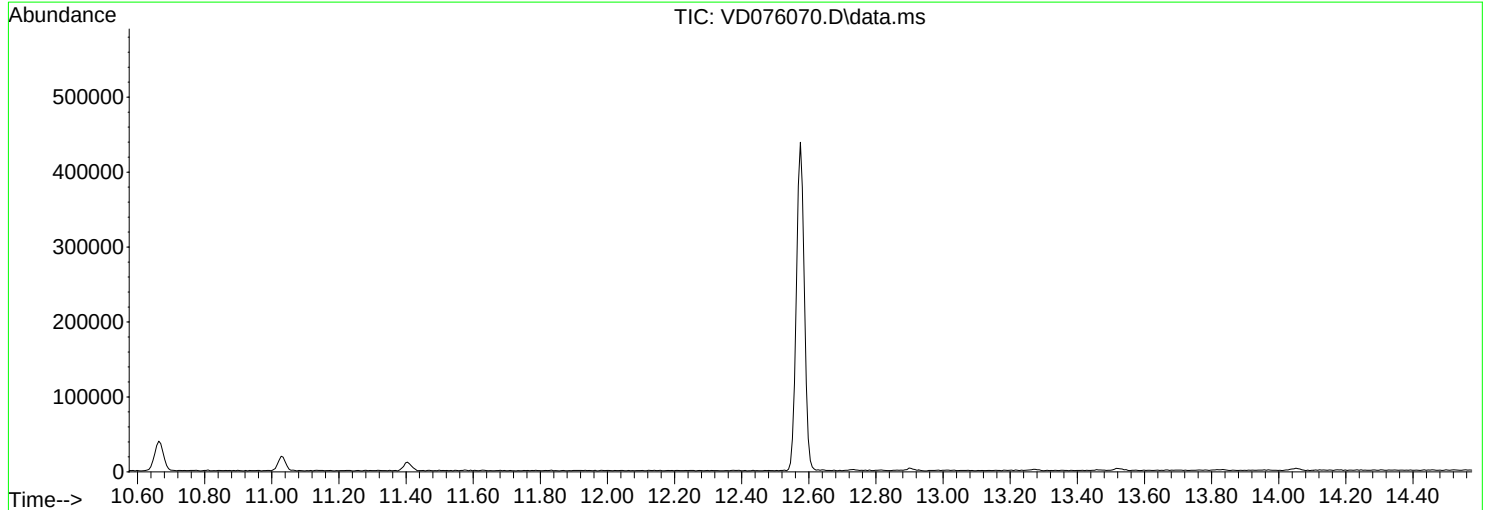

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	11520	PASS
75	95	30	80	48.8	36107	PASS
95	95	100	100	100.0	73987	PASS
96	95	5	9	6.2	4601	PASS
173	174	0.00	2	1.1	833	PASS
174	95	50	120	99.4	73547	PASS
175	174	5	9	7.3	5368	PASS
176	174	95	105	97.2	71475	PASS
177	176	5	10	6.7	4773	PASS

Scan 1859 (12.522 min): VD076070.D\data.ms
BFB131

m/z	Abundance
40.10	1194.0
44.10	572.0
207.00	190.0

Instrument :
MSVOA_D
ClientSampleId :
BFB131

m/z	Abundance
36.10	585.0
37.10	2406.0
38.10	2308.0
39.10	1223.0
40.10	1332.0
44.00	889.0
45.00	610.0
46.90	805.0
48.00	402.0
49.10	3010.0
50.10	10848.0
51.10	3796.0
52.00	213.0
55.00	153.0
56.00	885.0
57.00	1791.0
60.00	794.0
61.00	3442.0
62.00	4016.0
63.10	3643.0
63.90	489.0
65.00	368.0
68.10	7485.0
69.10	7233.0
70.10	695.0
72.00	589.0
73.00	3848.0
74.00	11718.0
75.00	34472.0
76.00	2998.0
77.20	438.0
78.00	387.0
78.90	3730.0
79.90	1023.0
81.00	3347.0
82.00	990.0
87.00	3798.0
88.00	3046.0
91.00	299.0
92.00	2175.0
93.00	3419.0
94.10	7797.0
95.10	71760.0
96.00	4714.0
103.90	358.0
105.20	263.0
106.10	267.0
116.00	259.0
116.90	464.0
117.80	257.0
118.90	602.0
124.90	185.0
127.00	154.0
128.00	454.0
128.80	185.0
129.80	333.0
132.90	245.0
133.30	181.0
133.70	194.0
134.90	227.0
141.00	581.0
142.90	937.0
144.80	393.0
157.00	197.0
170.90	438.0
172.00	634.0
173.00	864.0
174.00	68984.0
175.00	5210.0
176.00	67192.0
177.00	4569.0
177.80	242.0
191.10	411.0
193.10	216.0
207.00	564.0
249.20	271.0
251.00	160.0
265.10	367.0
267.00	210.0
281.10	3194.0
282.10	916.0
283.00	647.0

Instrument :
MSVOA_D
ClientSampleId :
BFB131

m/z	Abundance
36.10	469.0
37.10	2884.0
38.00	2721.0
39.00	1250.0
39.90	1318.0
44.00	1047.0
45.00	754.0
47.00	916.0
48.00	227.0
49.00	2867.0
50.10	12539.0
51.10	4212.0
52.10	316.0
54.90	232.0
56.00	1036.0
57.10	1968.0
60.00	907.0
61.00	3688.0
62.00	4460.0
63.10	3613.0
64.10	622.0
65.10	692.0
66.90	308.0
68.00	8107.0
69.00	8336.0
70.10	717.0
72.00	620.0
73.00	4532.0
74.10	13548.0
75.10	40888.0
76.00	2993.0
76.80	762.0
77.80	429.0
79.00	3823.0
79.90	720.0
80.90	4250.0
81.90	741.0
87.00	4335.0
87.90	3515.0
91.00	624.0
92.00	2458.0
93.00	3225.0
94.10	8779.0
95.10	81472.0
96.10	5123.0
103.10	165.0
103.80	445.0
105.80	312.0
110.90	286.0
112.80	222.0
115.80	293.0
116.80	748.0
117.80	311.0
118.90	785.0
125.00	355.0
127.80	381.0
128.70	177.0
129.90	388.0
130.80	193.0
133.00	679.0
134.20	368.0
135.00	259.0
140.90	799.0
143.00	1290.0
144.90	554.0
147.10	162.0
147.90	246.0
155.00	305.0
156.90	211.0
171.00	383.0
172.00	1035.0
173.00	774.0
174.00	81072.0
175.00	5963.0
176.00	78184.0
177.00	5394.0
190.90	400.0
191.90	175.0
193.00	788.0
207.00	428.0
248.90	188.0
251.00	265.0
265.00	267.0
281.10	3931.0
282.10	1006.0
283.10	680.0

Instrument :
MSVOA_D
ClientSampleId :
BFB131

m/z	Abundance
35.90	452.0
37.10	2482.0
38.00	2540.0
39.10	984.0
39.90	1037.0
44.00	976.0
45.00	470.0
47.00	699.0
47.90	482.0
49.10	2144.0
50.10	11172.0
51.10	3858.0
56.00	1070.0
57.10	2100.0
60.20	417.0
61.00	2978.0
62.10	3433.0
63.10	2769.0
64.10	484.0
65.10	415.0
66.90	290.0
68.00	7154.0
69.00	6177.0
70.10	508.0
71.90	453.0
73.00	3931.0
74.10	12276.0
75.00	32960.0
76.10	2743.0
77.00	331.0
77.80	210.0
78.90	3160.0
79.90	834.0
80.90	2910.0
82.00	706.0
87.00	4174.0
87.90	3503.0
90.80	259.0
92.00	1998.0
93.00	3568.0
94.10	8951.0
95.10	68728.0
96.10	3967.0
97.00	189.0
103.90	310.0
105.90	274.0
114.90	154.0
116.00	269.0
116.90	671.0
117.80	344.0
118.90	443.0
125.00	298.0
127.90	328.0
129.90	287.0
130.90	167.0
133.10	676.0
134.00	273.0
135.00	164.0
136.90	182.0
141.00	564.0
142.90	1030.0
144.90	340.0
146.00	247.0
147.80	207.0
154.90	260.0
164.90	155.0
170.90	330.0
172.00	658.0
172.90	862.0
174.00	70584.0
175.00	4932.0
176.00	69048.0
177.00	4355.0
177.90	274.0
191.00	279.0
193.10	407.0
205.10	272.0
207.00	405.0
248.90	733.0
250.90	270.0
265.00	773.0
265.80	215.0
281.20	4618.0
282.10	1541.0
283.10	661.0

Instrument :
MSVOA_D
ClientSampleId :
BFB131