


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD051219\
 Data File : VD062251.D
 Acq On : 12 May 2019 9:43
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D050719S.M
 Title : SW846 8260
 Last Update : Tue May 07 14:26:29 2019

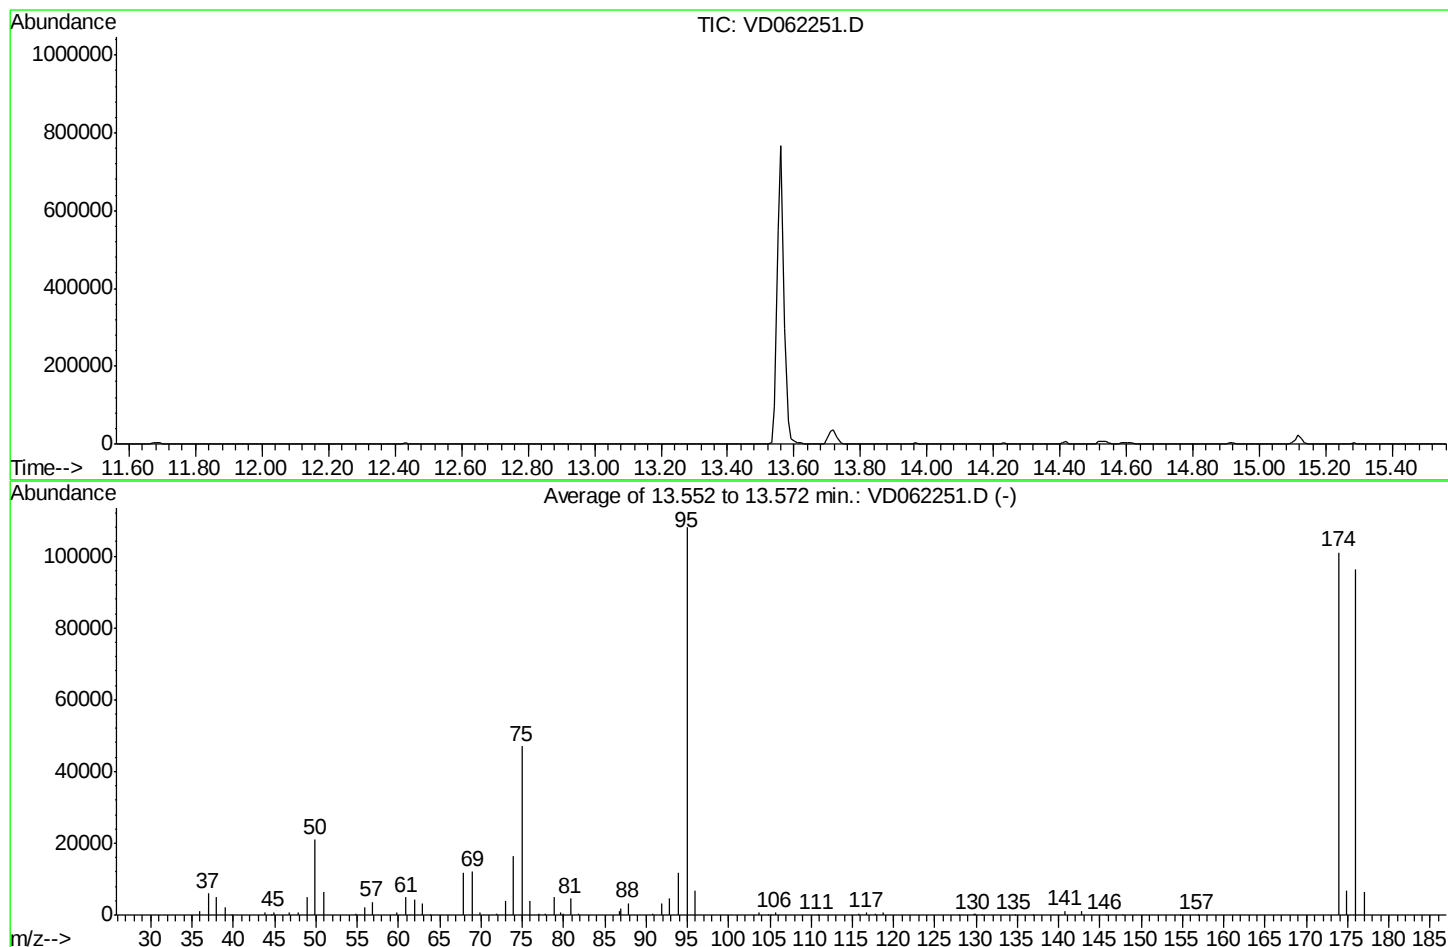

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	20954	PASS
75	95	30	60	43.5	47000	PASS
95	95	100	100	100.0	108037	PASS
96	95	5	9	6.2	6736	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	93.6	101069	PASS
175	174	5	9	6.6	6676	PASS
176	174	95	101	95.4	96416	PASS
177	176	5	9	6.5	6314	PASS