


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD051219\
Data File : VD062272.D
Acq On : 12 May 2019 21:46
Operator : FY/SY
Sample : BFB
Misc : 5.00µ/5mL/MSVOA D/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D050719S.M
Title : SW846 8260
Last Update : Tue May 07 14:26:29 2019

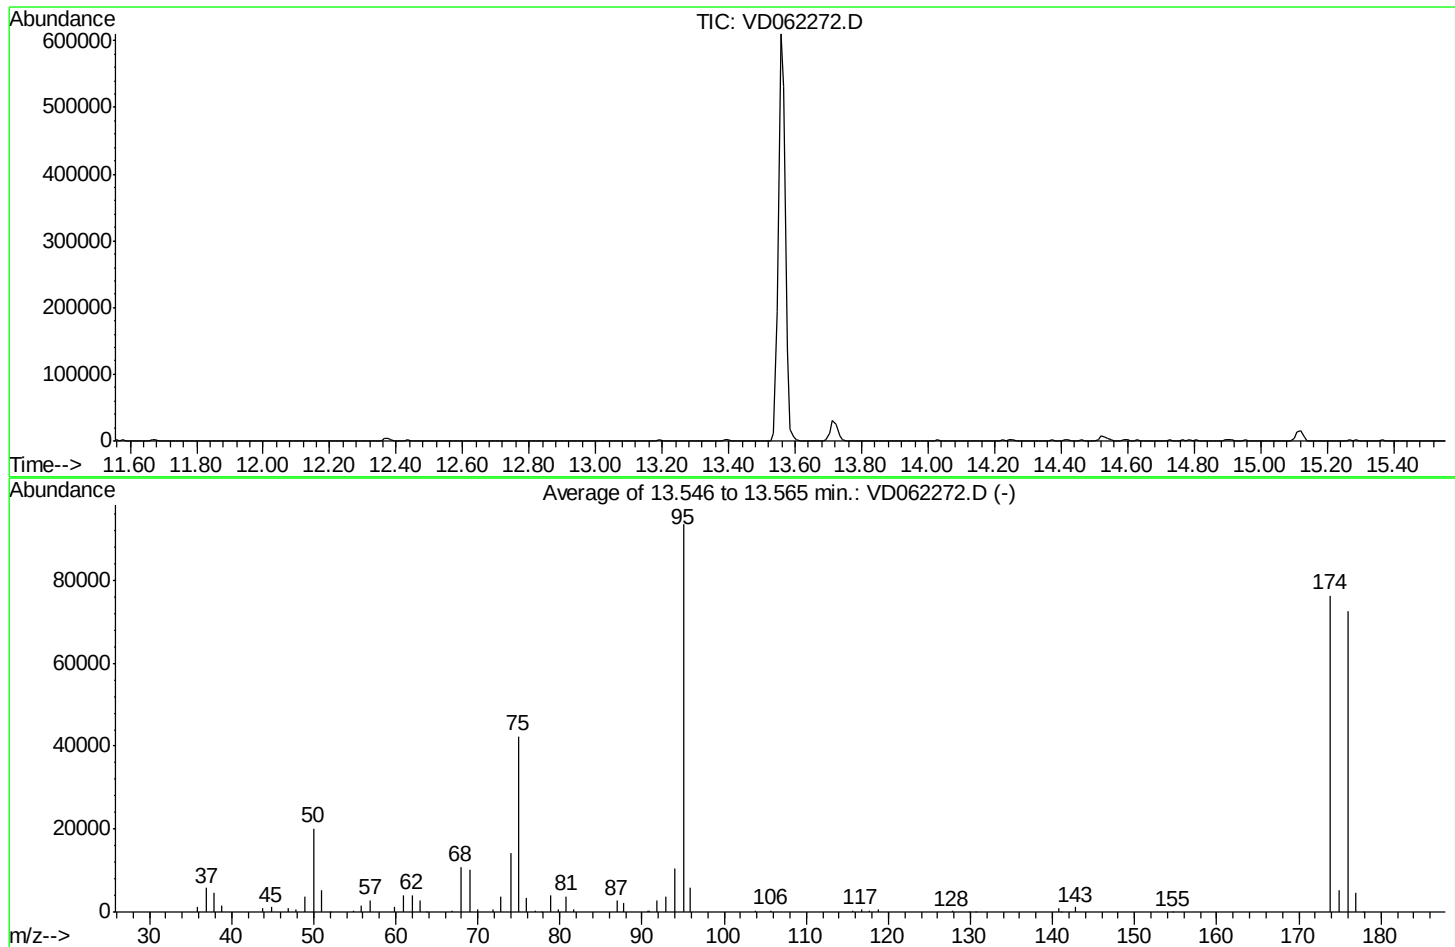

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	20092	PASS
75	95	30	60	45.3	42336	PASS
95	95	100	100	100.0	93501	PASS
96	95	5	9	6.3	5889	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.7	76346	PASS
175	174	5	9	6.8	5173	PASS
176	174	95	101	95.2	72680	PASS
177	176	5	9	6.3	4555	PASS