


Methyl Iodide

Response Ratio

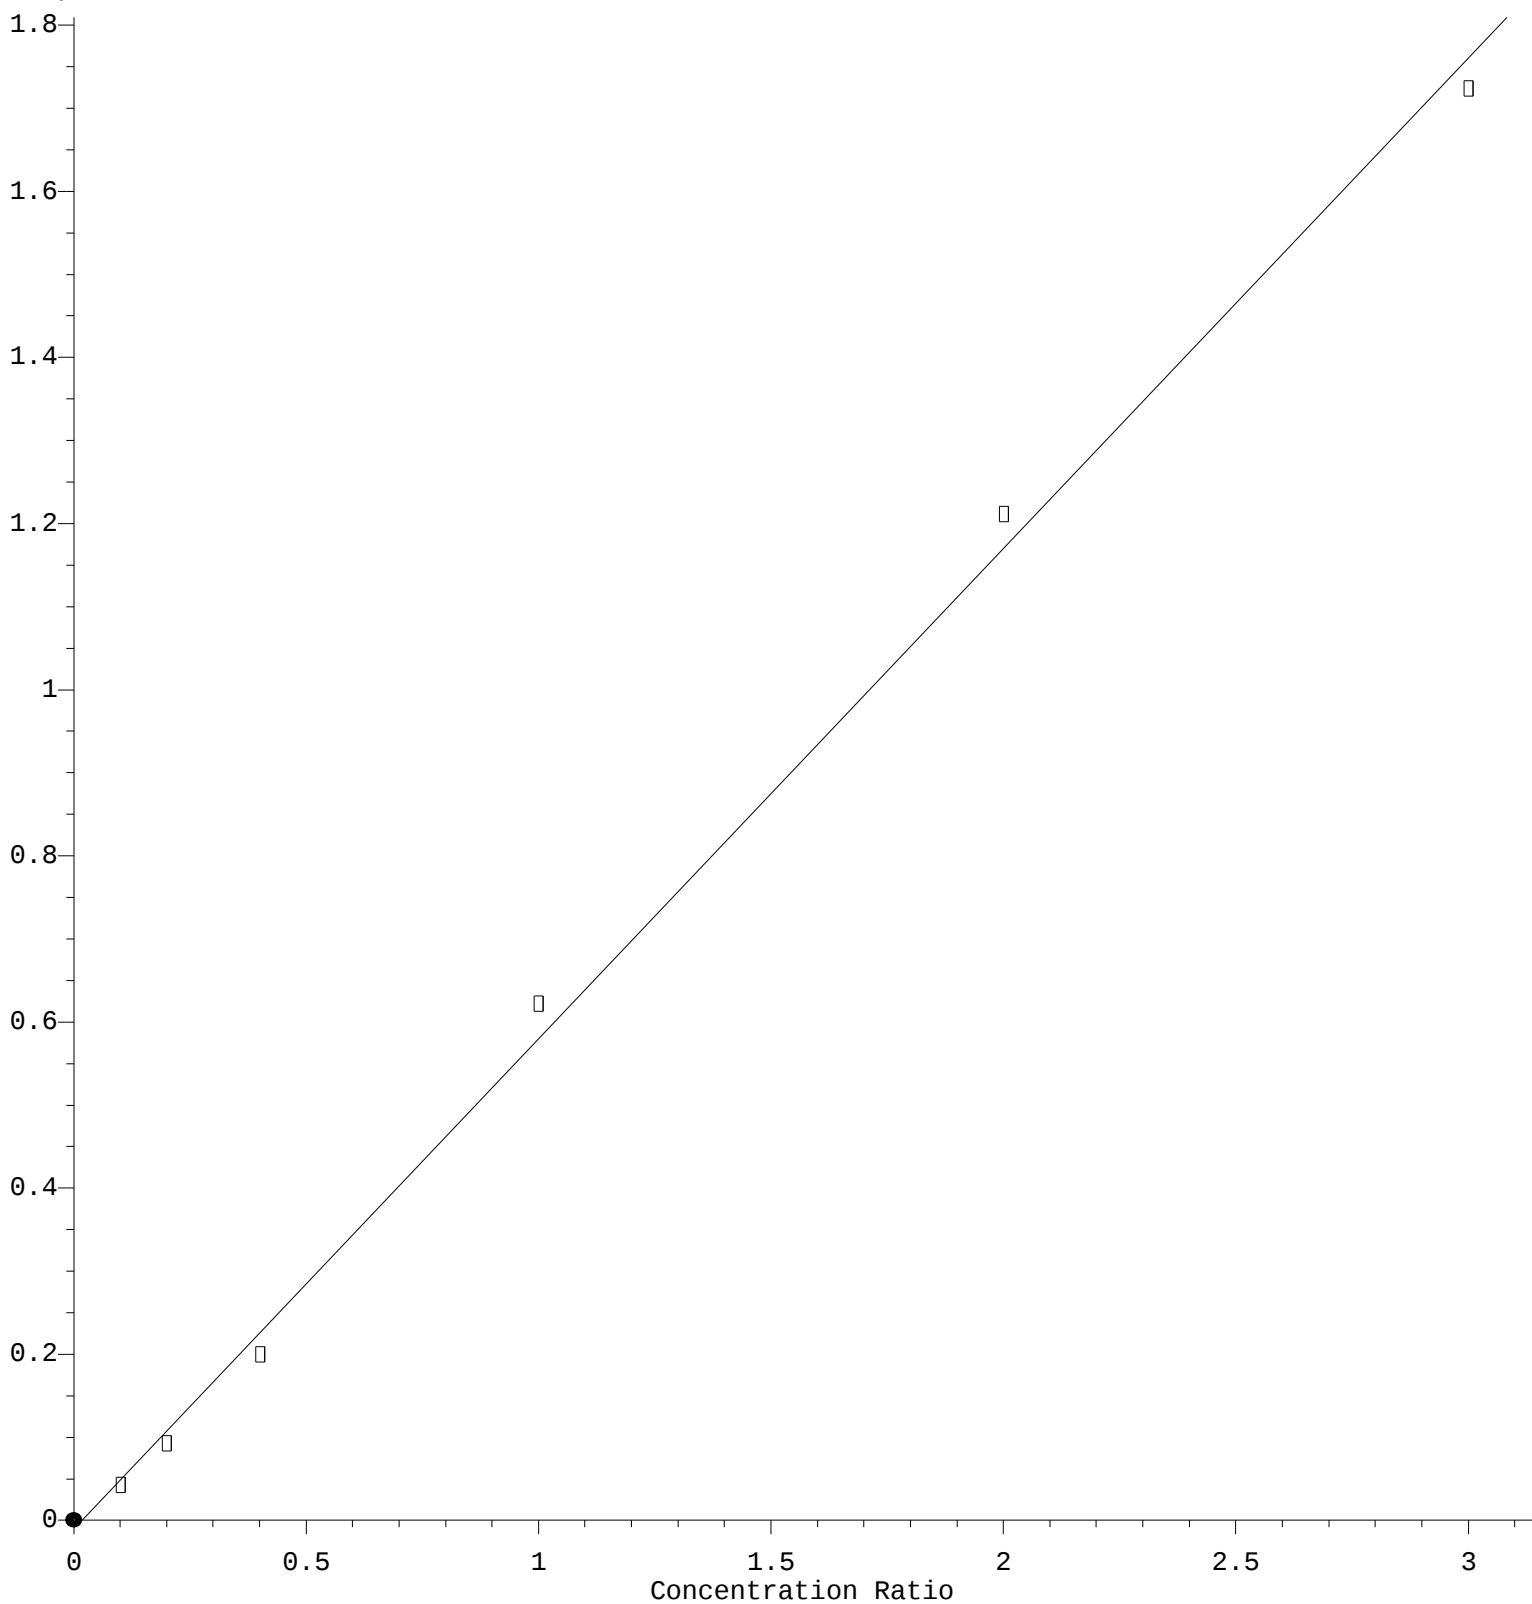


$$\text{Response} = 5.904\text{e-}001 * \text{Amt} - 1.091\text{e-}002$$

Coef of Det (r^2) = 0.997550 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051221S.M

Calibration Table Last Updated: Thu May 13 04:01:29 2021


Tert butylalcohol

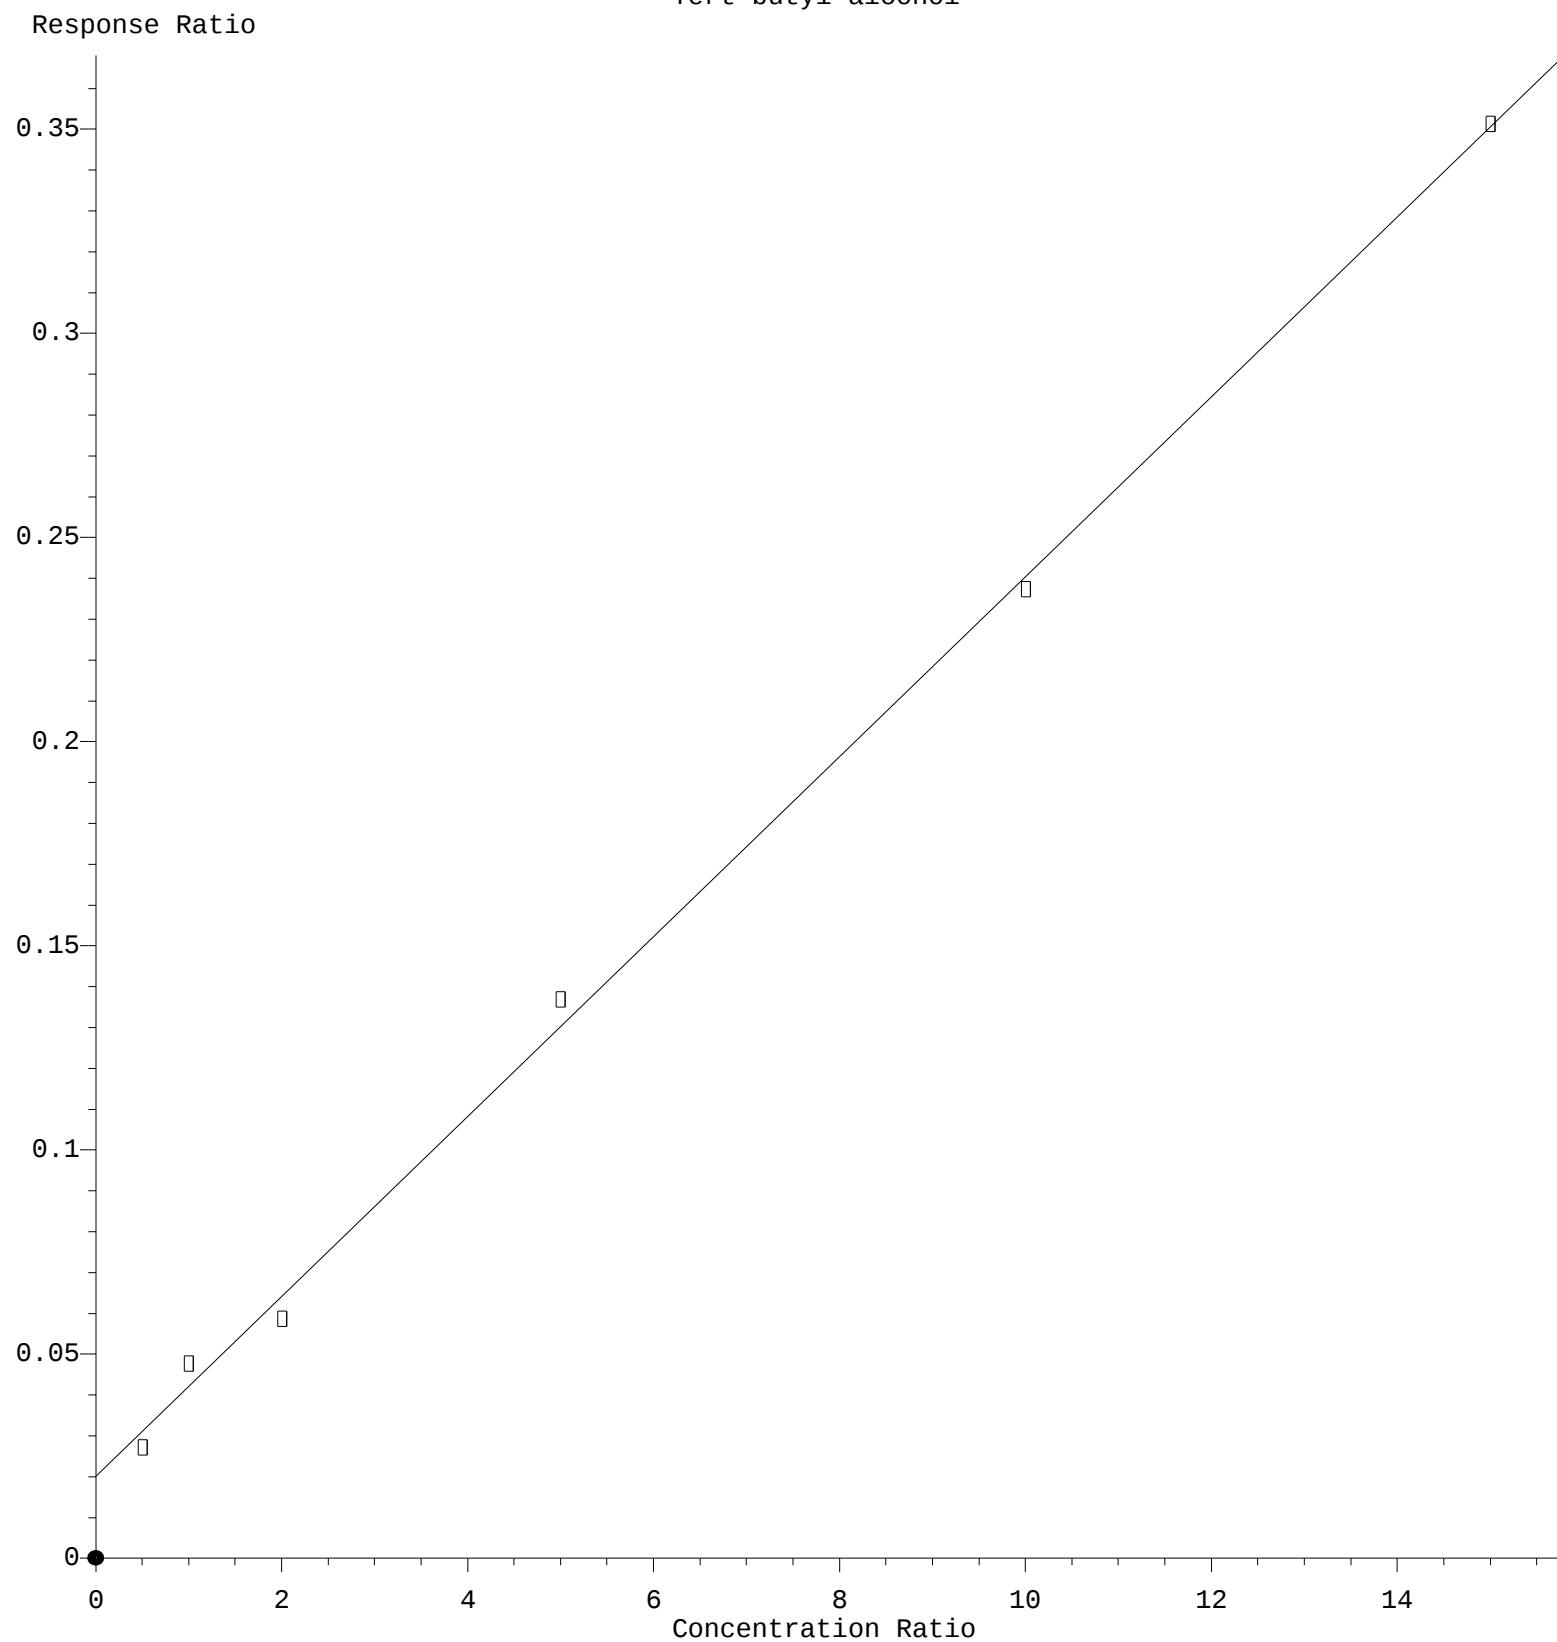

Response = 2.205e-002 * Amt + 1.998e-002
 Coef of Det (r^2) = 0.998412 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051221S.M
 Calibration Table Last Updated: Thu May 13 04:01:29 2021

Methylene Chloride

Response Ratio

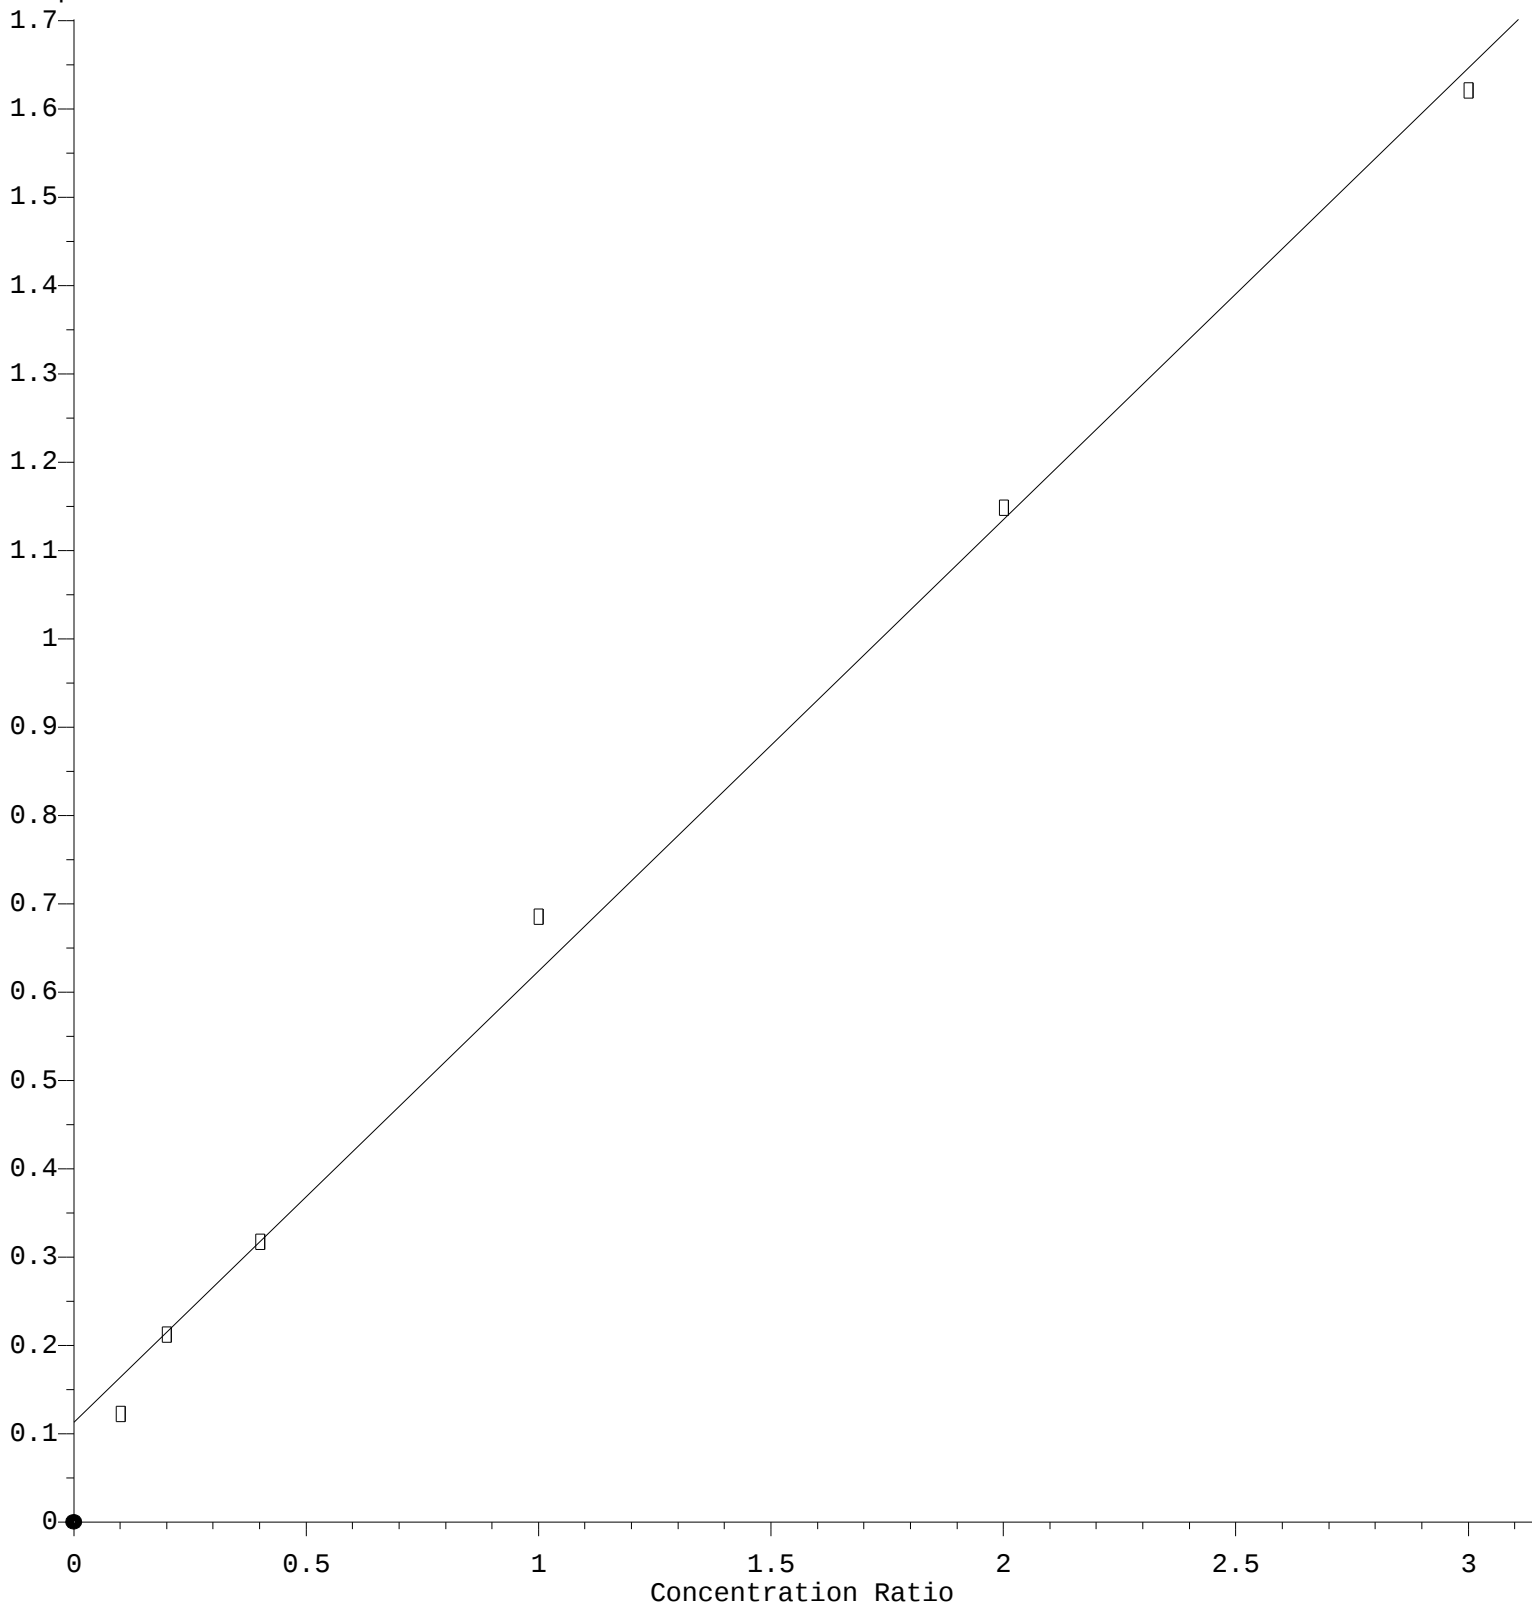


$$\text{Response} = 5.112\text{e-}001 * \text{Amt} + 1.134\text{e-}001$$

Coef of Det (r^2) = 0.996417 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051221S.M

Calibration Table Last Updated: Thu May 13 04:01:29 2021


1,4-Dioxane

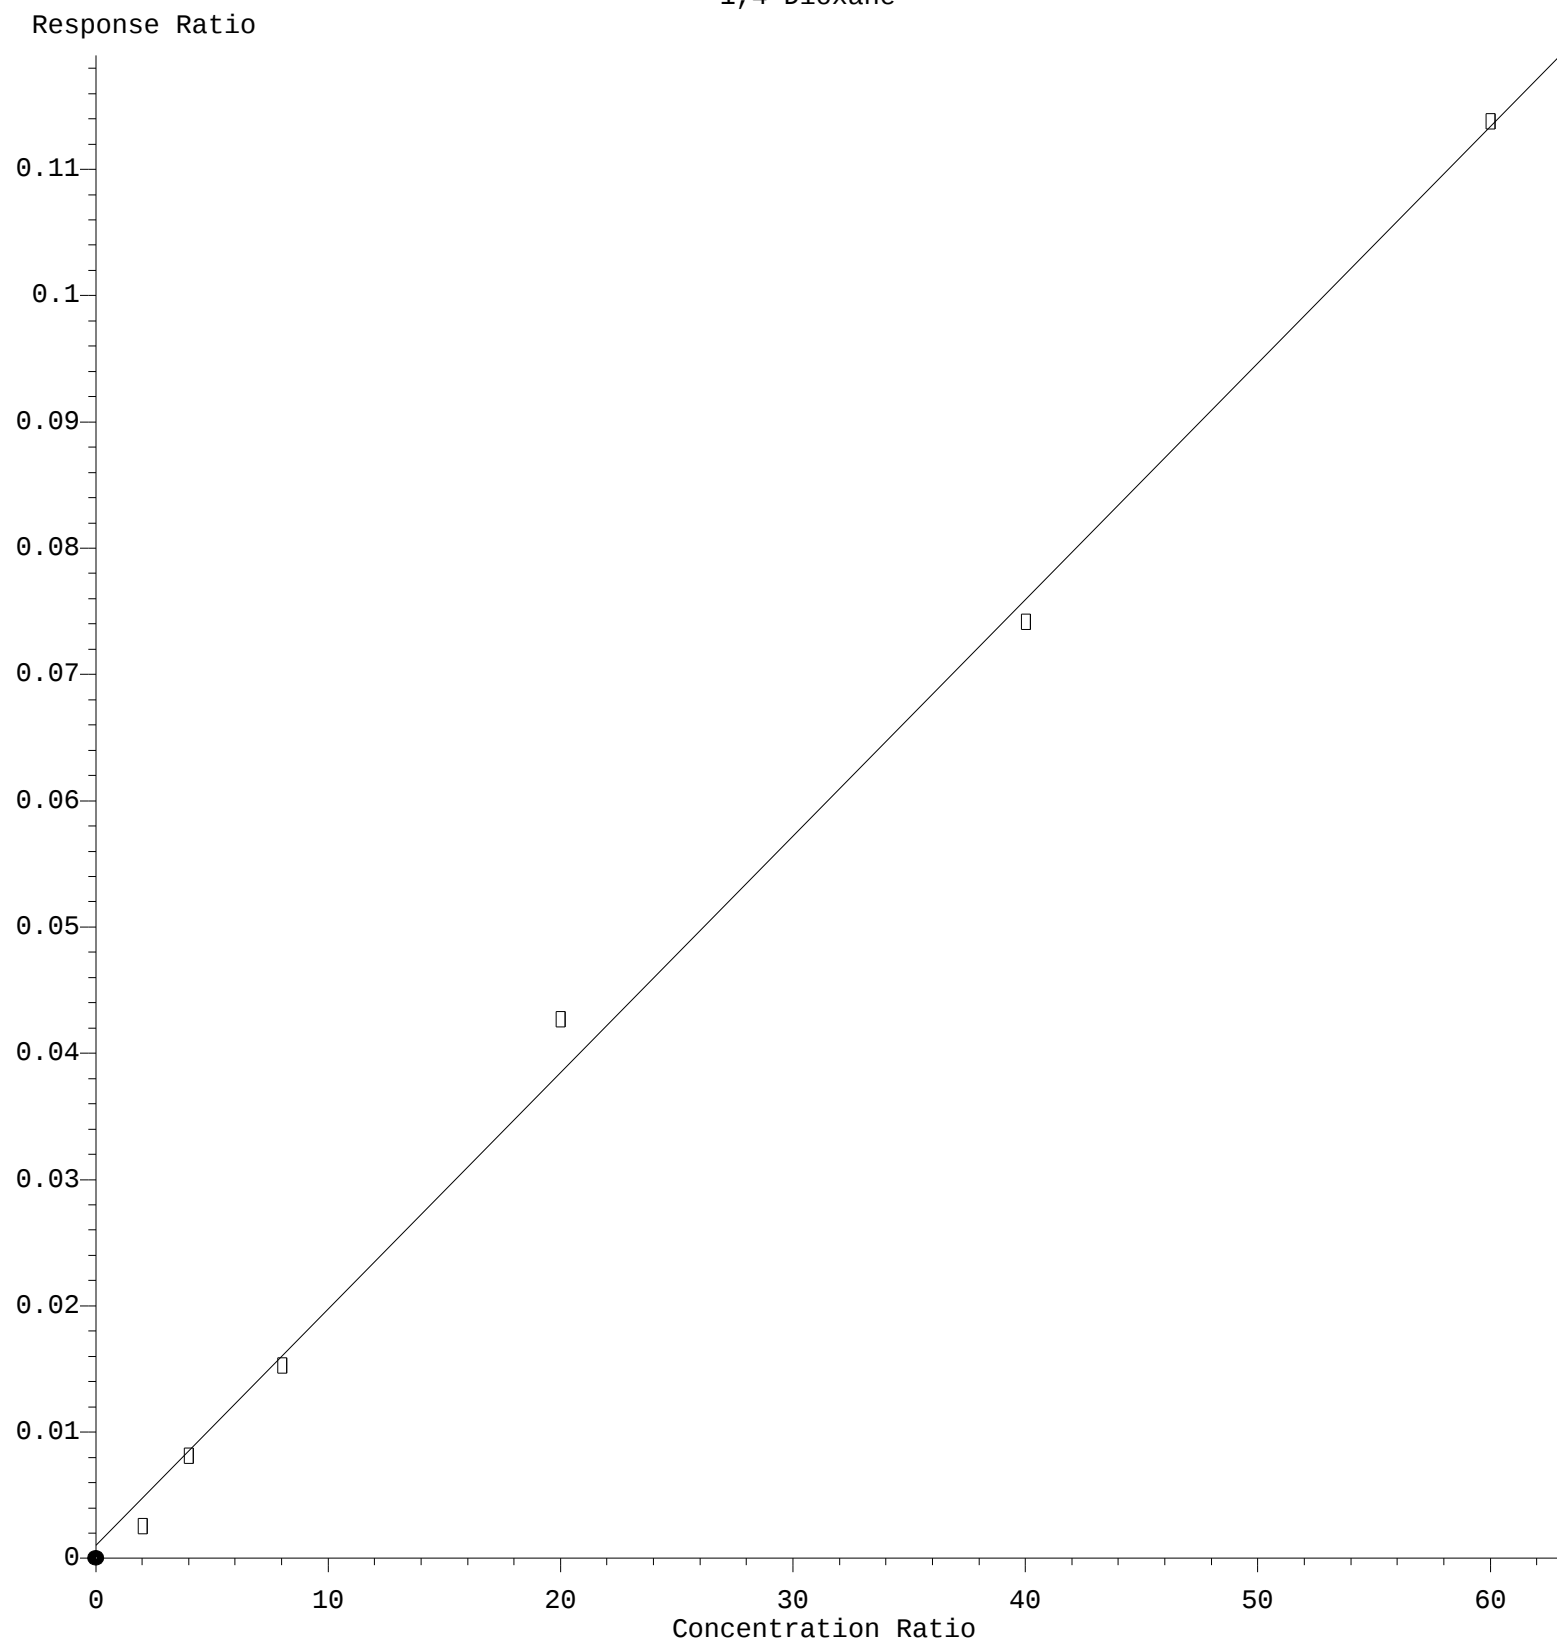

Response = $1.886 \times 10^{-3} \times \text{Amt} + 6.229 \times 10^{-4}$
 Coef of Det (r^2) = 0.997268 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051221S.M
 Calibration Table Last Updated: Thu May 13 04:01:29 2021

Ethyl methacrylate

Response Ratio

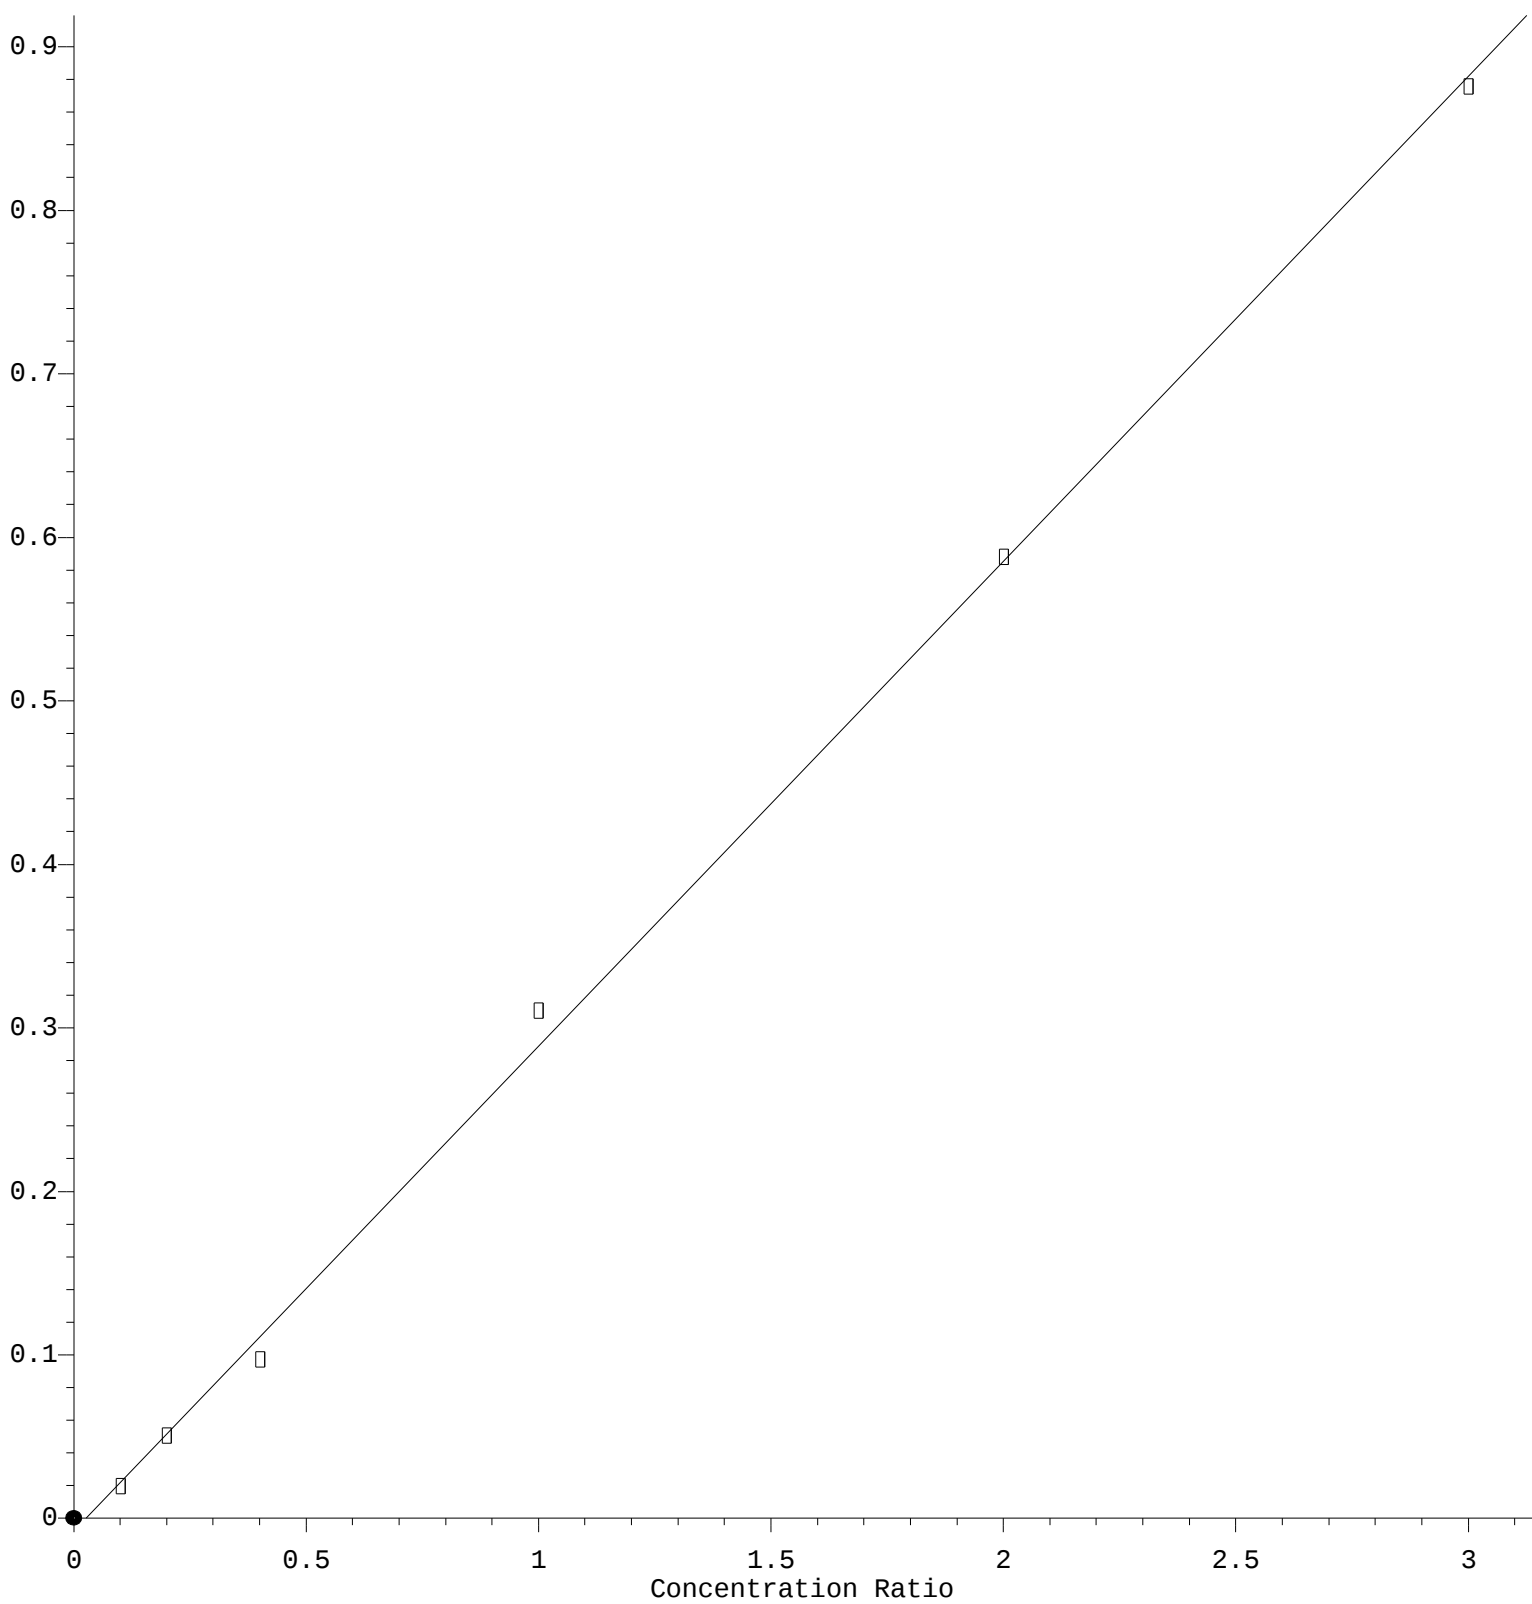

$$\text{Response} = 2.967\text{e-}001 * \text{Amt} - 7.813\text{e-}003$$


Coef of Det (r^2) = 0.998804 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051221S.M

Calibration Table Last Updated: Thu May 13 04:01:29 2021

Naphthalene

Response Ratio

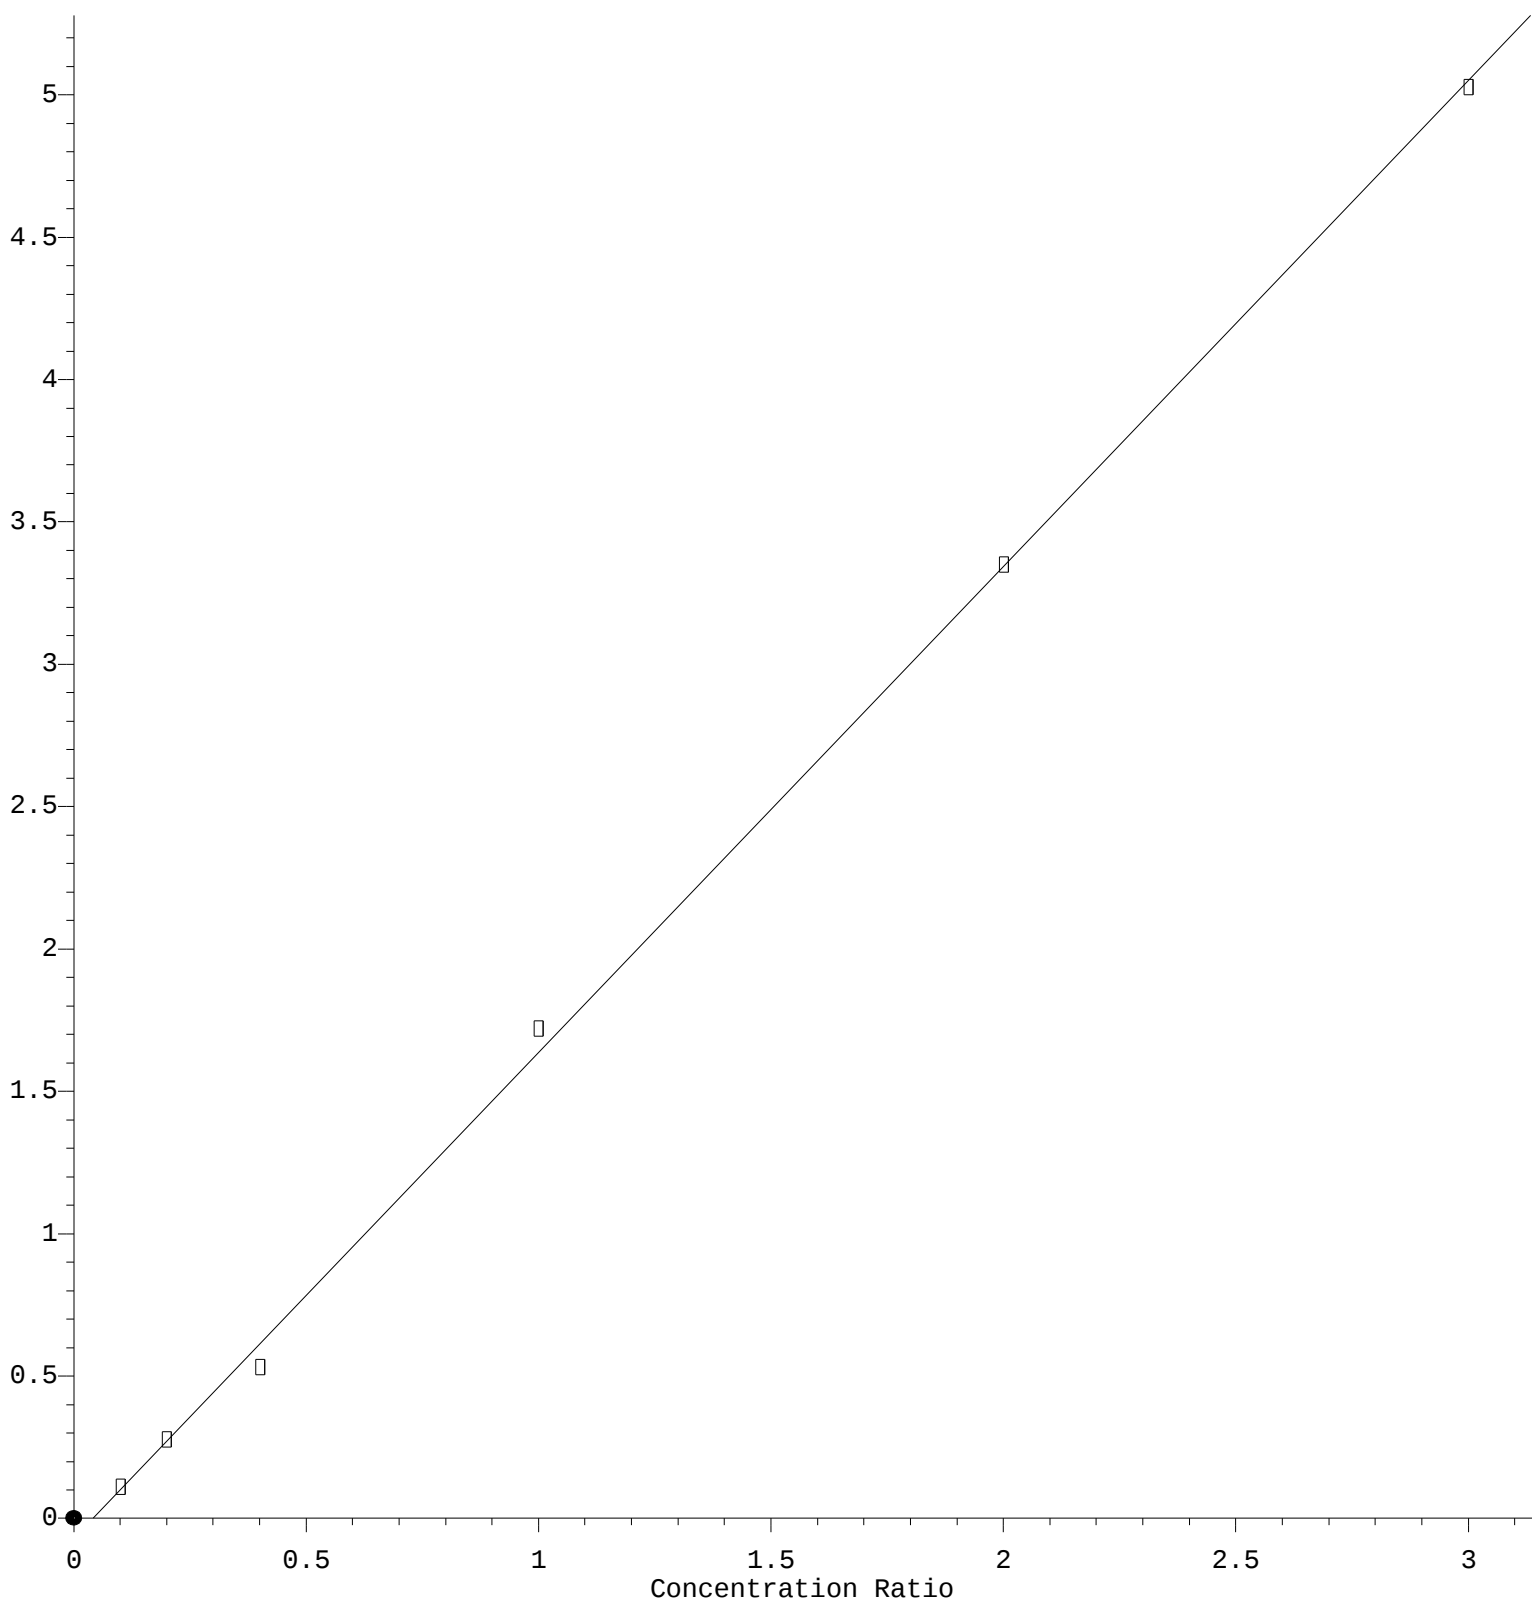

$$\text{Response} = 1.706e+000 * \text{Amt} - 6.978e-002$$

Coef of Det (r^2) = 0.999274 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051221S.M

Calibration Table Last Updated: Thu May 13 04:01:29 2021