

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051222\
 Data File : VD072954.D
 Acq On : 12 May 2022 18:18
 Operator : VA/SY
 Sample : N2782-05
 Misc : 6.16G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 P019-SS001-0612-01

Quant Time: May 13 05:56:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050222S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 03 08:33:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	304771	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.855	114	550156	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	533329	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	217472	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	182219	46.060	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	92.120%
35) Dibromofluoromethane	7.908	113	185908	48.115	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	96.240%
50) Toluene-d8	10.332	98	671788	48.470	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	96.940%
62) 4-Bromofluorobenzene	12.620	95	224691	43.478	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	86.960%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051222\
Data File : VD072954.D
Acq On : 12 May 2022 18:18
Operator : VA/SY
Sample : N2782-05
Misc : 6.16G/5.00ml/MSVOA_D/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
P019-SS001-0612-01

Quant Time: May 13 05:56:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050222S.M
Quant Title : SW846 8260
QLast Update : Tue May 03 08:33:49 2022
Response via : Initial Calibration

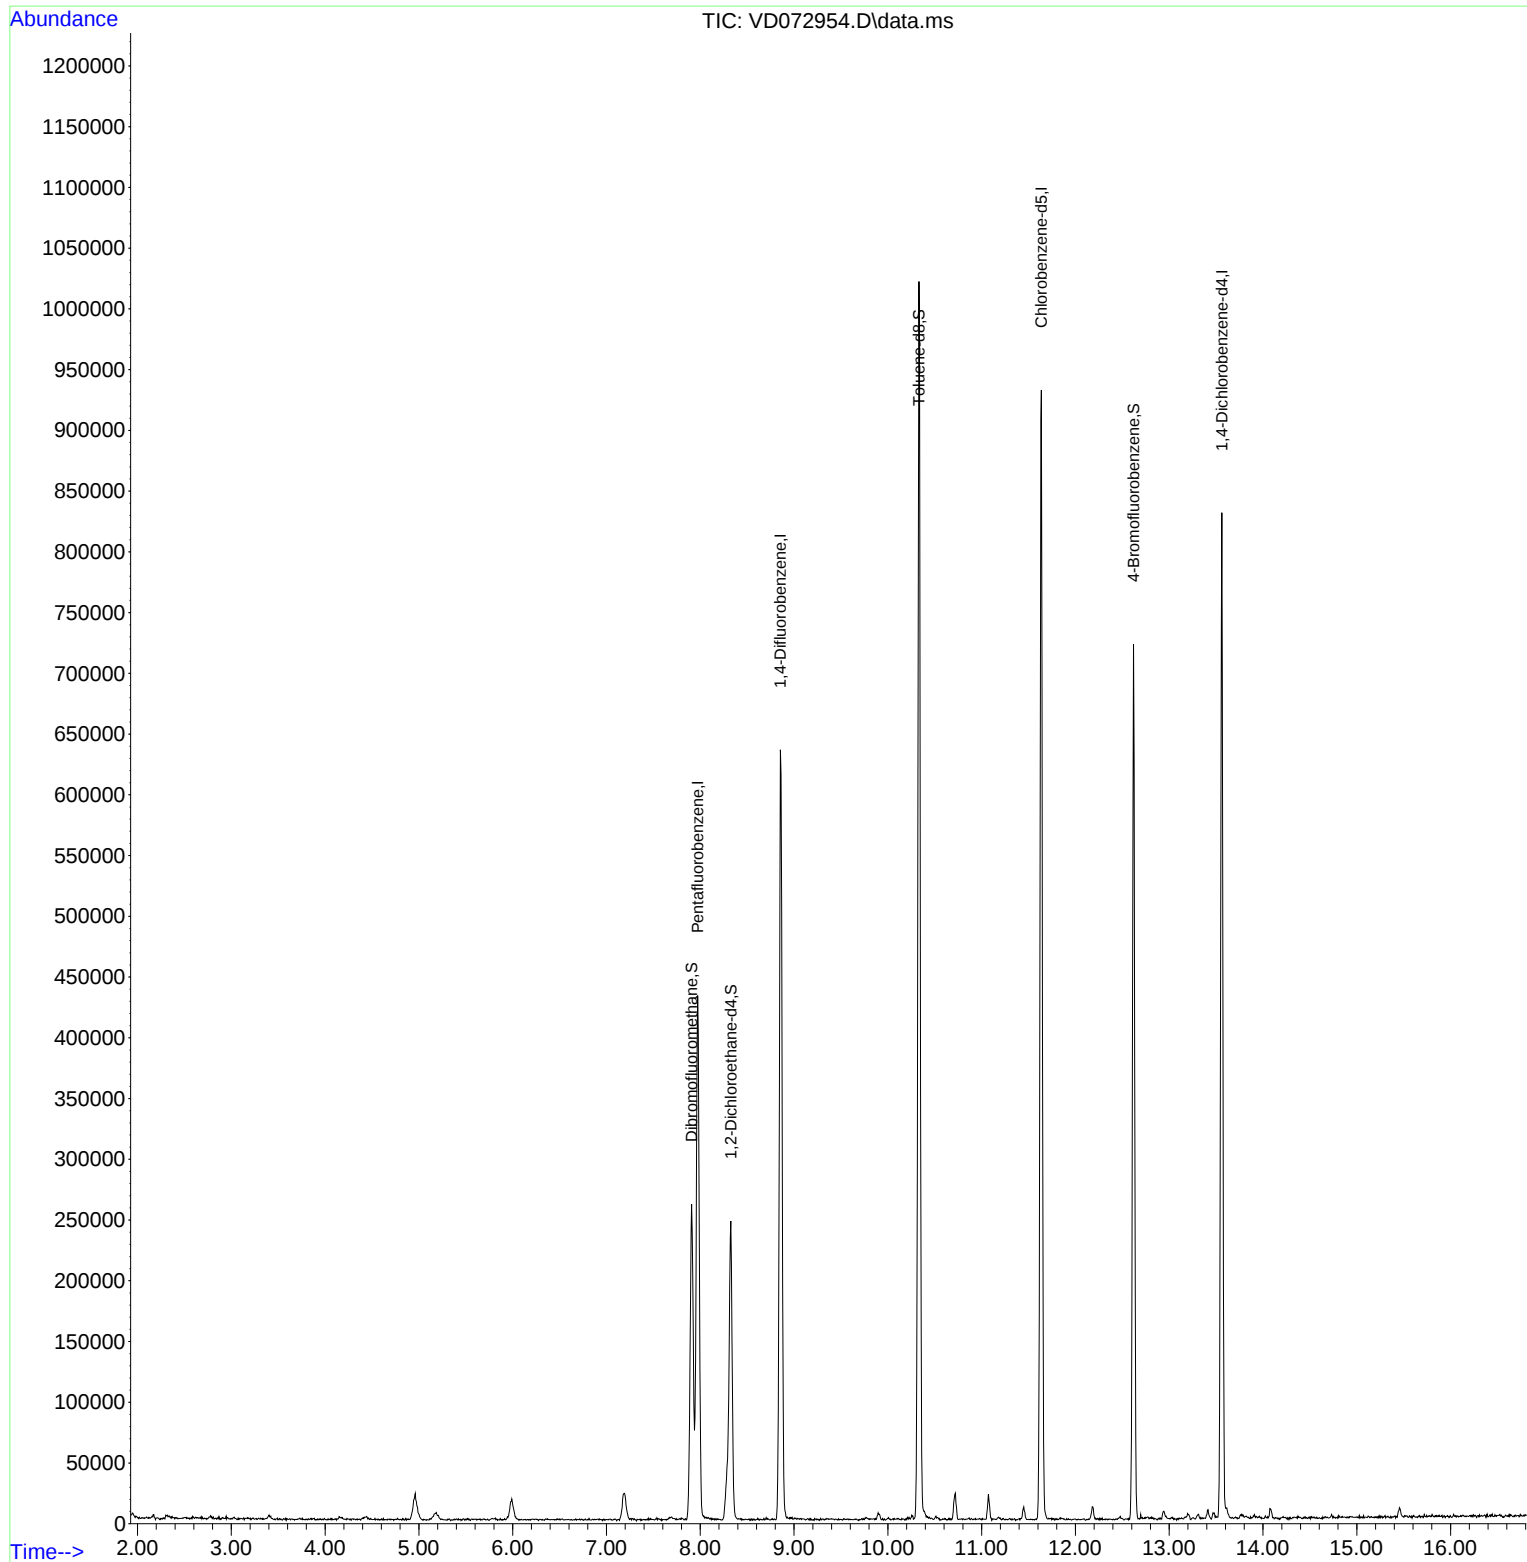

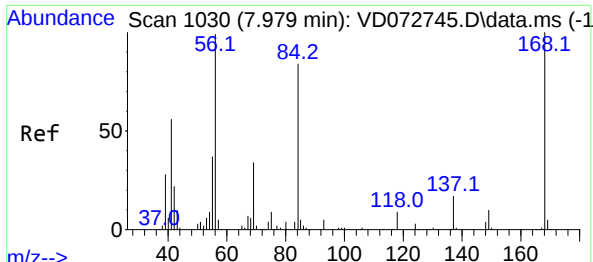

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.973 min Scan# 1029

Delta R.T. -0.006 min

Lab File: VD072954.D

Acq: 12 May 2022 18:18

Instrument :

MSVOA_D

ClientSampleId :





P019-SS001-0612-01

Tgt Ion:168 Resp: 304771

Ion Ratio Lower Upper

168 100

99 59.7 49.8 74.6

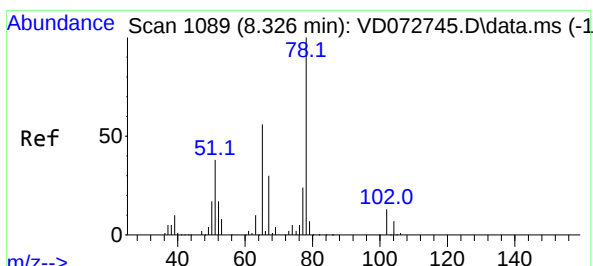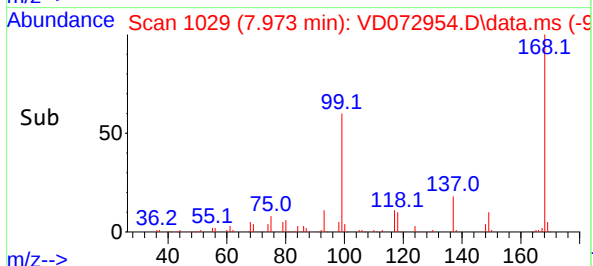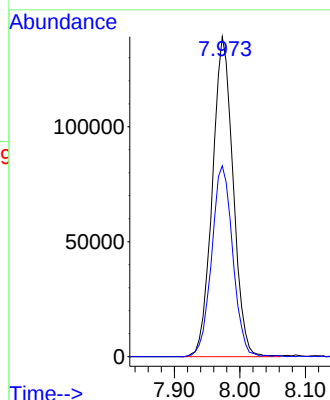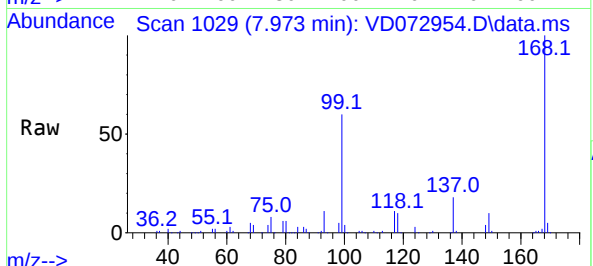

1,2-Dichloroethane-d4

Concen: 46.060 ug/l

RT: 8.326 min Scan# 1089

Delta R.T. 0.000 min

Lab File: VD072954.D




Acq: 12 May 2022 18:18


Tgt Ion: 65 Resp: 182219

Ion Ratio Lower Upper

65 100

67 53.2 0.0 101.4

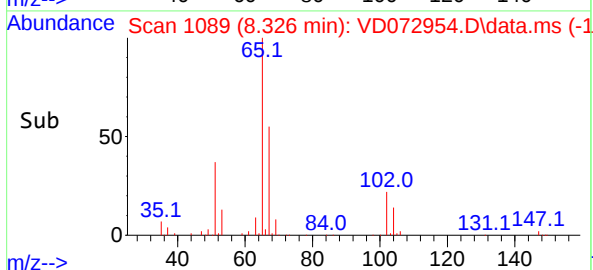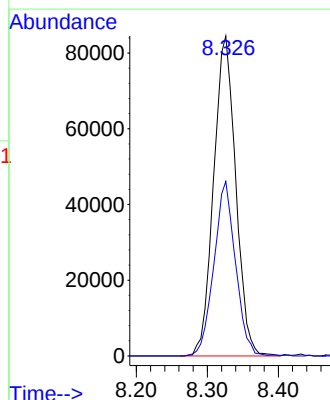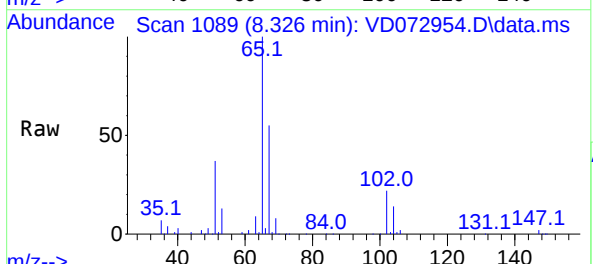

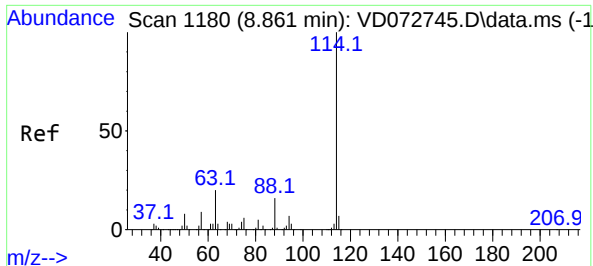

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.855 min Scan# 1180

Delta R.T. -0.006 min

Lab File: VD072954.D

Acq: 12 May 2022 18:18

Instrument :

MSVOA_D

ClientSampleId :

P019-SS001-0612-01





Tgt Ion:114 Resp: 550156

Ion Ratio Lower Upper

114 100

63 20.2 0.0 46.6

88 15.7 0.0 33.2

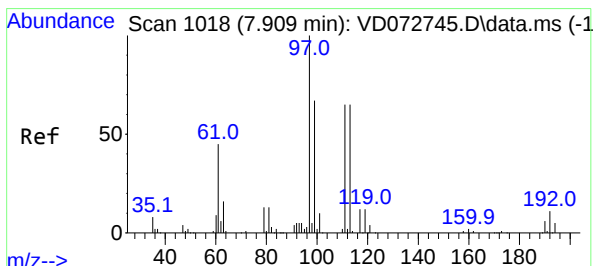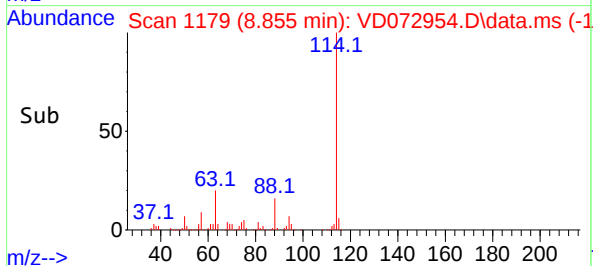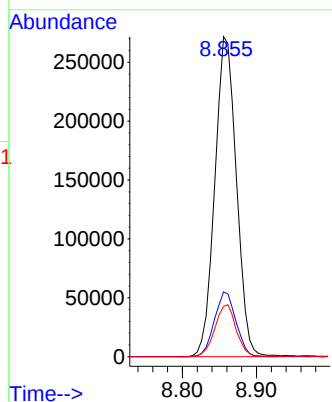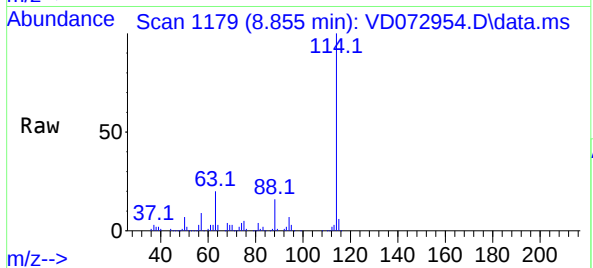

#35

Dibromofluoromethane

Concen: 48.115 ug/l

RT: 7.908 min Scan# 1018

Delta R.T. -0.001 min

Lab File: VD072954.D

Acq: 12 May 2022 18:18




Tgt Ion:113 Resp: 185908


Ion Ratio Lower Upper

113 100

111 102.1 83.8 125.6

192 18.3 14.6 21.8

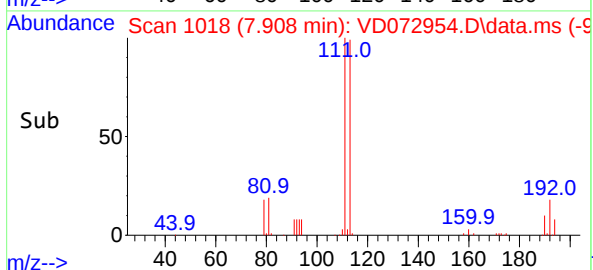
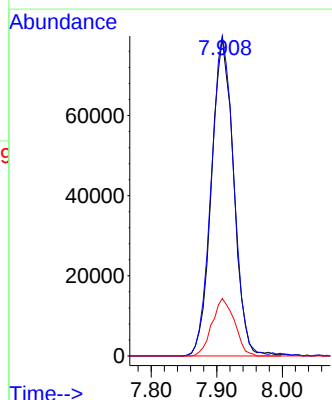
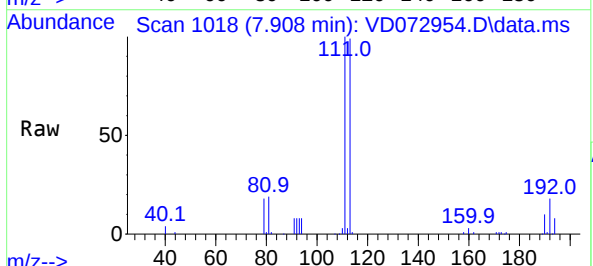


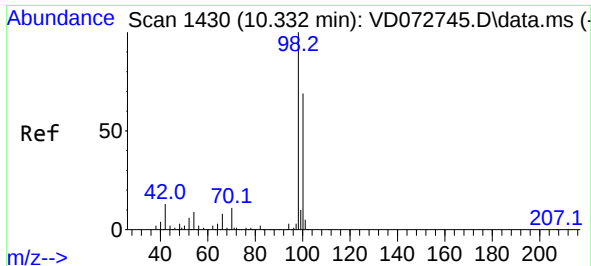

#50
Toluene-d8
Concen: 48.470 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD072954.D
Acq: 12 May 2022 18:18




Instrument :
MSVOA_D
ClientSampleId :
P019-SS001-0612-01


Tgt Ion: 98 Resp: 671788
Ion Ratio Lower Upper
98 100
100 66.8 52.4 78.6

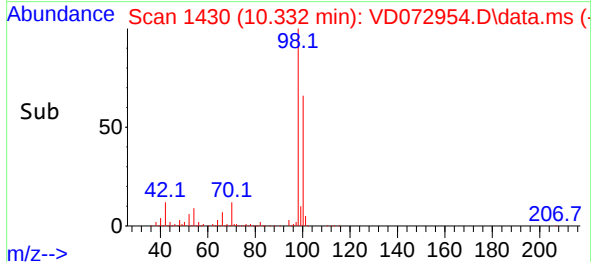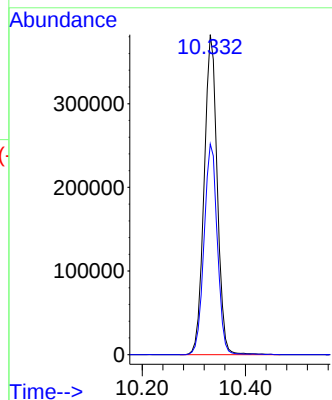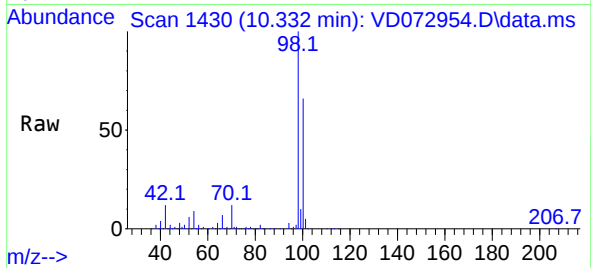

#62
4-Bromofluorobenzene
Concen: 43.478 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VD072954.D
Acq: 12 May 2022 18:18

Tgt Ion: 95 Resp: 224691
Ion Ratio Lower Upper
95 100
174 78.6 0.0 152.8
176 73.6 0.0 145.4


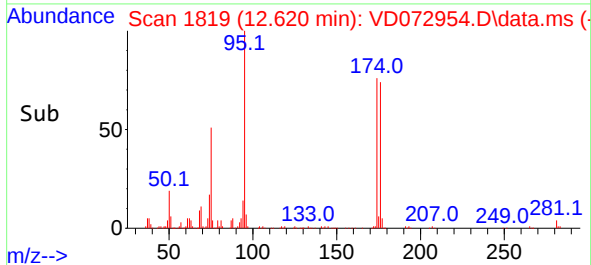
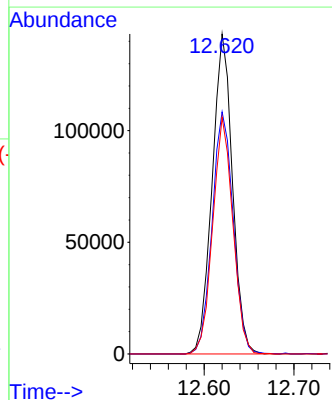
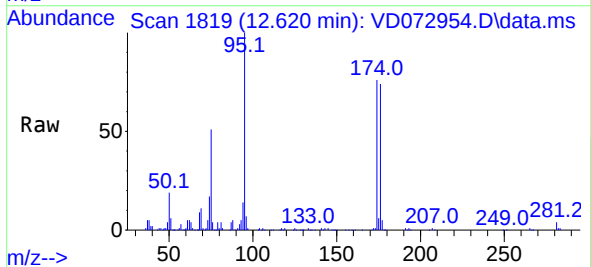


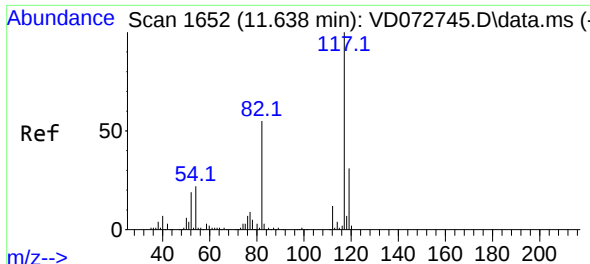

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 117
Delta R.T. -0.000 min
Lab File: VD072954.D
Acq: 12 May 2022 18:18

Instrument :
MSVOA_D
ClientSampleId :
P019-SS001-0612-01

Tgt Ion:117 Resp: 533329
Ion Ratio Lower Upper
117 100
82 54.4 45.3 67.9
119 32.4 26.6 40.0

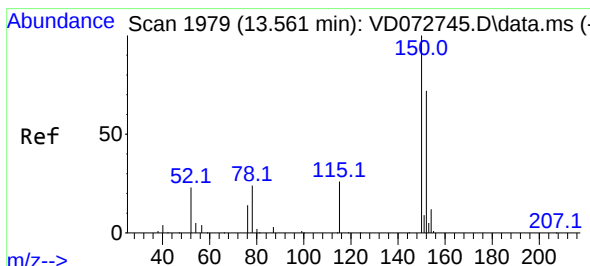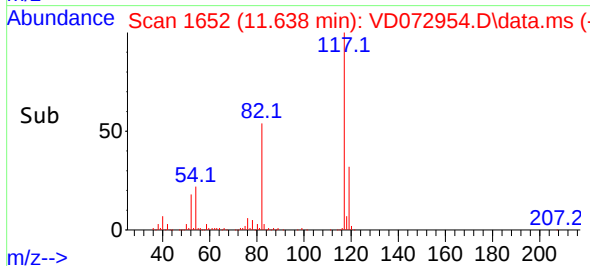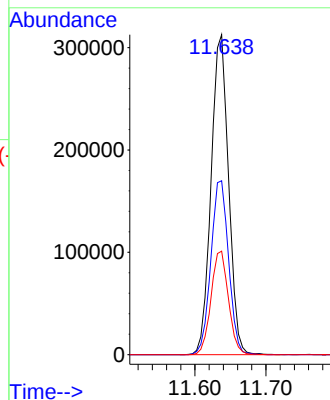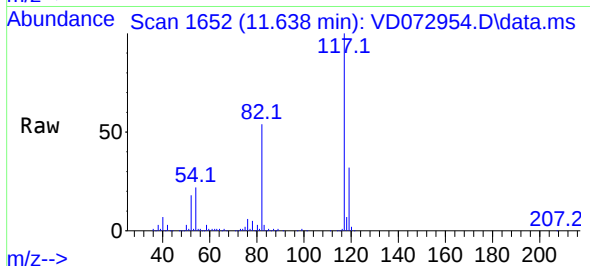

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.000 min
Lab File: VD072954.D
Acq: 12 May 2022 18:18

Tgt Ion:152 Resp: 217472
Ion Ratio Lower Upper
152 100
115 60.1 31.3 93.8
150 157.5 0.0 348.6

