

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051222\
 Data File : VD072964.D
 Acq On : 12 May 2022 23:09
 Operator : VA/SY
 Sample : N2817-06
 Misc : 4.16G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 P007-SS022-0006-01

Quant Time: May 13 05:59:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050222S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 03 08:33:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	309391	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	550260	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	530900	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	231285	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	164496	40.959	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	81.920%
35) Dibromofluoromethane	7.908	113	177868	46.026	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	92.060%
50) Toluene-d8	10.332	98	672367	48.503	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	97.000%
62) 4-Bromofluorobenzene	12.620	95	225250	43.578	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	87.160%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051222\
Data File : VD072964.D
Acq On : 12 May 2022 23:09
Operator : VA/SY
Sample : N2817-06
Misc : 4.16G/5.00ml/MSVOA_D/SOIL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
P007-SS022-0006-01

Quant Time: May 13 05:59:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050222S.M
Quant Title : SW846 8260
QLast Update : Tue May 03 08:33:49 2022
Response via : Initial Calibration

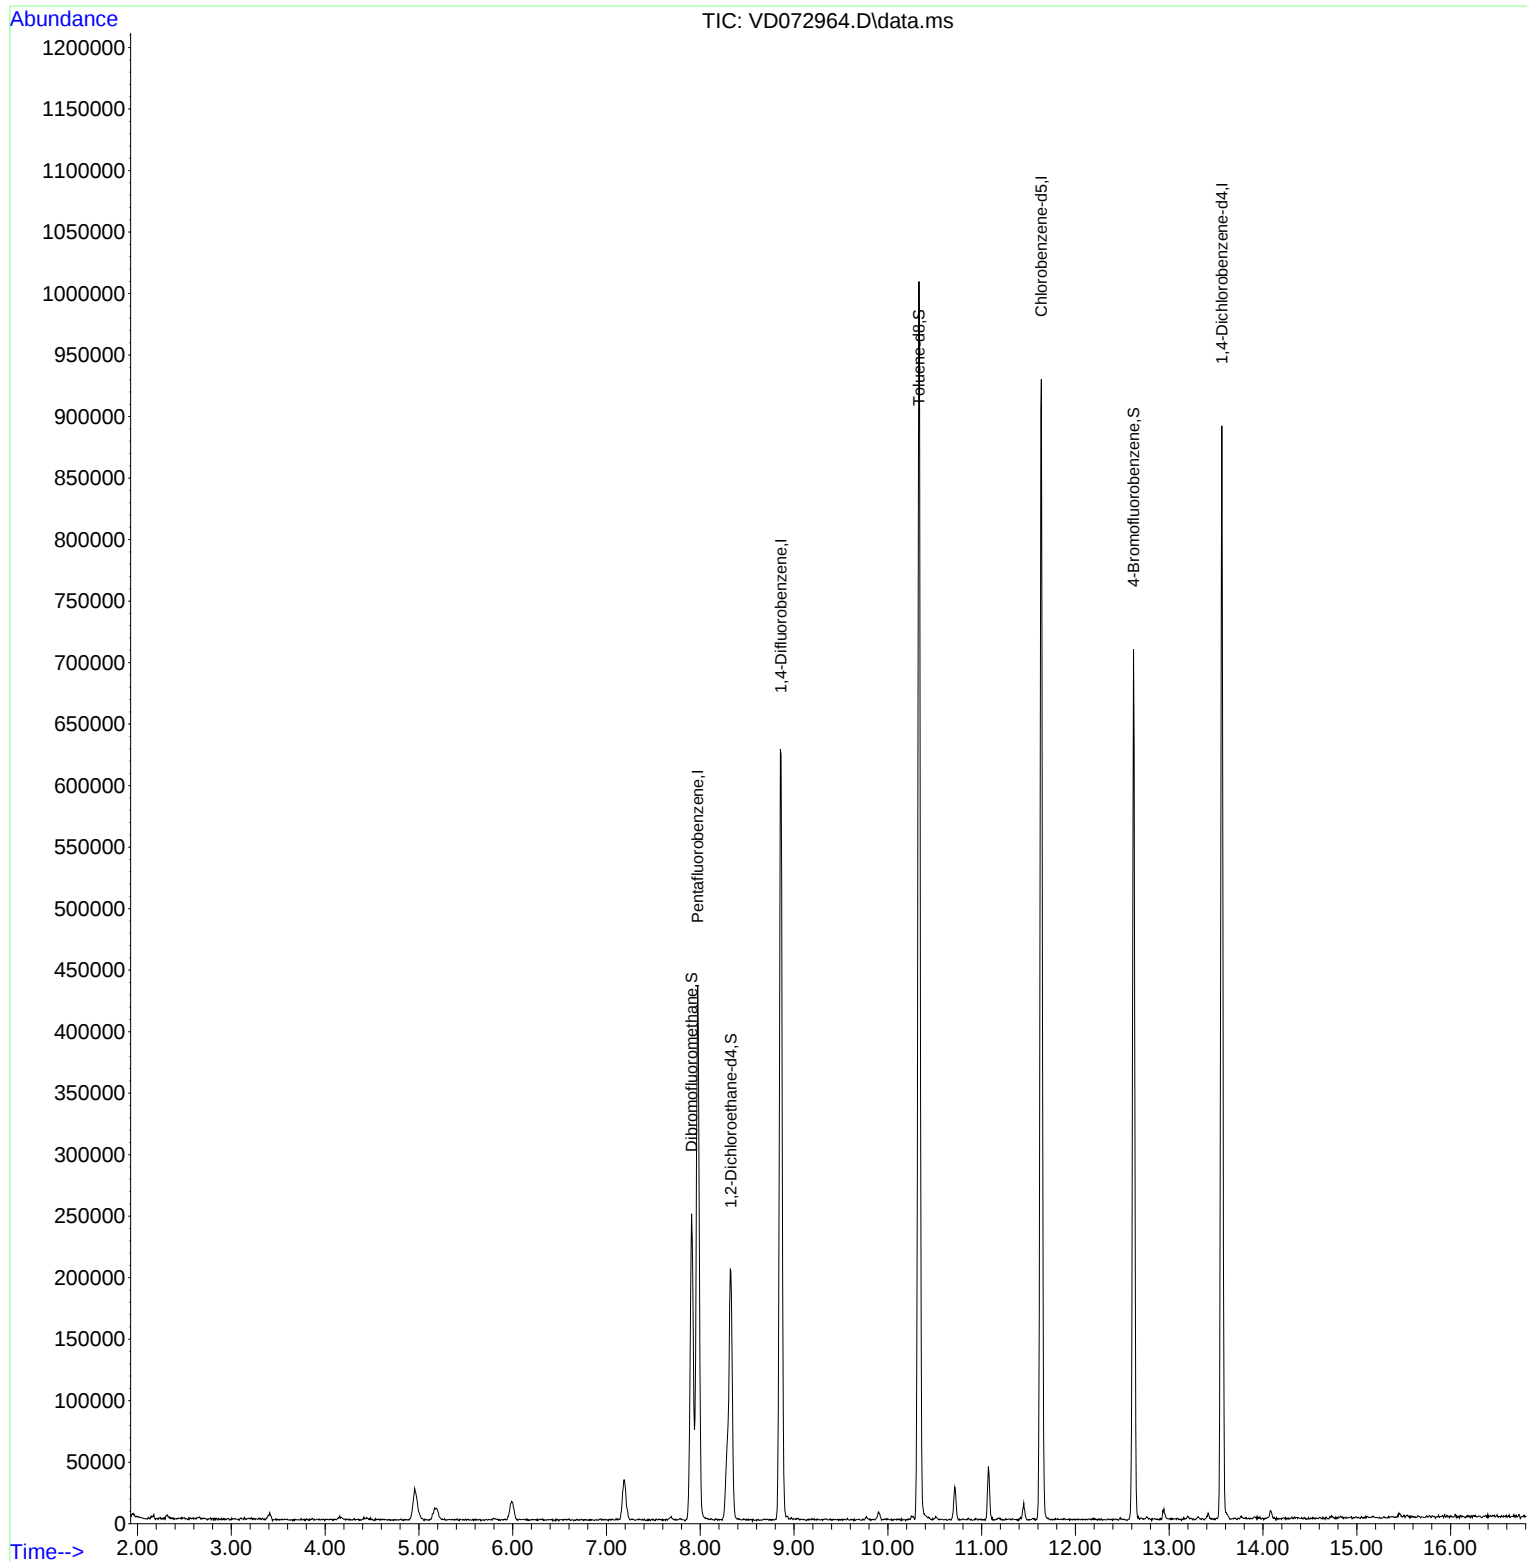



Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.973 min Scan# 1029

Delta R.T. -0.006 min

Lab File: VD072964.D

Acq: 12 May 2022 23:09

Instrument :

MSVOA_D

ClientSampleId :





P007-SS022-0006-01

Tgt Ion:168 Resp: 309391

Ion Ratio Lower Upper

168 100

99 57.4 49.8 74.6

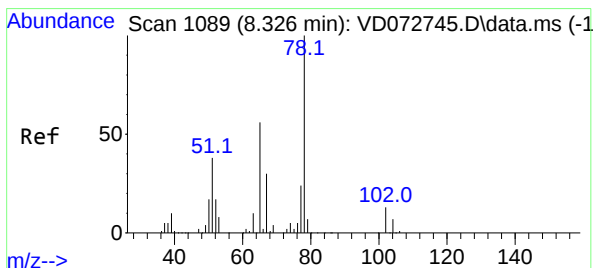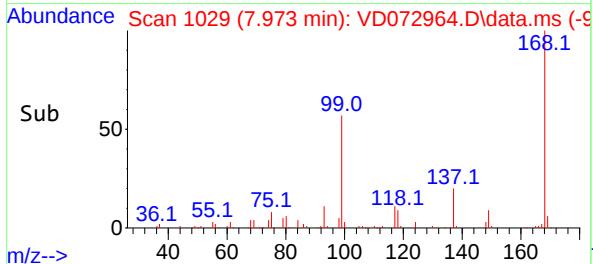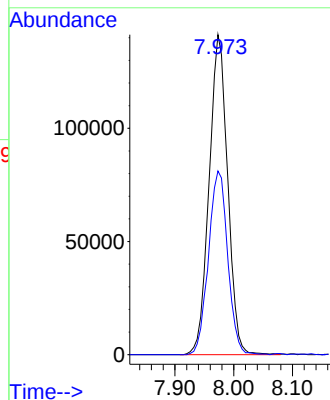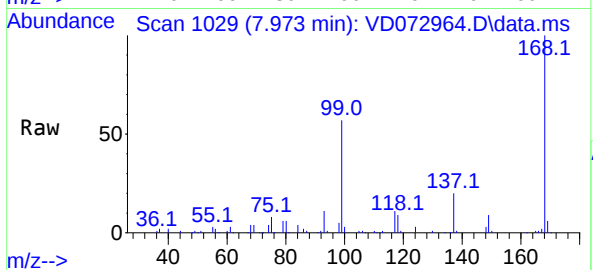

1,2-Dichloroethane-d4

Concen: 40.959 ug/l

RT: 8.326 min Scan# 1089

Delta R.T. 0.000 min

Lab File: VD072964.D




Acq: 12 May 2022 23:09


Tgt Ion: 65 Resp: 164496

Ion Ratio Lower Upper

65 100

67 51.7 0.0 101.4

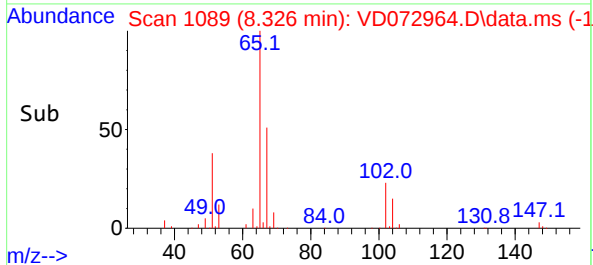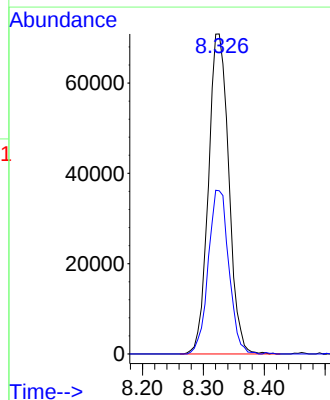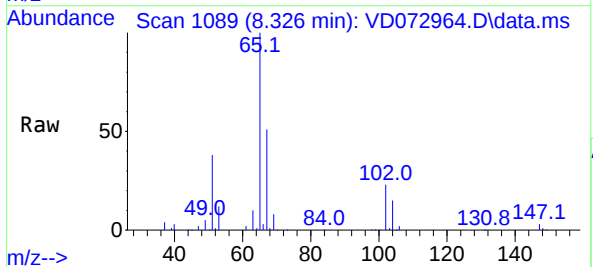

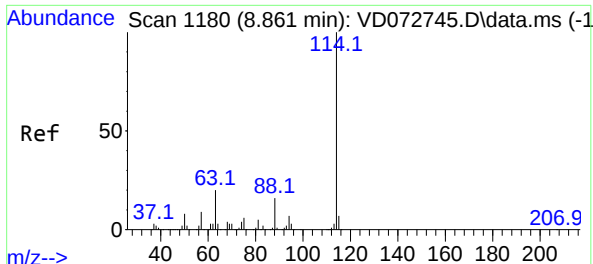

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.861 min Scan# 1180

Delta R.T. 0.000 min

Lab File: VD072964.D

Acq: 12 May 2022 23:09

Instrument :

MSVOA_D

ClientSampleId :

P007-SS022-0006-01





Tgt Ion:114 Resp: 550260

Ion Ratio Lower Upper

114 100

63 20.2 0.0 46.6

88 15.4 0.0 33.2

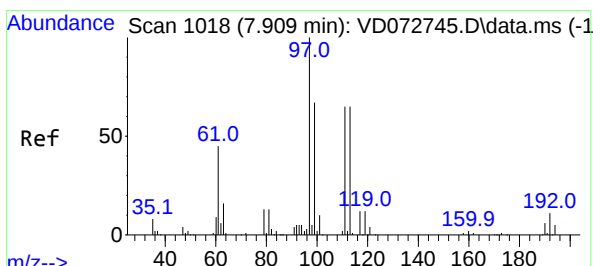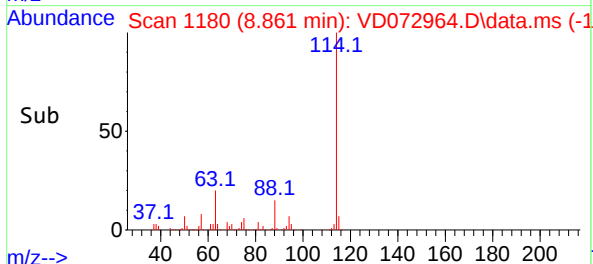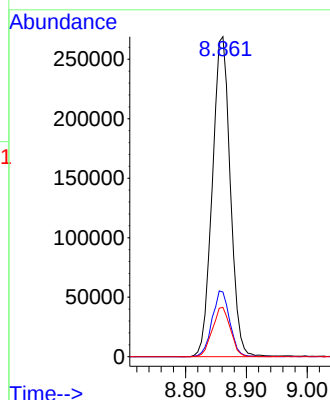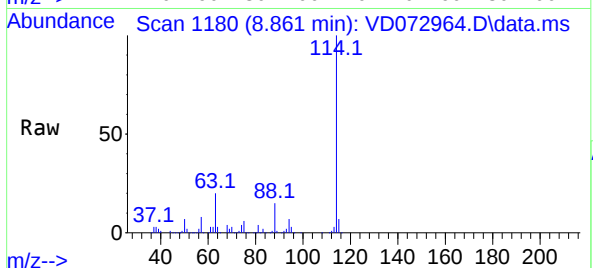

#35

Dibromofluoromethane

Concen: 46.026 ug/l

RT: 7.908 min Scan# 1018

Delta R.T. -0.001 min

Lab File: VD072964.D

Acq: 12 May 2022 23:09




Tgt Ion:113 Resp: 177868


Ion Ratio Lower Upper

113 100

111 104.6 83.8 125.6

192 18.1 14.6 21.8

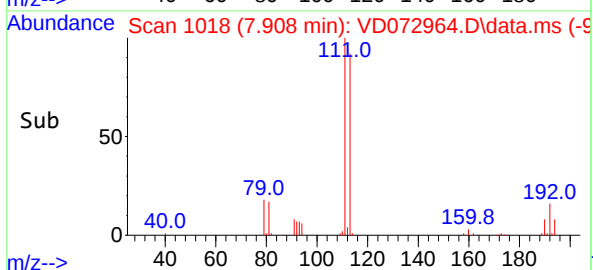
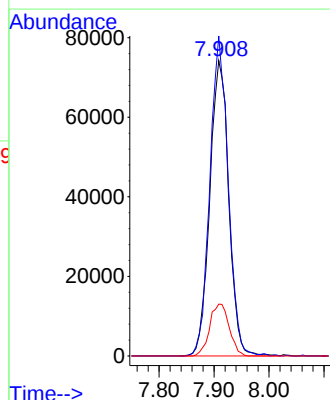
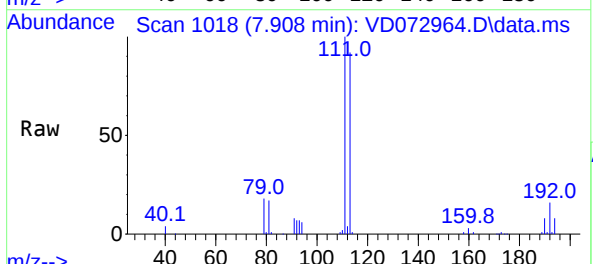


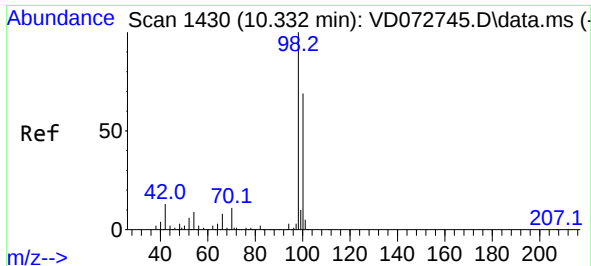

#50
Toluene-d8
Concen: 48.503 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD072964.D
Acq: 12 May 2022 23:09




Instrument :
MSVOA_D
ClientSampleId :
P007-SS022-0006-01


Tgt Ion: 98 Resp: 672367
Ion Ratio Lower Upper
98 100
100 64.7 52.4 78.6

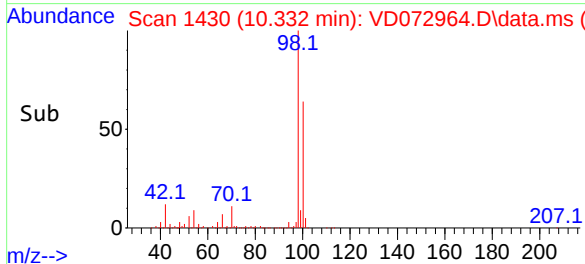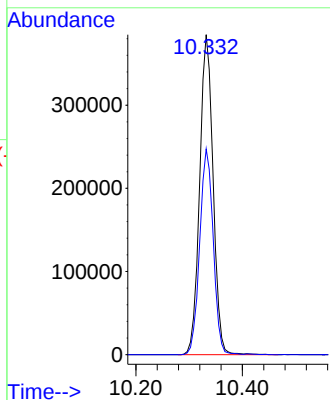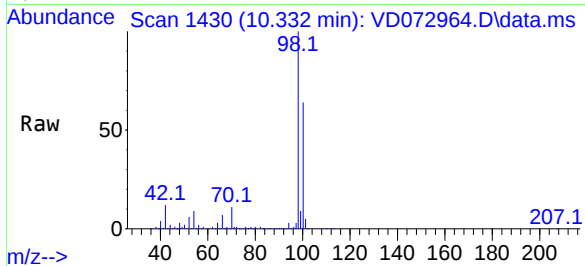

#62
4-Bromofluorobenzene
Concen: 43.578 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VD072964.D
Acq: 12 May 2022 23:09

Tgt Ion: 95 Resp: 225250
Ion Ratio Lower Upper
95 100
174 78.6 0.0 152.8
176 73.0 0.0 145.4


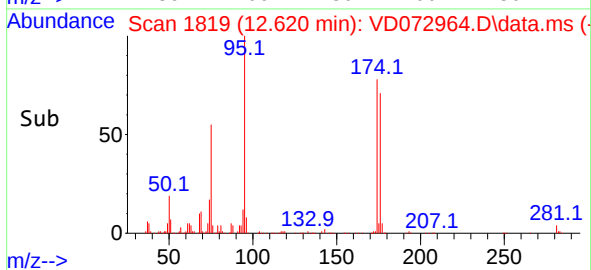
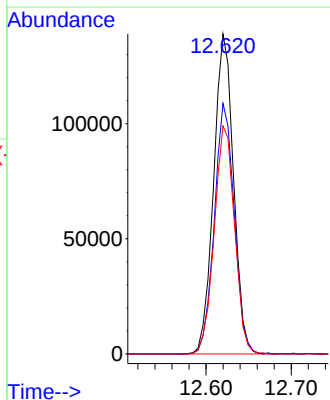
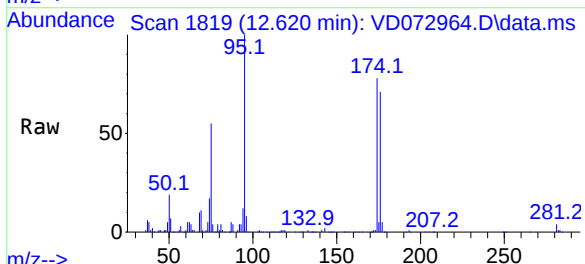


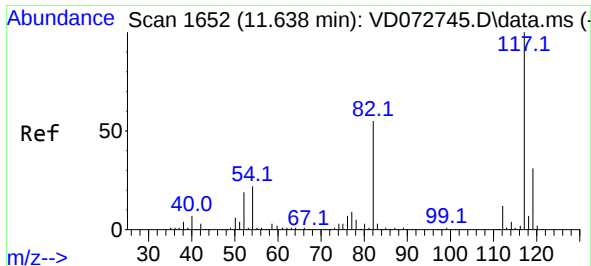

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1
Delta R.T. -0.000 min
Lab File: VD072964.D
Acq: 12 May 2022 23:09

Instrument :
MSVOA_D
ClientSampleId :
P007-SS022-0006-01

Tgt Ion:117 Resp: 530900
Ion Ratio Lower Upper
117 100
82 56.2 45.3 67.9
119 33.2 26.6 40.0

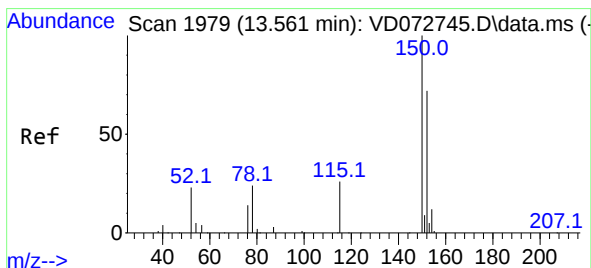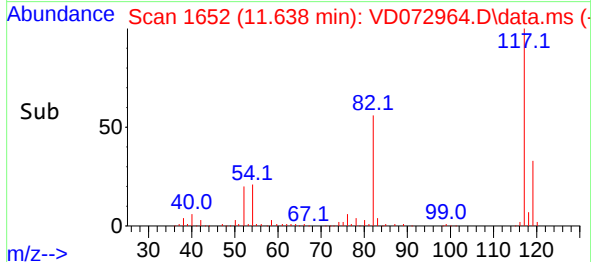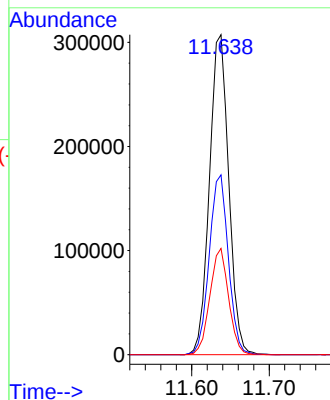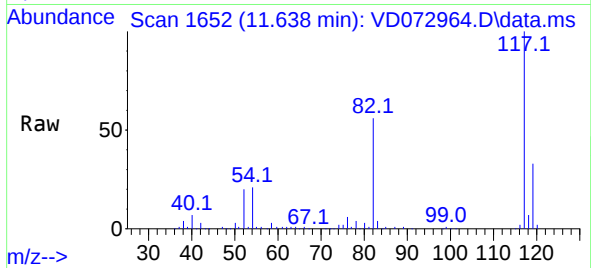

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.000 min
Lab File: VD072964.D
Acq: 12 May 2022 23:09

Tgt Ion:152 Resp: 231285
Ion Ratio Lower Upper
152 100
115 60.5 31.3 93.8
150 157.5 0.0 348.6

