

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051223\
 Data File : VD076105.D
 Acq On : 12 May 2023 13:37
 Operator : KP/SY
 Sample : 02591-22
 Misc : 3.71G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 JREJ7

Quant Time: May 14 23:56:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun May 14 23:54:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	379748	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	359036	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	138262	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.269	65	102822	17.700	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.800%
7) Chloroethane-d5	2.799	69	100478	18.840	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.360%
11) 1,1-Dichloroethene-d2	3.911	65	25155	17.201	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.800%
21) 2-Butanone-d5	6.993	46	35775	45.739	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.480%
24) Chloroform-d	7.569	84	154259	19.389	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	77.560%
26) 1,2-Dichloroethane-d4	8.228	65	71921	20.566	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	82.280%
32) Benzene-d6	8.199	84	285710	17.651	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	70.600%
36) 1,2-Dichloropropane-d6	9.210	67	96739	19.396	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	77.600%
41) Toluene-d8	10.269	98	237942	16.495	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	65.960%
43) trans-1,3-Dichloroprop...	10.528	79	32918	17.582	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.320%
47) 2-Hexanone-d5	10.875	63	26136	35.783	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.560%
56) 1,1,2,2-Tetrachloroeth...	12.651	84	83521	19.446	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	77.800%
66) 1,2-Dichlorobenzene-d4	13.816	152	74019	18.740	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	74.960%#
Target Compounds						Qvalue
16) Methylene chloride	4.793	84	17366	2.812	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051223\
Data File : VD076105.D
Acq On : 12 May 2023 13:37
Operator : KP/SY
Sample : 02591-22
Misc : 3.71G/10.00ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
JREJ7

Quant Time: May 14 23:56:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051123SMA.M
Quant Title : SFAM01.0
QLast Update : Sun May 14 23:54:23 2023
Response via : Initial Calibration

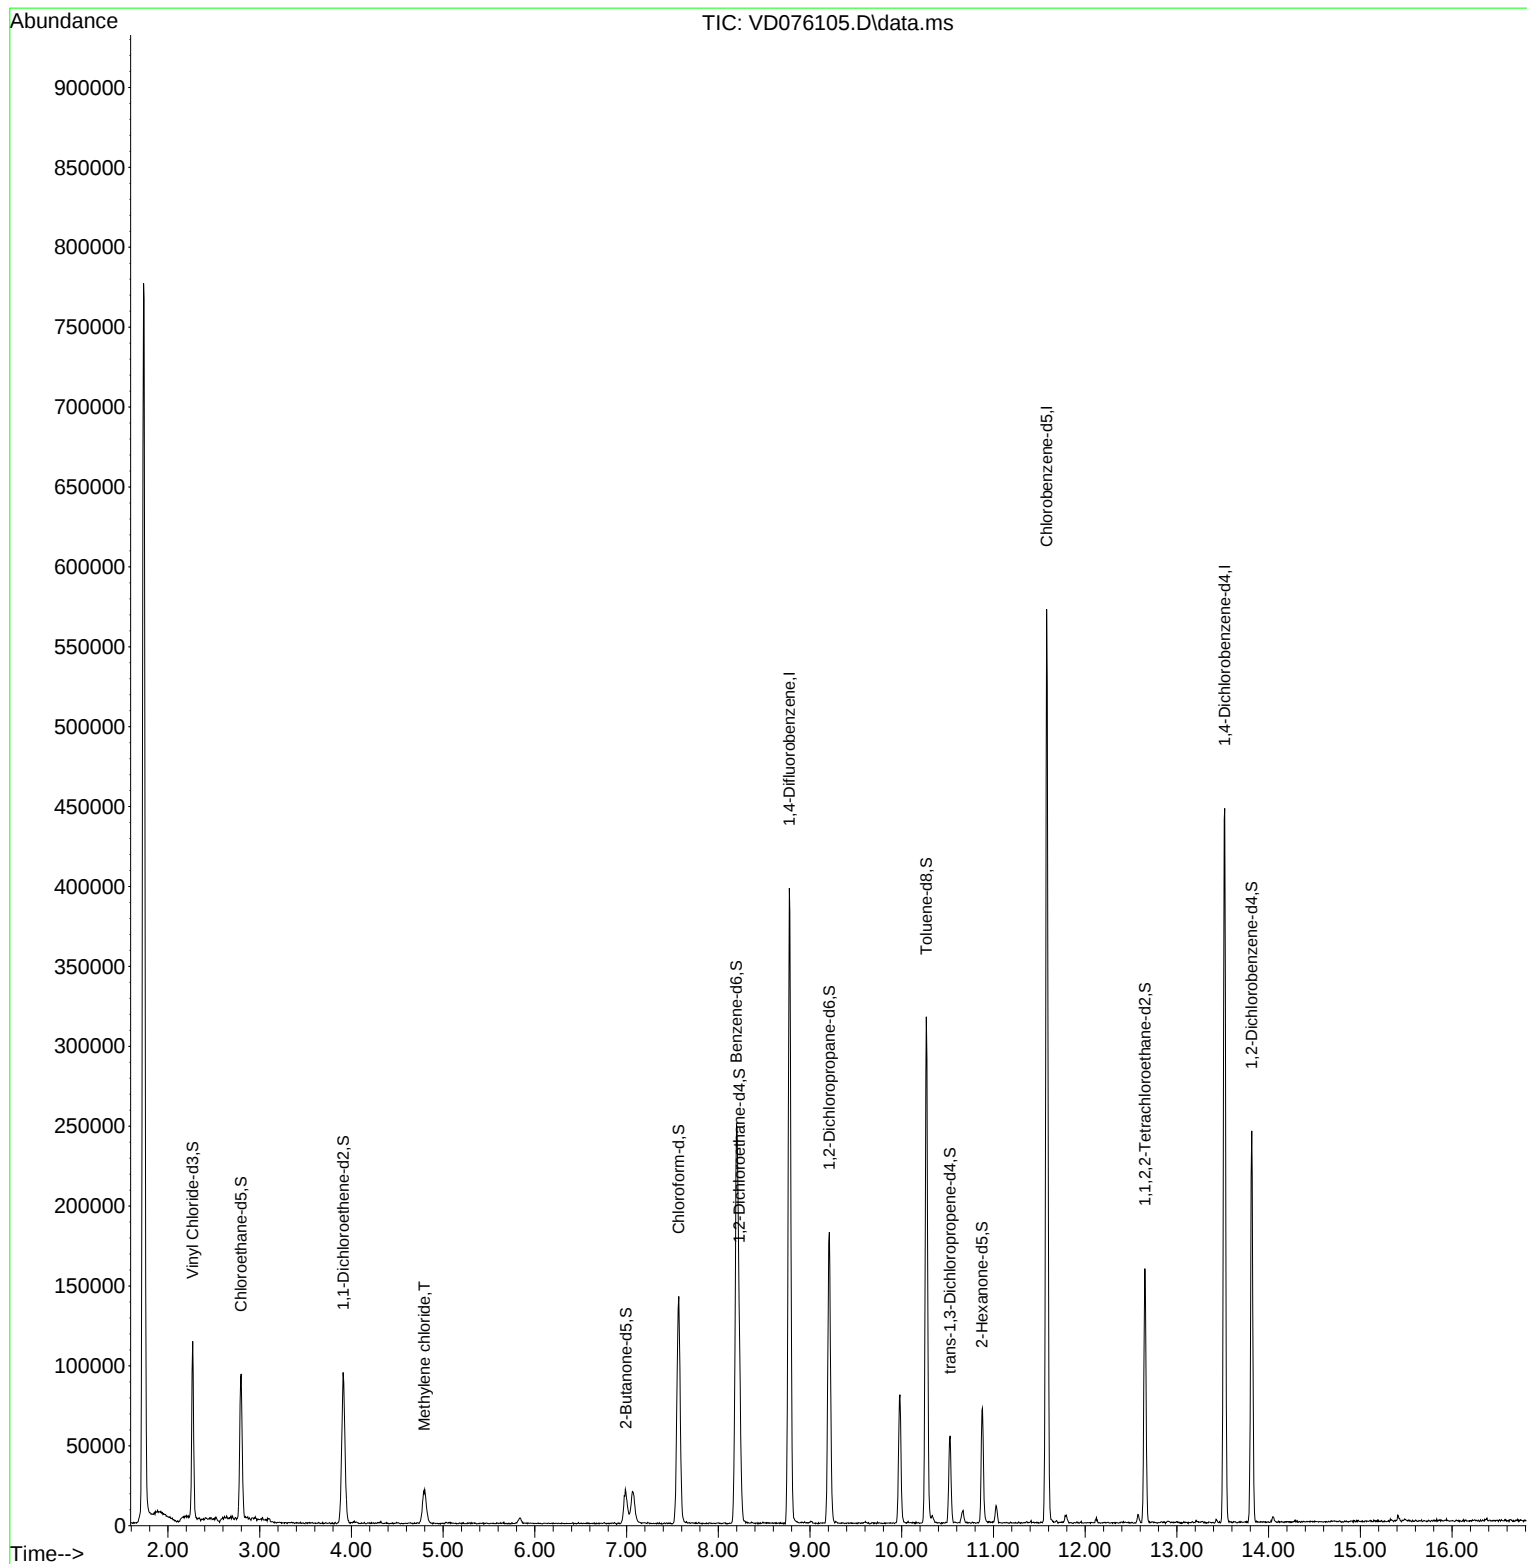

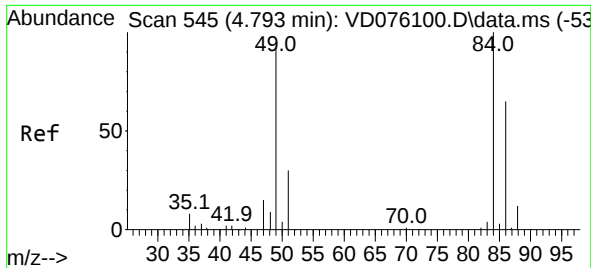

#16
Methylene chloride
Concen: 2.812 ug/L
RT: 4.793 min Scan# 54
Delta R.T. -0.000 min
Lab File: VD076105.D
Acq: 12 May 2023 13:37

Instrument :
MSVOA_D
ClientSampleId :
JREJ7

Tgt Ion: 84 Resp: 17366
Ion Ratio Lower Upper
84 100
86 68.5 45.8 85.2
49 84.6 60.8 112.8

