
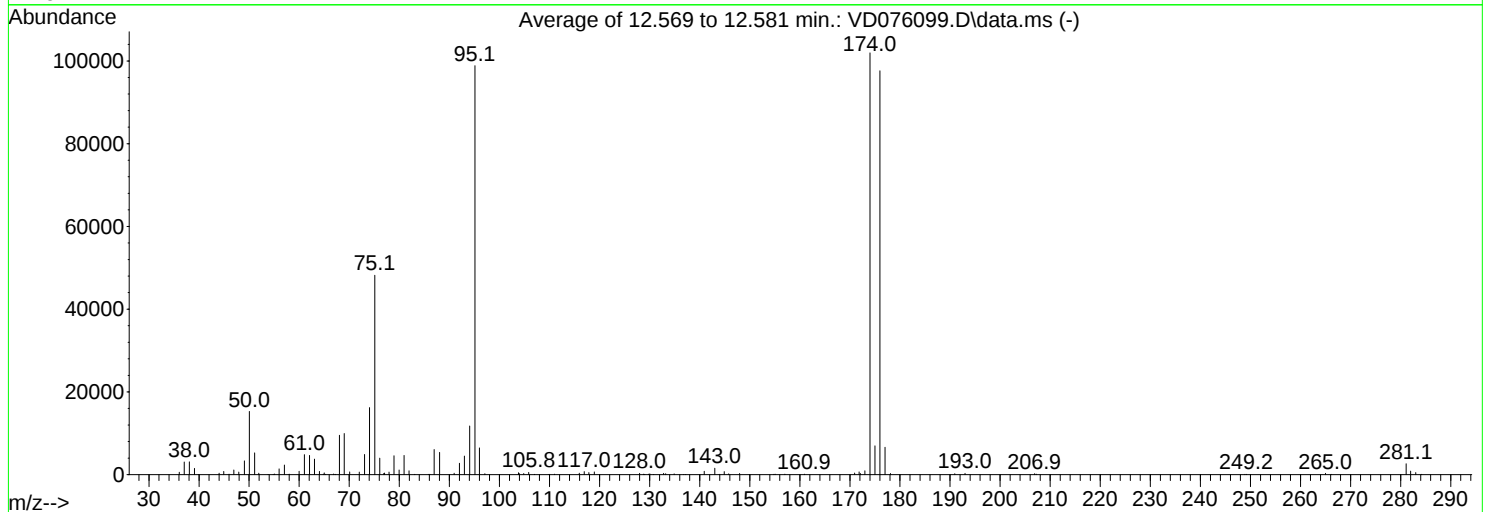


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051223\
 Data File : VD076099.D
 Acq On : 12 May 2023 09:35
 Operator : KP/SY
 Sample : BFB132
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB132

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051123SMA.M
 Title : SFAM01.0
 Last Update : Sun May 14 23:54:23 2023

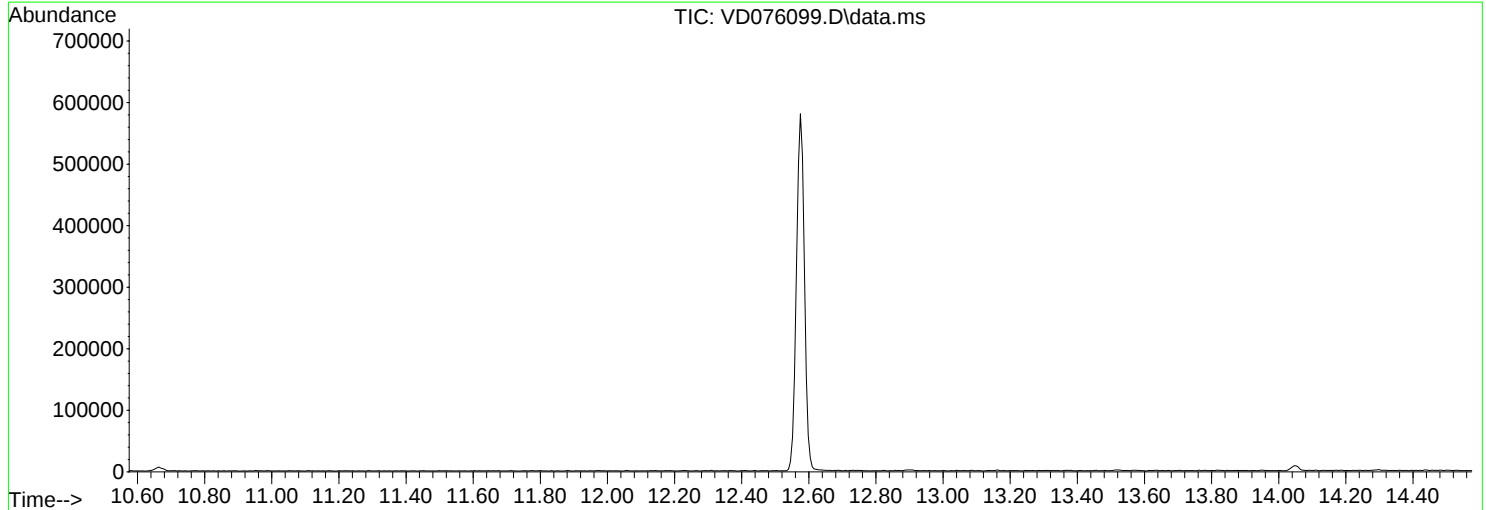

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	15271	PASS
75	95	30	80	48.8	48211	PASS
95	95	100	100	100.0	98845	PASS
96	95	5	9	6.6	6478	PASS
173	174	0.00	2	0.9	919	PASS
174	95	50	120	103.2	101963	PASS
175	174	5	9	6.8	6944	PASS
176	174	95	105	95.7	97608	PASS
177	176	5	10	6.8	6599	PASS

Scan 1860 (12.528 min): VD076099.D\data.ms
BFB132

m/z	Abundance
40.00	1079.0
44.00	686.0

Instrument :
MSVOA_D
ClientSampleId :
BFB132

m/z	Abundance
36.00	627.0
37.10	3148.0
38.00	3199.0
39.10	1729.0
39.90	1003.0
44.00	864.0
45.00	634.0
47.00	950.0
48.00	612.0
49.00	3387.0
50.10	14143.0
51.10	4831.0
52.10	242.0
55.10	420.0
56.10	1322.0
57.10	1743.0
60.00	851.0
61.00	4721.0
62.10	4354.0
63.00	3872.0
64.00	651.0
64.80	380.0
65.30	292.0
66.90	192.0
68.00	8799.0
69.00	10393.0
70.10	795.0
72.00	803.0
73.10	4419.0
74.00	14839.0
75.10	46112.0
76.10	4212.0
76.90	821.0
77.90	492.0
79.00	4994.0
79.90	1046.0
81.00	4780.0
81.90	943.0
86.90	5962.0
88.10	5565.0
90.90	407.0
92.00	2832.0
93.00	4221.0
94.10	11277.0
95.10	94024.0
96.00	6491.0
97.20	230.0
103.80	678.0
104.90	272.0
105.80	409.0
109.90	192.0
116.00	345.0
117.00	600.0
117.80	517.0
119.00	787.0
128.00	221.0
128.80	213.0
130.10	163.0
132.80	215.0
133.20	324.0
135.00	223.0
136.80	166.0
141.00	599.0
143.00	1836.0
144.90	842.0
148.00	260.0
155.10	189.0
170.90	368.0
171.80	943.0
173.00	784.0
174.00	94280.0
175.00	6103.0
176.00	89256.0
177.00	6263.0
178.10	349.0
191.00	199.0
192.90	290.0
206.90	298.0
265.00	255.0
281.10	2056.0
282.00	425.0
283.20	352.0

Instrument :
MSVOA_D
ClientSampleId :
BFB132

m/z	Abundance
36.00	602.0
37.00	3249.0
38.10	3288.0
39.10	1460.0
40.00	1375.0
44.00	1057.0
44.90	997.0
46.00	234.0
46.90	1364.0
47.90	662.0
49.00	3570.0
50.00	18392.0
51.10	6154.0
51.90	428.0
54.80	253.0
55.90	1621.0
57.00	2754.0
58.00	150.0
60.10	749.0
61.00	5340.0
62.10	4786.0
63.00	3898.0
64.00	939.0
65.00	470.0
66.90	300.0
68.00	10658.0
69.00	10592.0
70.20	515.0
72.00	582.0
73.00	5483.0
74.10	18616.0
75.10	52712.0
76.10	4469.0
77.10	722.0
78.00	565.0
78.90	4272.0
80.00	1144.0
80.90	4694.0
82.00	766.0
85.90	294.0
87.00	6856.0
88.00	5660.0
91.00	282.0
92.00	2755.0
93.00	5109.0
94.10	13067.0
95.10	109200.0
96.00	6511.0
97.10	272.0
103.80	686.0
104.90	287.0
105.90	664.0
111.00	336.0
116.00	394.0
117.00	843.0
117.90	494.0
118.90	645.0
128.10	400.0
128.80	167.0
130.00	407.0
130.80	172.0
132.80	357.0
134.90	155.0
137.20	157.0
140.90	1126.0
143.00	1877.0
143.90	182.0
144.90	771.0
145.80	279.0
147.90	193.0
154.80	284.0
160.90	259.0
171.00	434.0
171.90	1014.0
173.00	1246.0
174.00	112456.0
175.00	7605.0
176.00	105048.0
177.00	6769.0
178.10	254.0
190.90	297.0
193.00	205.0
207.20	392.0
249.20	280.0
265.00	320.0
281.10	2809.0
282.00	1100.0
283.00	599.0

Instrument :
MSVOA_D
ClientSampleId :
BFB132

m/z	Abundance
36.10	572.0
37.00	2765.0
38.00	2777.0
39.10	1317.0
40.00	955.0
44.00	1247.0
45.00	727.0
46.00	178.0
47.00	1026.0
47.90	570.0
49.10	3032.0
50.00	13278.0
51.10	4771.0
52.00	399.0
53.80	159.0
56.00	1260.0
57.00	2466.0
58.00	152.0
59.90	806.0
61.10	4441.0
62.00	4761.0
63.10	3480.0
64.10	698.0
65.00	820.0
67.20	212.0
68.10	9097.0
69.00	8899.0
70.00	629.0
72.10	440.0
73.10	4713.0
74.00	15148.0
75.10	45808.0
76.10	3337.0
77.00	443.0
77.90	796.0
78.90	4462.0
80.00	1199.0
80.90	4480.0
81.90	1037.0
83.10	297.0
86.10	222.0
87.00	5433.0
88.00	4962.0
91.00	407.0
92.00	2636.0
93.00	4117.0
94.00	10877.0
95.10	93312.0
96.00	6432.0
97.00	169.0
104.00	677.0
104.80	237.0
105.90	606.0
107.00	230.0
108.00	171.0
115.90	303.0
116.90	796.0
117.90	545.0
118.90	568.0
127.90	364.0
129.00	263.0
129.80	343.0
132.80	404.0
133.20	350.0
134.80	195.0
140.80	709.0
143.10	940.0
144.90	560.0
145.80	273.0
148.00	374.0
149.90	163.0
155.00	197.0
157.00	351.0
160.90	158.0
171.00	420.0
172.10	778.0
173.00	727.0
174.00	99152.0
175.00	7123.0
176.00	98520.0
177.00	6766.0
178.10	239.0
190.90	186.0
193.10	472.0
206.90	450.0
248.90	228.0
265.00	333.0
266.10	226.0
281.10	3081.0
282.00	1057.0
282.90	558.0
284.20	273.0

Instrument :
MSVOA_D
ClientSampleId :
BFB132