


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD051319\
 Data File : VD062294.D
 Acq On : 13 May 2019 9:44
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D050719S.M
 Title : SW846 8260
 Last Update : Tue May 07 14:26:29 2019

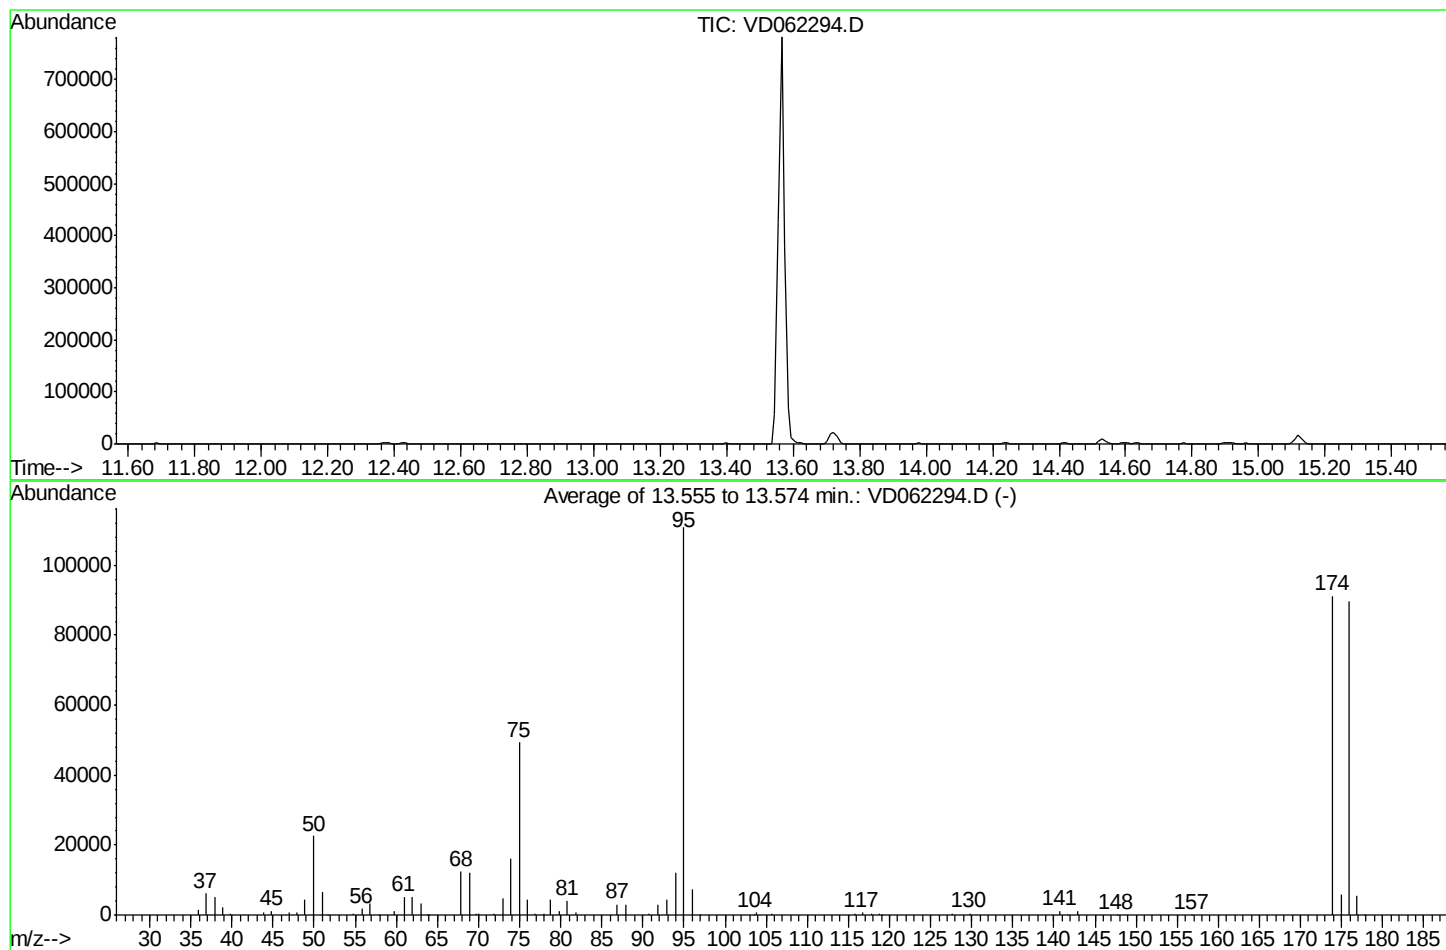

AutoFind: Scans 1233, 1234, 1235; Background Corrected with Scan 1228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	22654	PASS
75	95	30	60	44.4	49250	PASS
95	95	100	100	100.0	110856	PASS
96	95	5	9	6.8	7490	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.2	91170	PASS
175	174	5	9	6.5	5936	PASS
176	174	95	101	98.6	89861	PASS
177	176	5	9	6.3	5671	PASS