
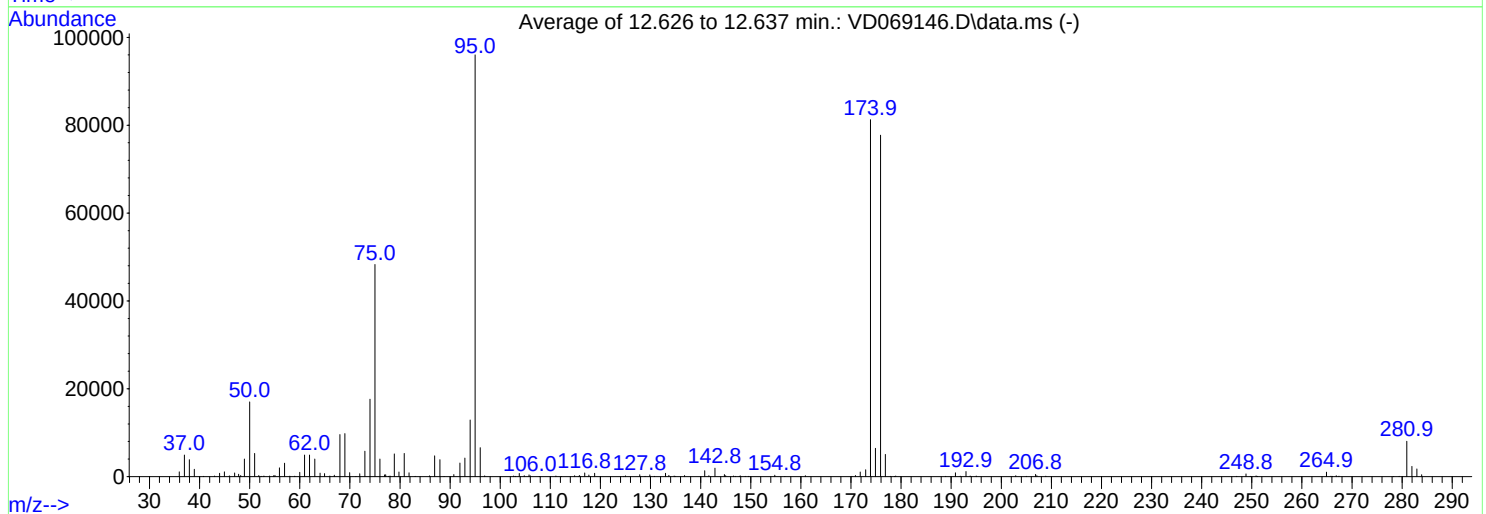


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051321\
Data File : VD069146.D
Acq On : 13 May 2021 09:40
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051221S.M
Title : SW846 8260
Last Update : Thu May 13 04:01:29 2021

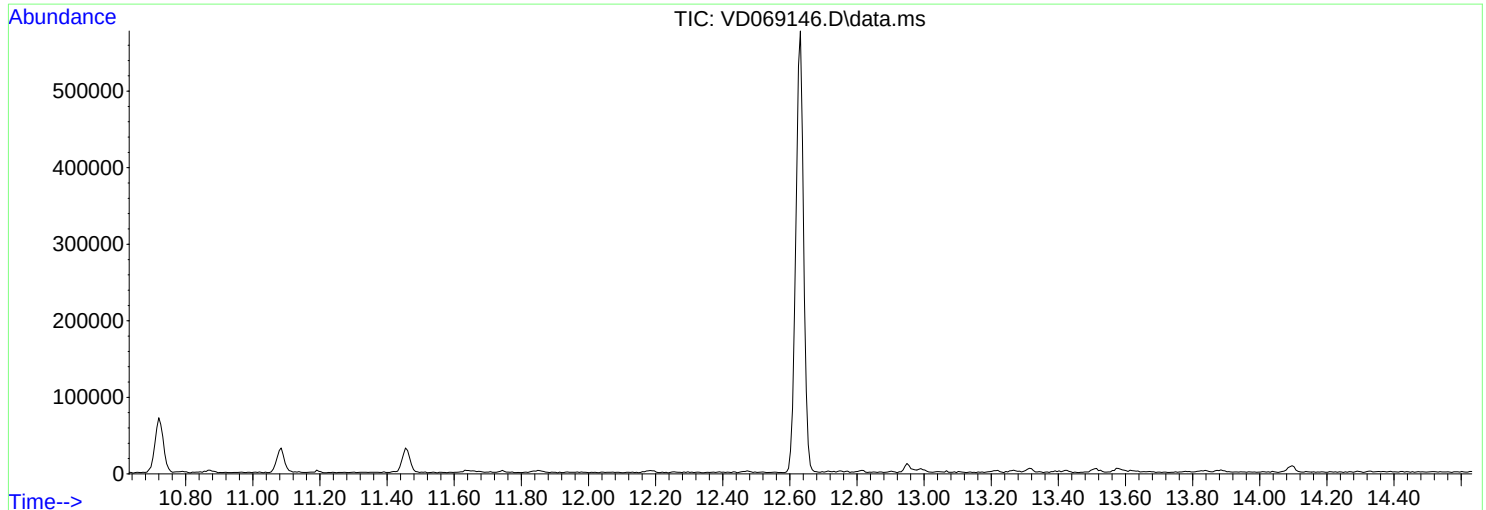

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	17008	PASS
75	95	30	60	50.3	48315	PASS
95	95	100	100	100.0	96021	PASS
96	95	5	9	6.9	6585	PASS
173	174	0.00	2	1.9	1576	PASS
174	95	50	100	84.6	81277	PASS
175	174	5	9	7.9	6458	PASS
176	174	95	101	95.6	77723	PASS
177	176	5	9	6.5	5056	PASS