

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051322\
 Data File : VD073025.D
 Acq On : 14 May 2022 09:07
 Operator : VA/SY
 Sample : N2823-11
 Misc : 5.09G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SC-11

Quant Time: May 16 05:22:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050222S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 03 08:33:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	377311	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	669847	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	666391	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	307454	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	195429	39.901	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	79.800%
35) Dibromofluoromethane	7.908	113	213709	45.427	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	90.860%
50) Toluene-d8	10.332	98	813028	48.179	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	96.360%
62) 4-Bromofluorobenzene	12.620	95	299993	47.676	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	95.360%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051322\
Data File : VD073025.D
Acq On : 14 May 2022 09:07
Operator : VA/SY
Sample : N2823-11
Misc : 5.09G/5.00ml/MSVOA_D/SOIL
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SC-11

Quant Time: May 16 05:22:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050222S.M
Quant Title : SW846 8260
QLast Update : Tue May 03 08:33:49 2022
Response via : Initial Calibration




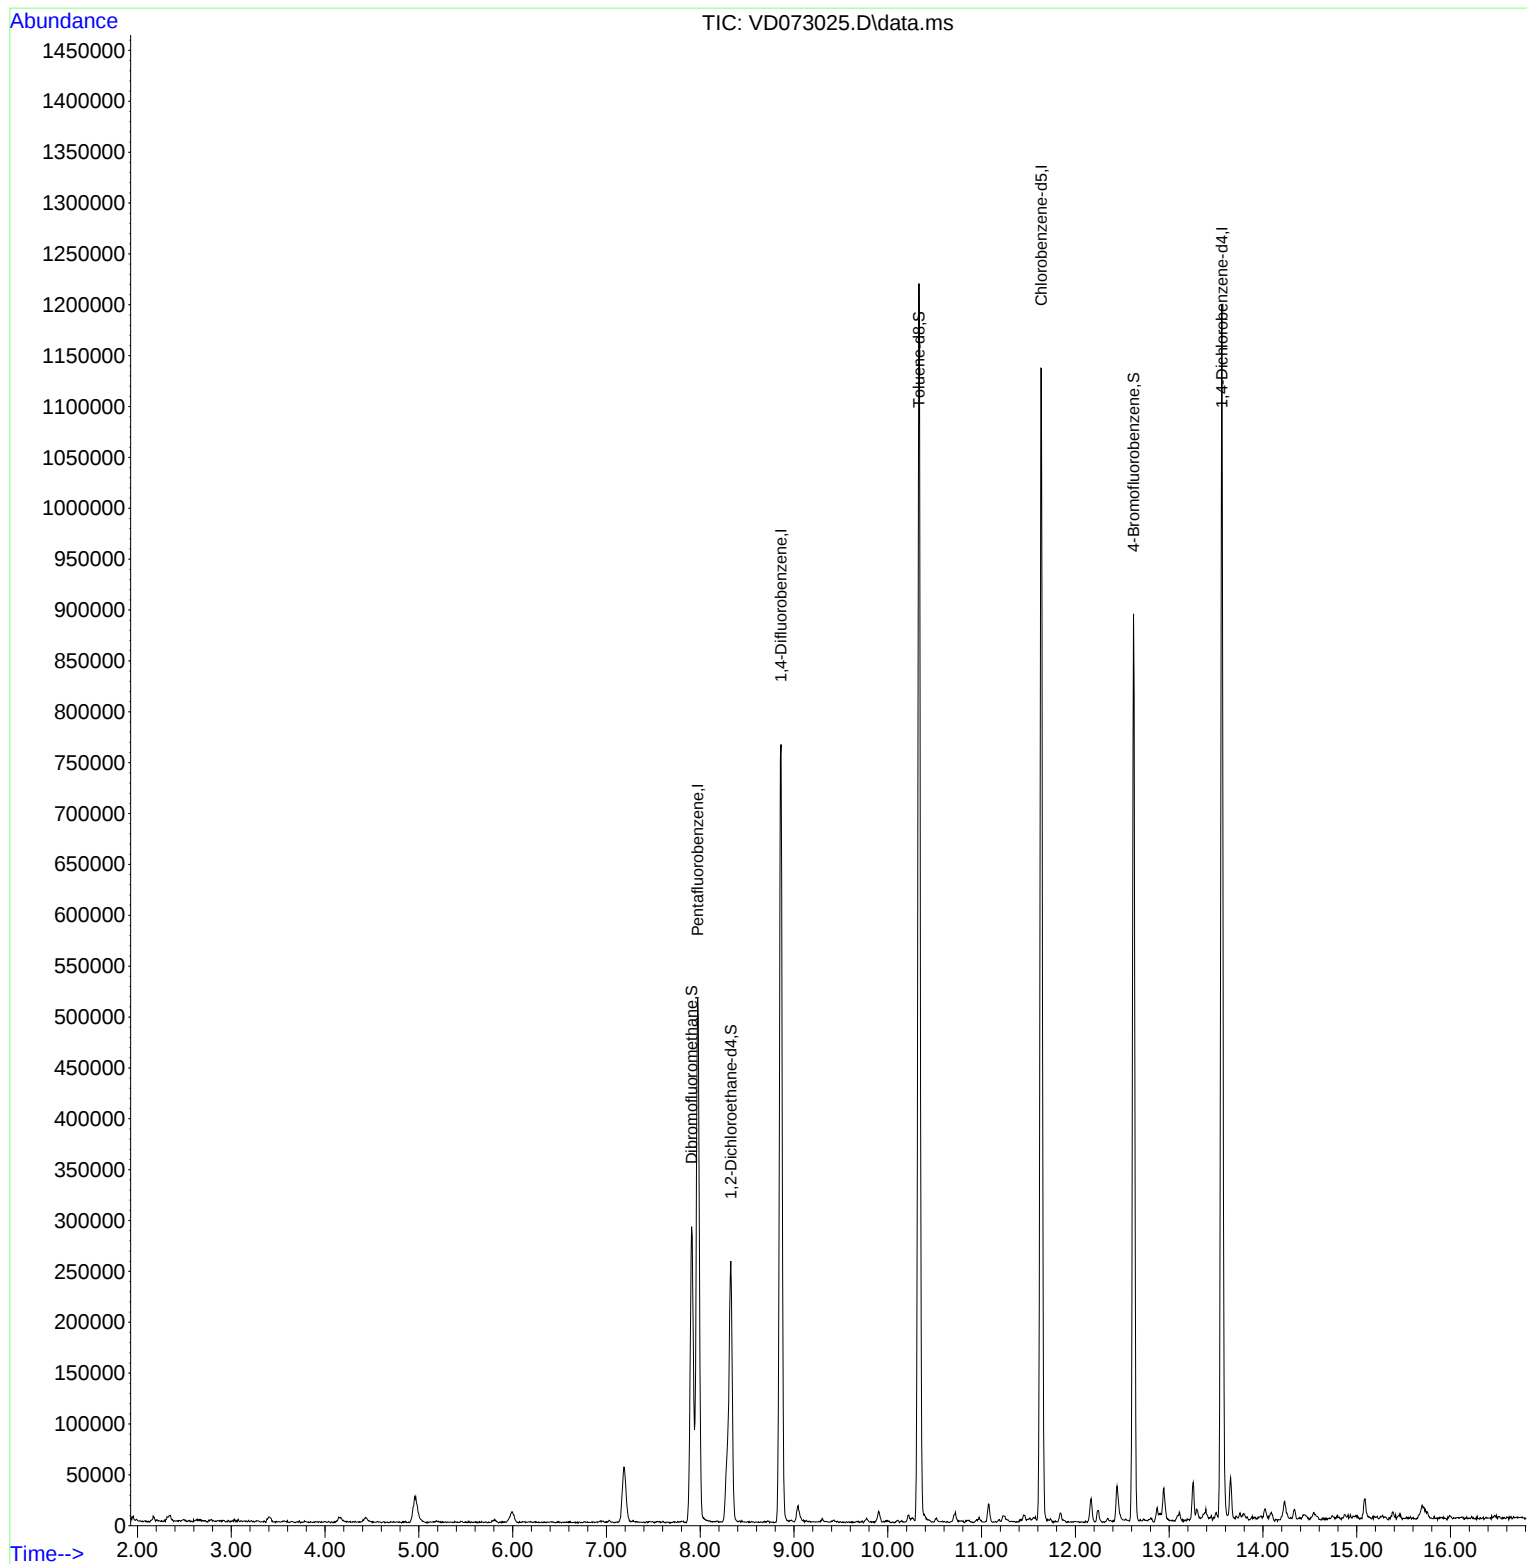




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. -0.006 min
Lab File: VD073025.D
Acq: 14 May 2022 09:07




Instrument :
MSVOA_D
ClientSampleId :
SC-11

Tgt Ion:168 Resp: 377311
Ion Ratio Lower Upper
168 100
99 59.7 49.8 74.6

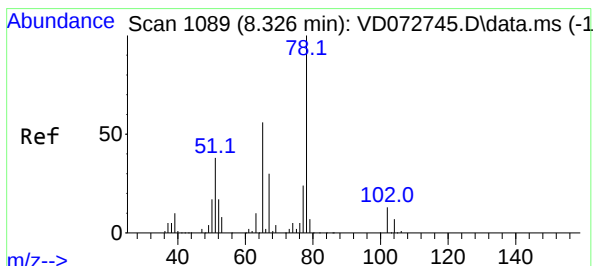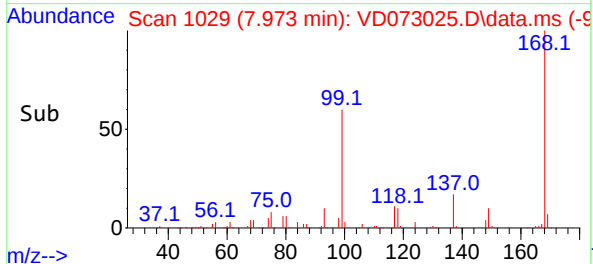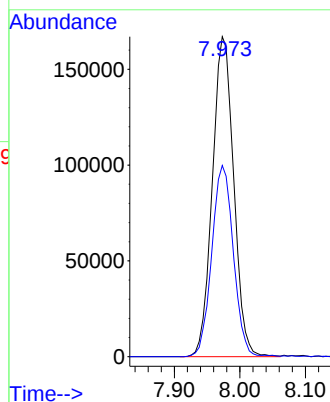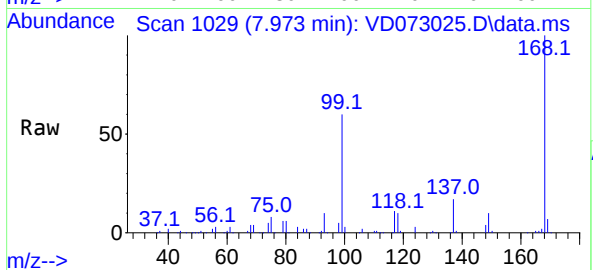

#33
1,2-Dichloroethane-d4
Concen: 39.901 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. 0.000 min
Lab File: VD073025.D
Acq: 14 May 2022 09:07

Tgt Ion: 65 Resp: 195429
Ion Ratio Lower Upper
65 100
67 54.0 0.0 101.4

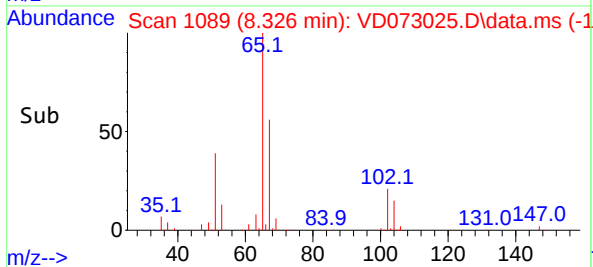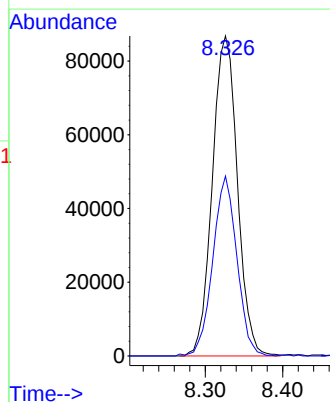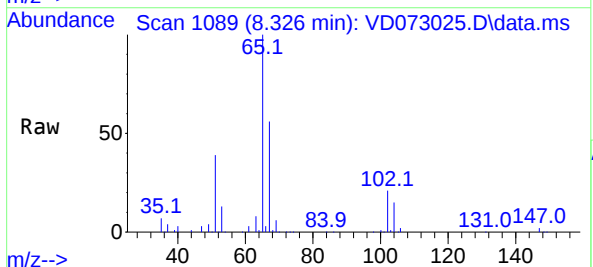



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.861 min Scan# 1180

Delta R.T. 0.000 min

Lab File: VD073025.D

Acq: 14 May 2022 09:07

Instrument :

MSVOA_D

ClientSampleId :

SC-11





Tgt Ion:114 Resp: 669847

Ion Ratio Lower Upper

114 100

63 21.3 0.0 46.6

88 14.9 0.0 33.2

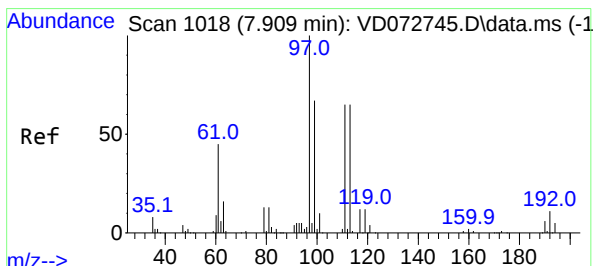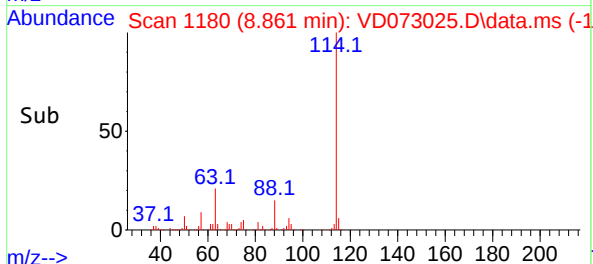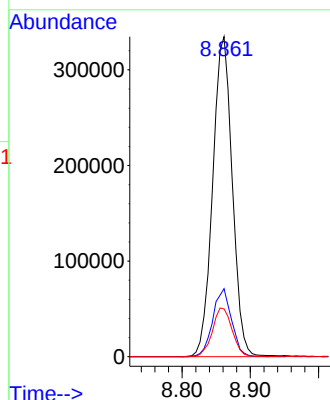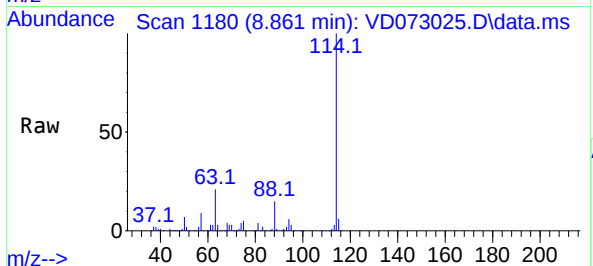

#35

Dibromofluoromethane

Concen: 45.427 ug/l

RT: 7.908 min Scan# 1018

Delta R.T. -0.001 min

Lab File: VD073025.D

Acq: 14 May 2022 09:07




Tgt Ion:113 Resp: 213709


Ion Ratio Lower Upper

113 100

111 102.2 83.8 125.6

192 17.9 14.6 21.8

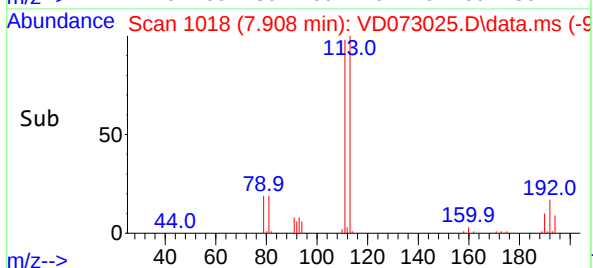
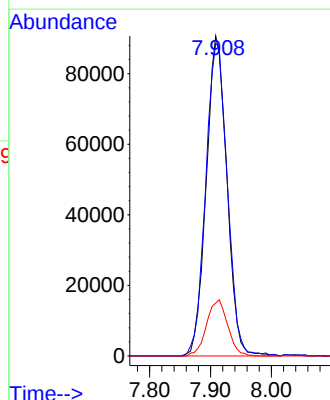
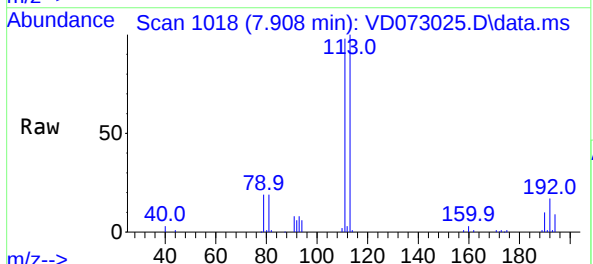


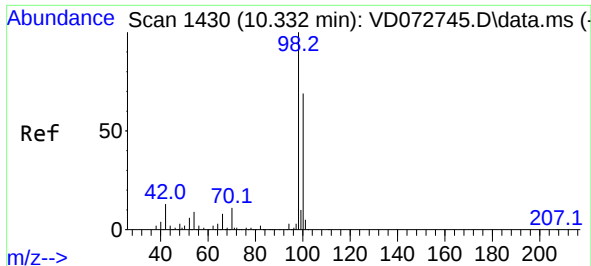

#50
Toluene-d8
Concen: 48.179 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD073025.D
Acq: 14 May 2022 09:07




Instrument :
MSVOA_D
ClientSampleId :
SC-11


Tgt Ion: 98 Resp: 813028
Ion Ratio Lower Upper
98 100
100 66.0 52.4 78.6

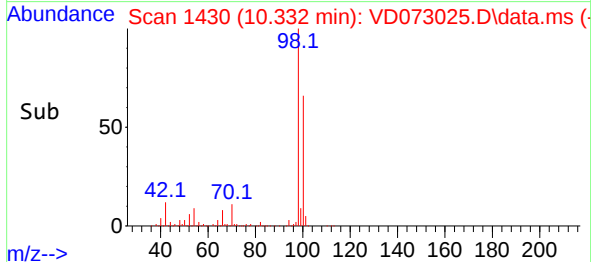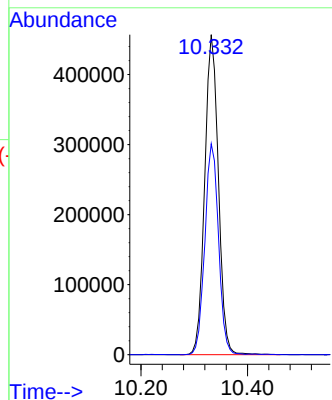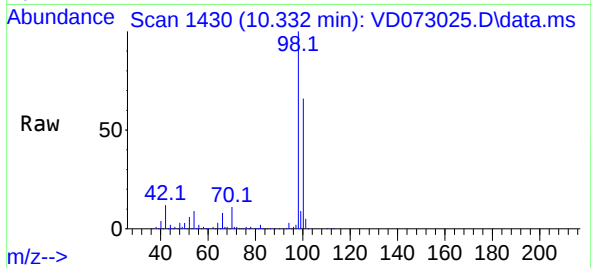

#62
4-Bromofluorobenzene
Concen: 47.676 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. 0.000 min
Lab File: VD073025.D
Acq: 14 May 2022 09:07

Tgt Ion: 95 Resp: 299993
Ion Ratio Lower Upper
95 100
174 76.6 0.0 152.8
176 72.0 0.0 145.4


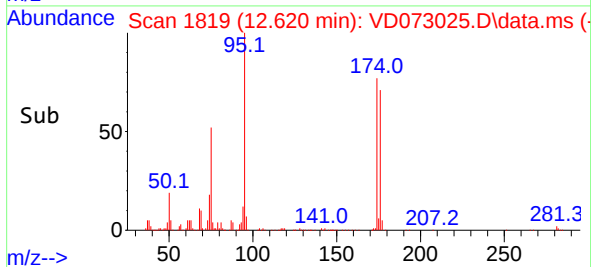
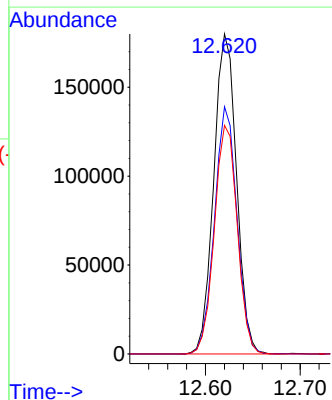
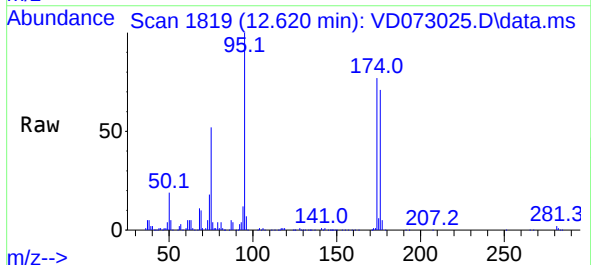


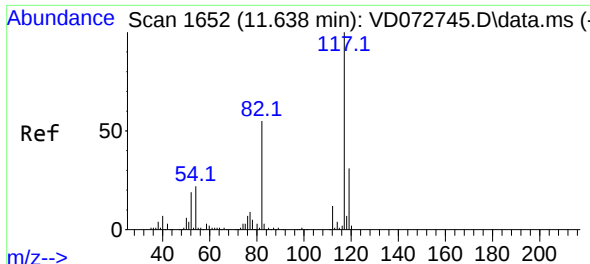

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. -0.000 min
Lab File: VD073025.D
Acq: 14 May 2022 09:07

Instrument :
MSVOA_D
ClientSampleId :
SC-11

Tgt Ion:117 Resp: 666391
Ion Ratio Lower Upper
117 100
82 54.4 45.3 67.9
119 32.2 26.6 40.0

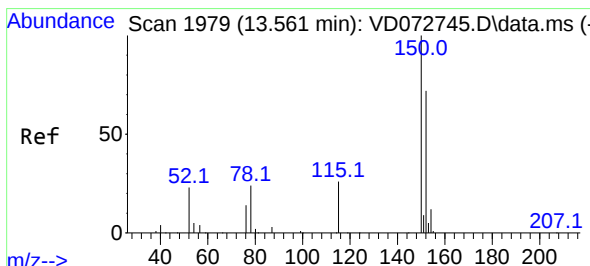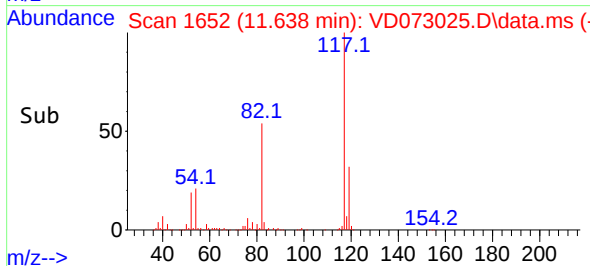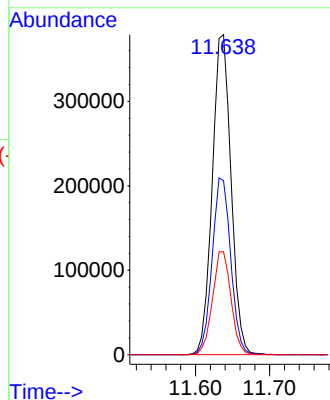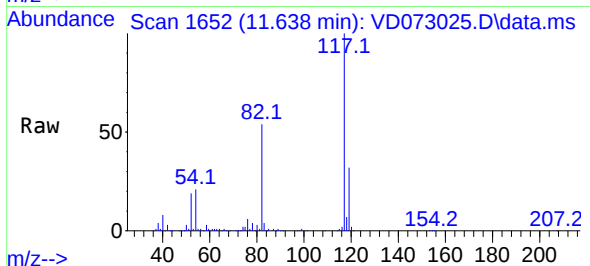

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.000 min
Lab File: VD073025.D
Acq: 14 May 2022 09:07

Tgt Ion:152 Resp: 307454
Ion Ratio Lower Upper
152 100
115 60.6 31.3 93.8
150 156.9 0.0 348.6

