
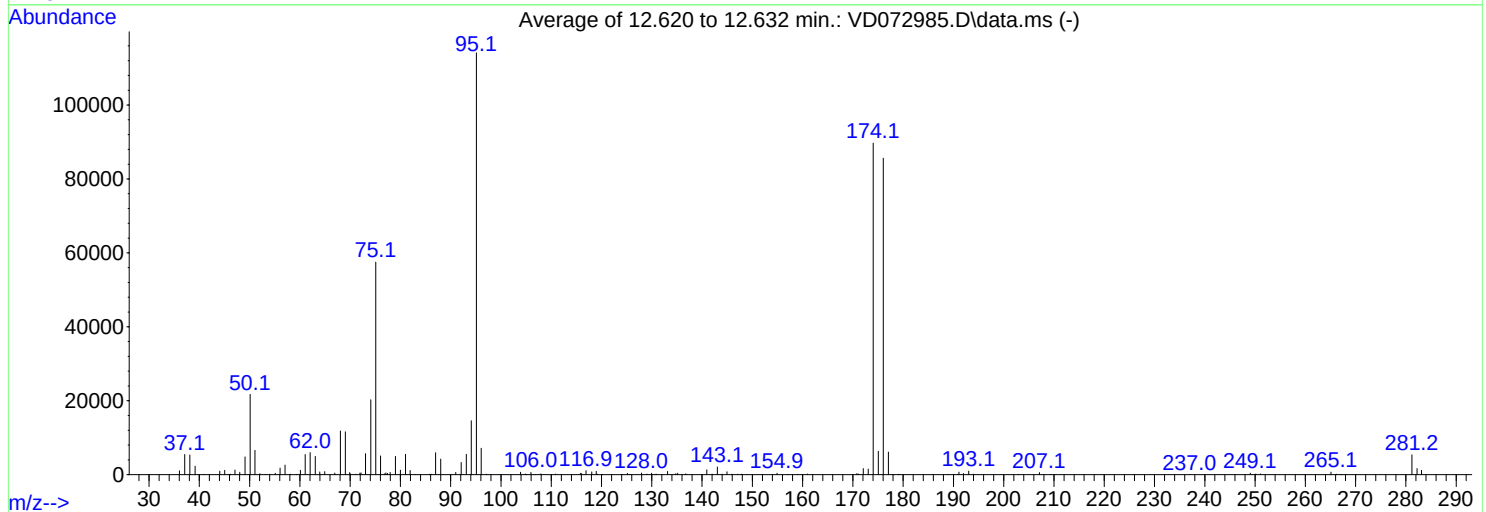


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051322\
Data File : VD072985.D
Acq On : 13 May 2022 12:36
Operator : VA/SY
Sample : BFB
Misc : 5.00 G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050222S.M
Title : SW846 8260
Last Update : Tue May 03 08:33:49 2022

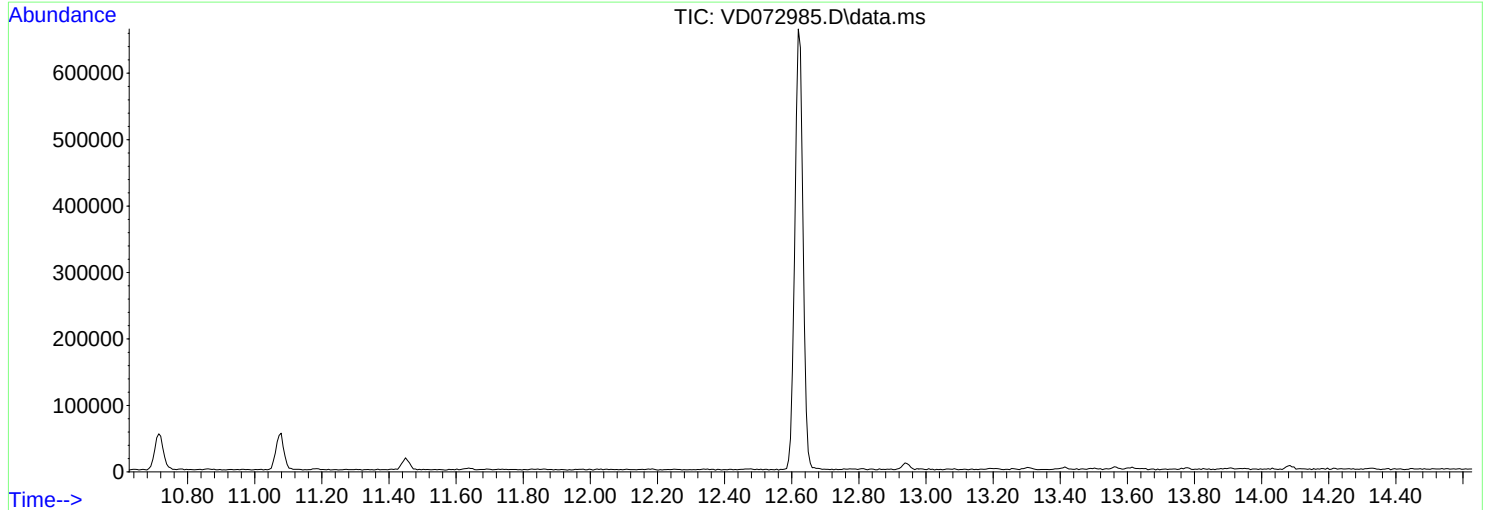

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	21717	PASS
75	95	30	60	50.4	57491	PASS
95	95	100	100	100.0	114123	PASS
96	95	5	9	6.3	7149	PASS
173	174	0.00	2	1.7	1529	PASS
174	95	50	100	78.6	89680	PASS
175	174	5	9	7.1	6323	PASS
176	174	95	101	95.5	85613	PASS
177	176	5	9	7.1	6090	PASS