

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_D\DATA\VD051419\
 Data File : VD062365.D
 Acq On : 15 May 2019 1:14
 Operator : FY/SY
 Sample : K2756-11RE
 Misc : 6.09g/5mL/MSVOA_D/SOIL
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 P021-SS007-0002-01RE

Quant Time: May 15 03:44:39 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D050719S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 07 14:26:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.07	168	46517	50.00	ug/l	0.04
34) 1,4-Difluorobenzene	8.23	114	84001	50.00	ug/l	0.03
63) Chlorobenzene-d5	12.38	117	75362	50.00	ug/l	0.02
72) 1,4-Dichlorobenzene-d4	14.52	152	37373	50.00	ug/l	0.01

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.47	65	50635	117.13	ug/l	0.04
Spiked Amount	50.000		Recovery	=	234.26%	
35) Dibromofluoromethane	6.94	113	39602	56.82	ug/l	0.04
Spiked Amount	50.000		Recovery	=	113.64%	
50) Toluene-d8	10.42	98	56029	33.34	ug/l	0.02
Spiked Amount	50.000		Recovery	=	66.68%	
62) 4-Bromofluorobenzene	13.56	95	29822	44.19	ug/l	0.01
Spiked Amount	50.000		Recovery	=	88.38%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_D\DATA\VD051419\
Data File : VD062365.D
Acq On : 15 May 2019 1:14
Operator : FY/SY
Sample : K2756-11RE
Misc : 6.09g/5mL/MSVOA_D/SOIL
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
P021-SS007-0002-01RE

Quant Time: May 15 03:44:39 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D050719S.M
Quant Title : SW846 8260
QLast Update : Tue May 07 14:26:29 2019
Response via : Initial Calibration

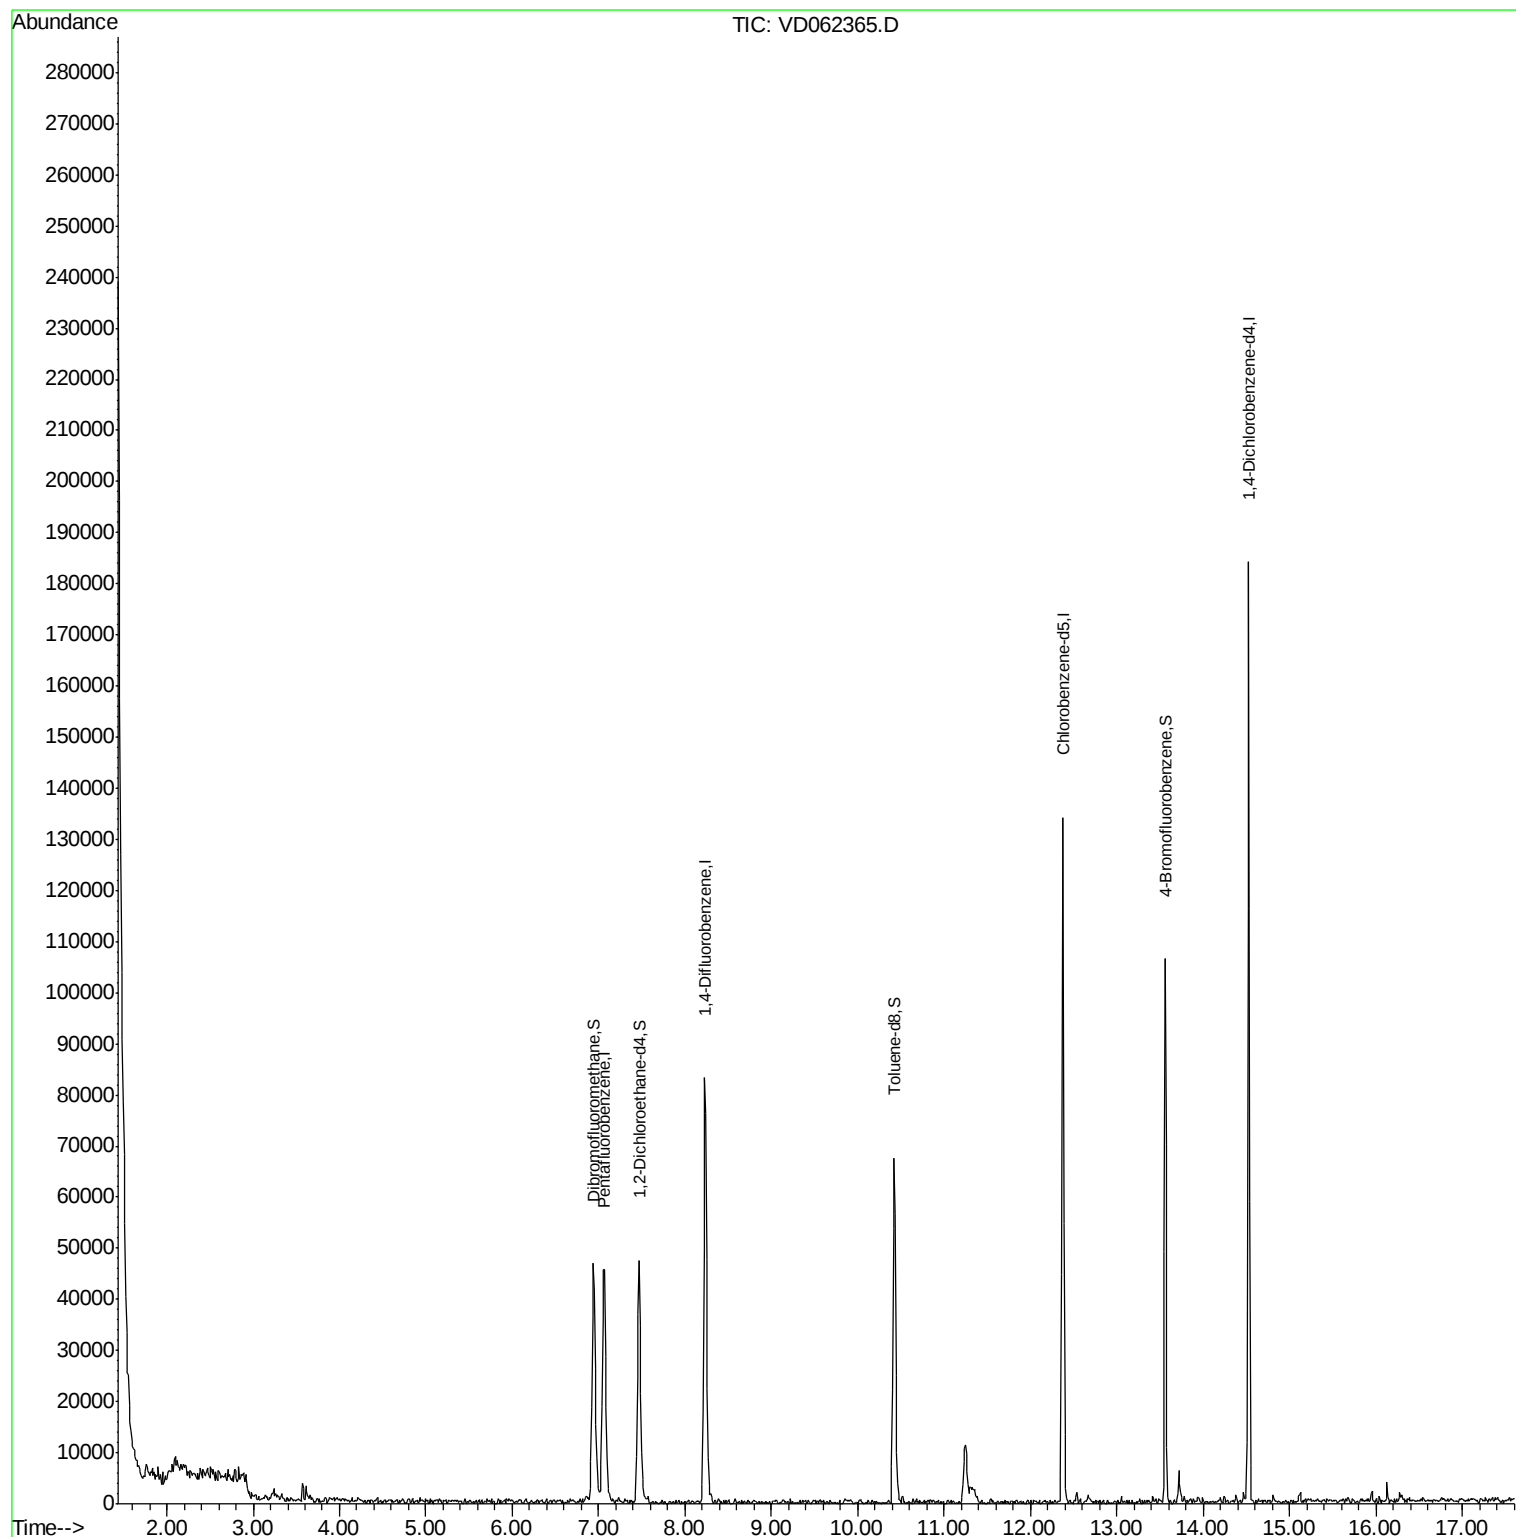

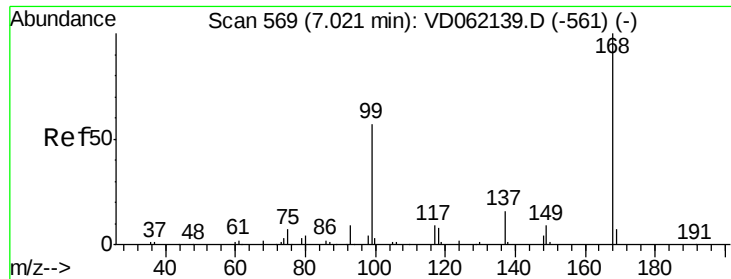

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.07 min Scan# 573

Delta R.T. 0.04 min

Lab File: VD062365.D

Acq: 15 May 2019 1:14

Instrument :

MSVOA_D

ClientSampleId :


P021-SS007-0002-01RE

Tgt Ion:168 Resp: 46517

Ion Ratio Lower Upper


168 100

99 57.5 46.5 69.7


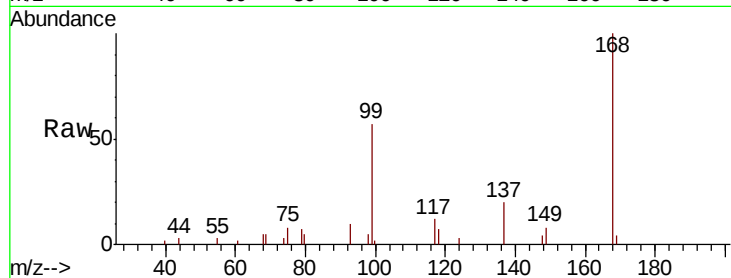


Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

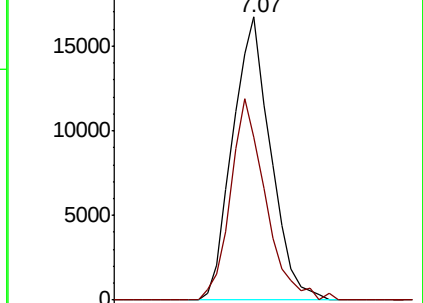

Time-->

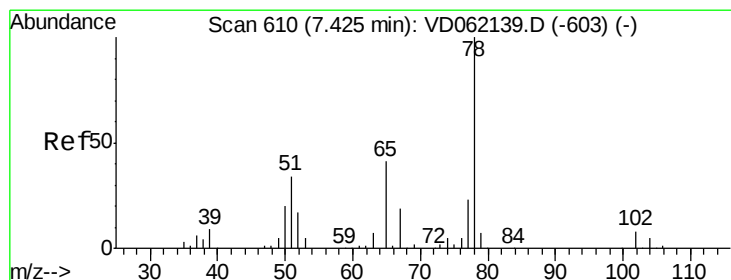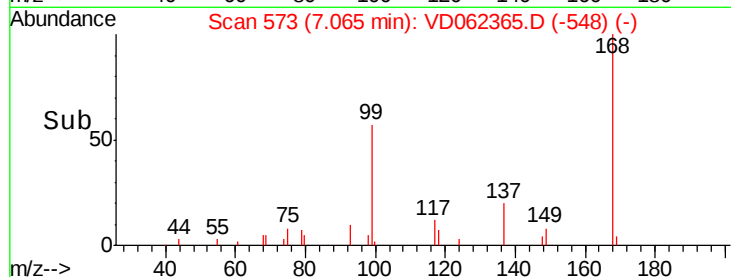

#33

1,2-Dichloroethane-d4

Concen: 117.132 ug/l

RT: 7.47 min Scan# 614

Delta R.T. 0.04 min

Lab File: VD062365.D


Acq: 15 May 2019 1:14

Tgt Ion: 65 Resp: 50635

Ion Ratio Lower Upper


65 100

67 42.7 0.0 98.0

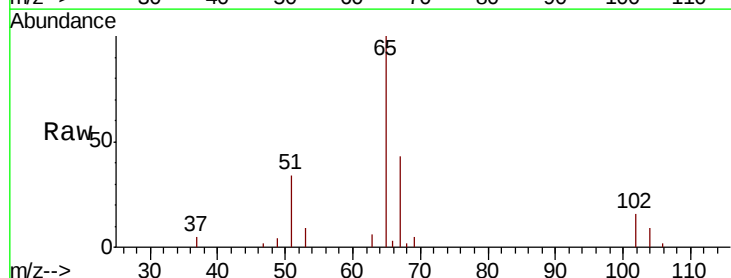



Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC

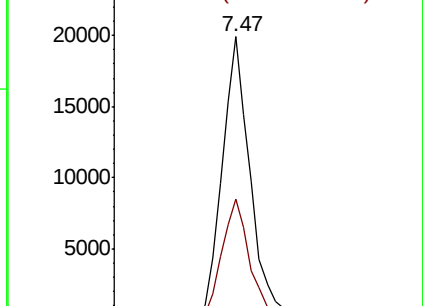

Time-->

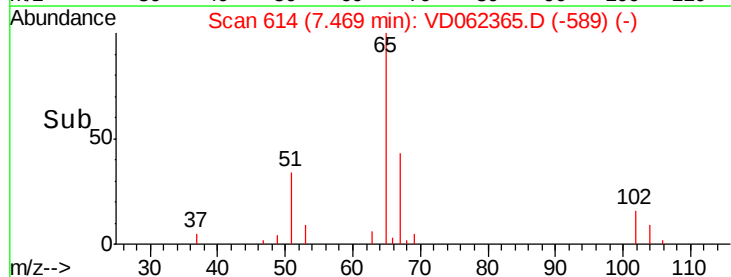


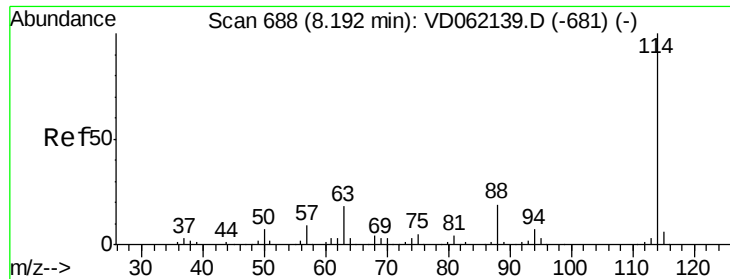




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.23 min Scan# 691
 Delta R.T. 0.03 min
 Lab File: VD062365.D
 Acq: 15 May 2019 1:14

Instrument :
 MSVOA_D
 ClientSampleId :
 P021-SS007-0002-01RE

Tgt Ion:114 Resp: 84001
 Ion Ratio Lower Upper
 114 100
 63 19.2 0.0 32.4
 88 19.7 0.0 33.6

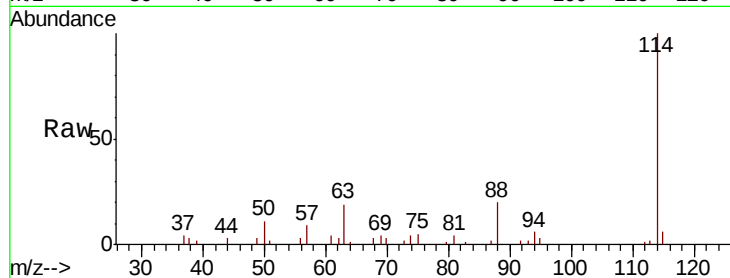


Abundance Ion 114.00 (113.70 to 114.70): V
 Ion 62.95 (62.65 to 63.65): V
 Ion 87.90 (87.60 to 88.60): V

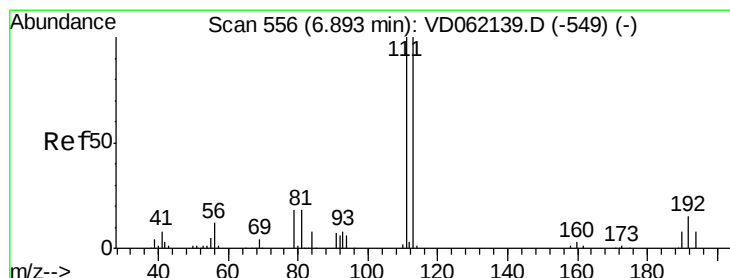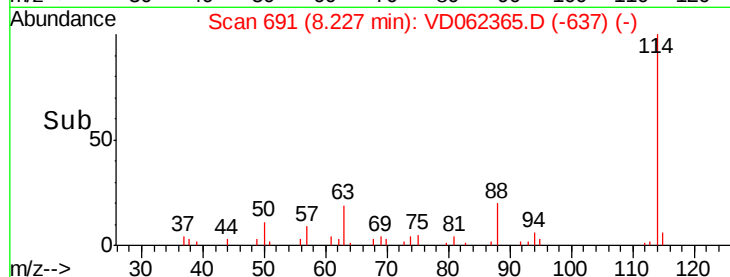
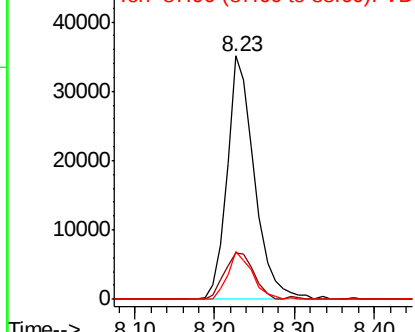



#35
 Dibromofluoromethane
 Concen: 56.821 ug/l
 RT: 6.94 min Scan# 560
 Delta R.T. 0.04 min
 Lab File: VD062365.D
 Acq: 15 May 2019 1:14

Tgt Ion:113 Resp: 39602
 Ion Ratio Lower Upper
 113 100
 111 88.6 78.5 117.7
 192 13.3 13.0 19.4

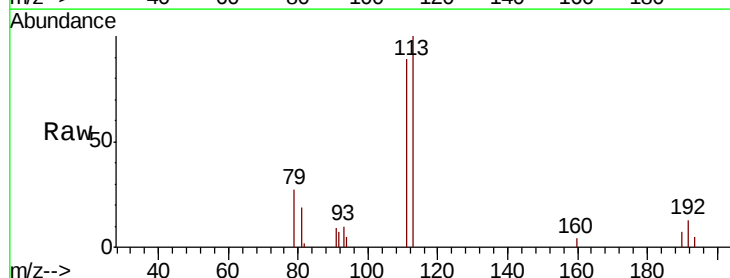

Abundance Ion 112.90 (112.60 to 113.60): V
 Ion 110.90 (110.60 to 111.60): V
 Ion 191.80 (191.50 to 192.50): V

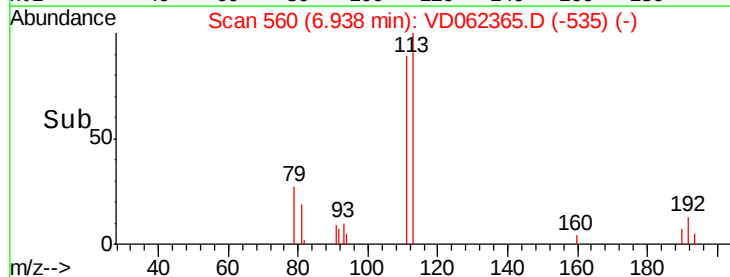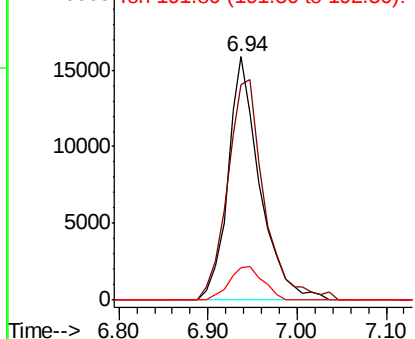

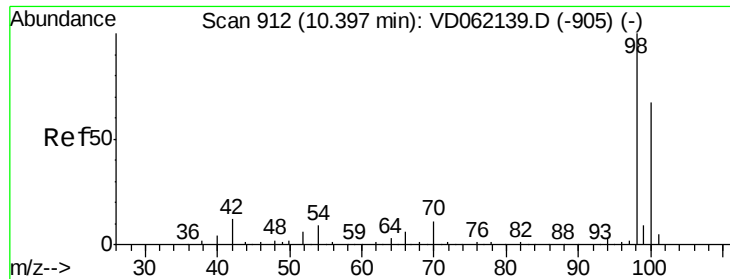

#50

Toluene-d8

Concen: 33.342 ug/l

RT: 10.42 min Scan# 914

Delta R.T. 0.02 min

Lab File: VD062365.D

Acq: 15 May 2019 1:14

Instrument :

MSVOA_D

ClientSampleId :


P021-SS007-0002-01RE

Tgt Ion: 98 Resp: 56029

Ion Ratio Lower Upper




98 100

100 66.0 53.8 80.8

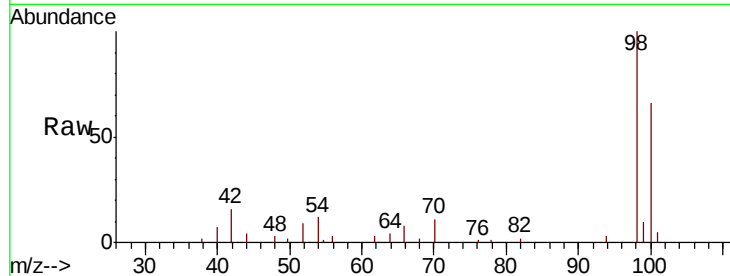

Abundance Ion 98.05 (97.75 to 98.75): VD062139.D (-905) (-)

Ion 100.05 (99.75 to 100.75): VD062139.D (-905) (-)

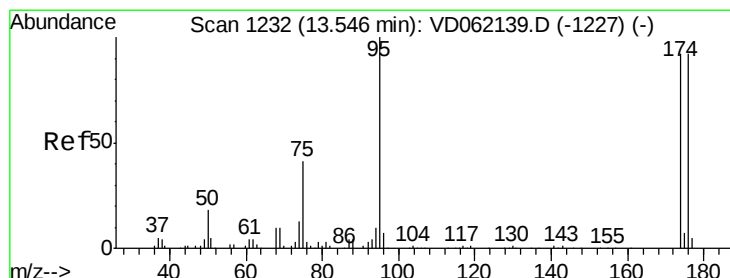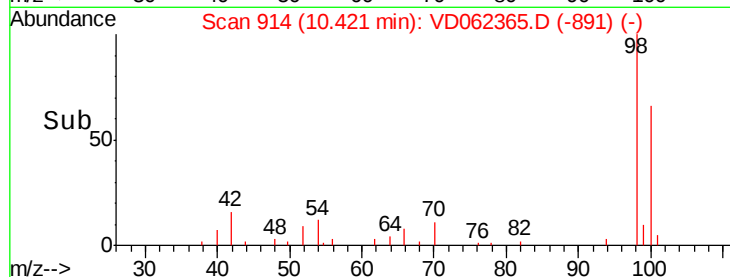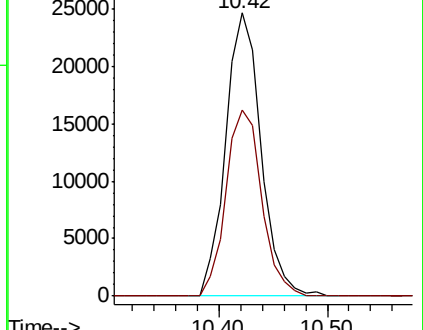

#62

4-Bromofluorobenzene

Concen: 44.194 ug/l

RT: 13.56 min Scan# 1233

Delta R.T. 0.01 min

Lab File: VD062365.D

Acq: 15 May 2019 1:14


Tgt Ion: 95 Resp: 29822

Ion Ratio Lower Upper

95 100

174 90.8 0.0 181.8



176 93.8 0.0 174.4

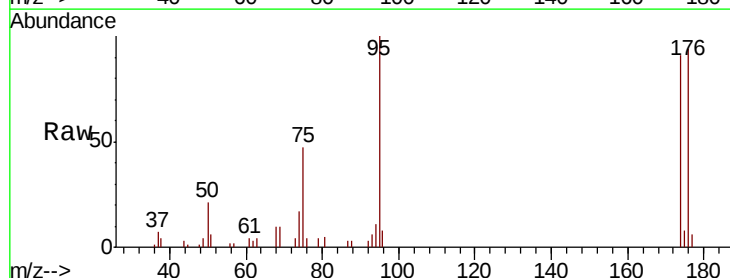


Abundance Ion 95.00 (94.70 to 95.70): VD062139.D (-1227) (-)

Ion 173.90 (173.60 to 174.60): VD062139.D (-1227) (-)

Ion 175.90 (175.60 to 176.60): VD062139.D (-1227) (-)

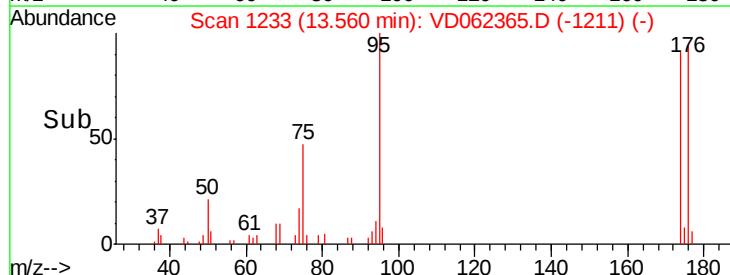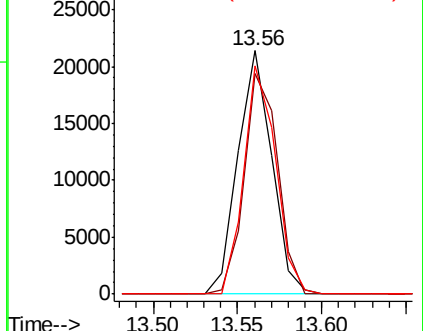


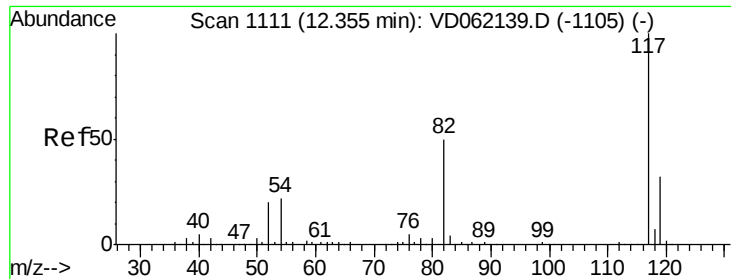




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 12.38 min Scan# 1113
Delta R.T. 0.02 min
Lab File: VD062365.D
Acq: 15 May 2019 1:14

Instrument :
MSVOA_D
ClientSampleId :
P021-SS007-0002-01RE

Tgt Ion:117 Resp: 75362
Ion Ratio Lower Upper
117 100
82 57.4 36.2 54.2#
119 30.3 26.2 39.4

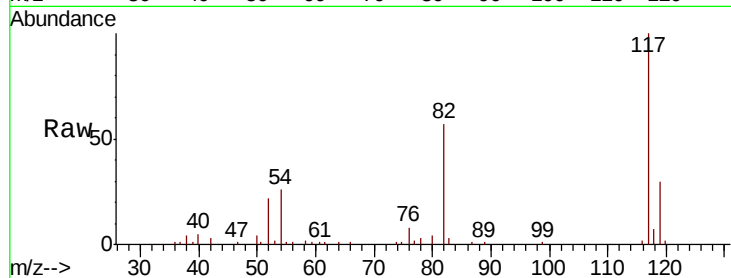


Abundance Ion 116.95 (116.65 to 117.65): V
Ion 82.05 (81.75 to 82.75): V
Ion 118.95 (118.65 to 119.65): V

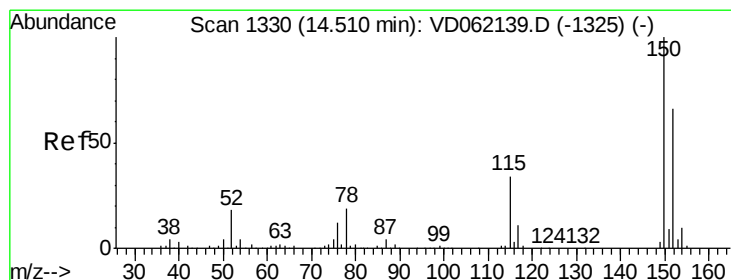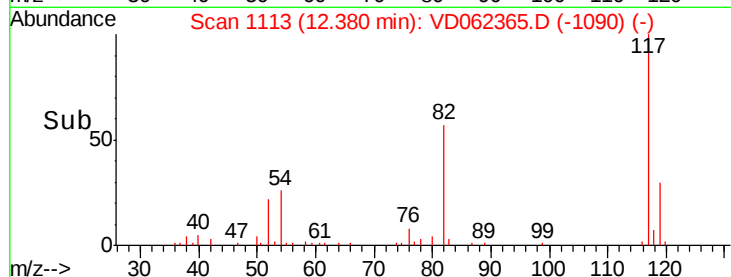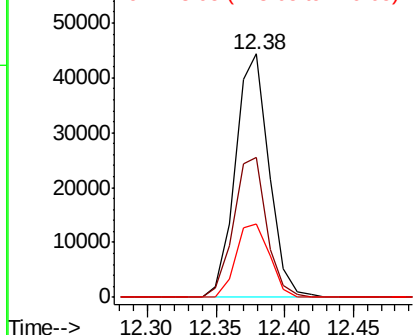

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 14.52 min Scan# 1331
Delta R.T. 0.01 min
Lab File: VD062365.D
Acq: 15 May 2019 1:14

Tgt Ion:152 Resp: 37373
Ion Ratio Lower Upper
152 100
115 53.5 30.9 92.7
150 156.0 0.0 314.8

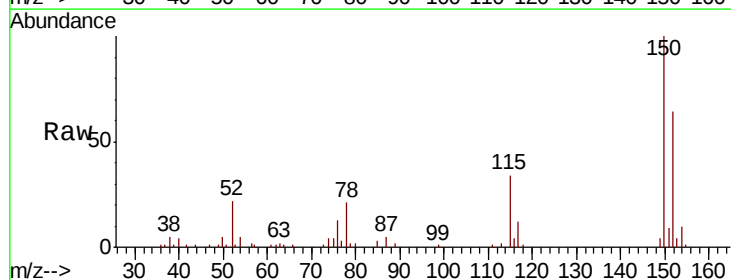

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 115.00 (114.70 to 115.70): V
Ion 149.90 (149.60 to 150.60): V

