

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_D\DATA\VD051419\
 Data File : VD062375.D
 Acq On : 15 May 2019 5:51
 Operator : FY/SY
 Sample : K2770-01
 Misc : 5.00g/5mL/MSVOA_D/SOIL
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 OILY-STONES

Quant Time: May 15 06:41:04 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D050719S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 07 14:26:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.06	168	593519	50.00	ug/l	0.04
34) 1,4-Difluorobenzene	8.24	114	842017	50.00	ug/l	0.05
63) Chlorobenzene-d5	12.37	117	556076	50.00	ug/l	0.02
72) 1,4-Dichlorobenzene-d4	14.52	152	239795	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.47	65	313189	56.78	ug/l	0.05
Spiked Amount	50.000		Recovery	=	113.56%	
35) Dibromofluoromethane	6.94	113	335223	47.98	ug/l	0.05
Spiked Amount	50.000		Recovery	=	95.96%	
50) Toluene-d8	10.43	98	553418	32.85	ug/l	0.03
Spiked Amount	50.000		Recovery	=	65.70%	
62) 4-Bromofluorobenzene	13.56	95	249037	36.82	ug/l	0.02
Spiked Amount	50.000		Recovery	=	73.64%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_D\DATA\VD051419\
Data File : VD062375.D
Acq On : 15 May 2019 5:51
Operator : FY/SY
Sample : K2770-01
Misc : 5.00g/5mL/MSVOA_D/SOIL
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
OILY-STONES

Quant Time: May 15 06:41:04 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D050719S.M
Quant Title : SW846 8260
QLast Update : Tue May 07 14:26:29 2019
Response via : Initial Calibration

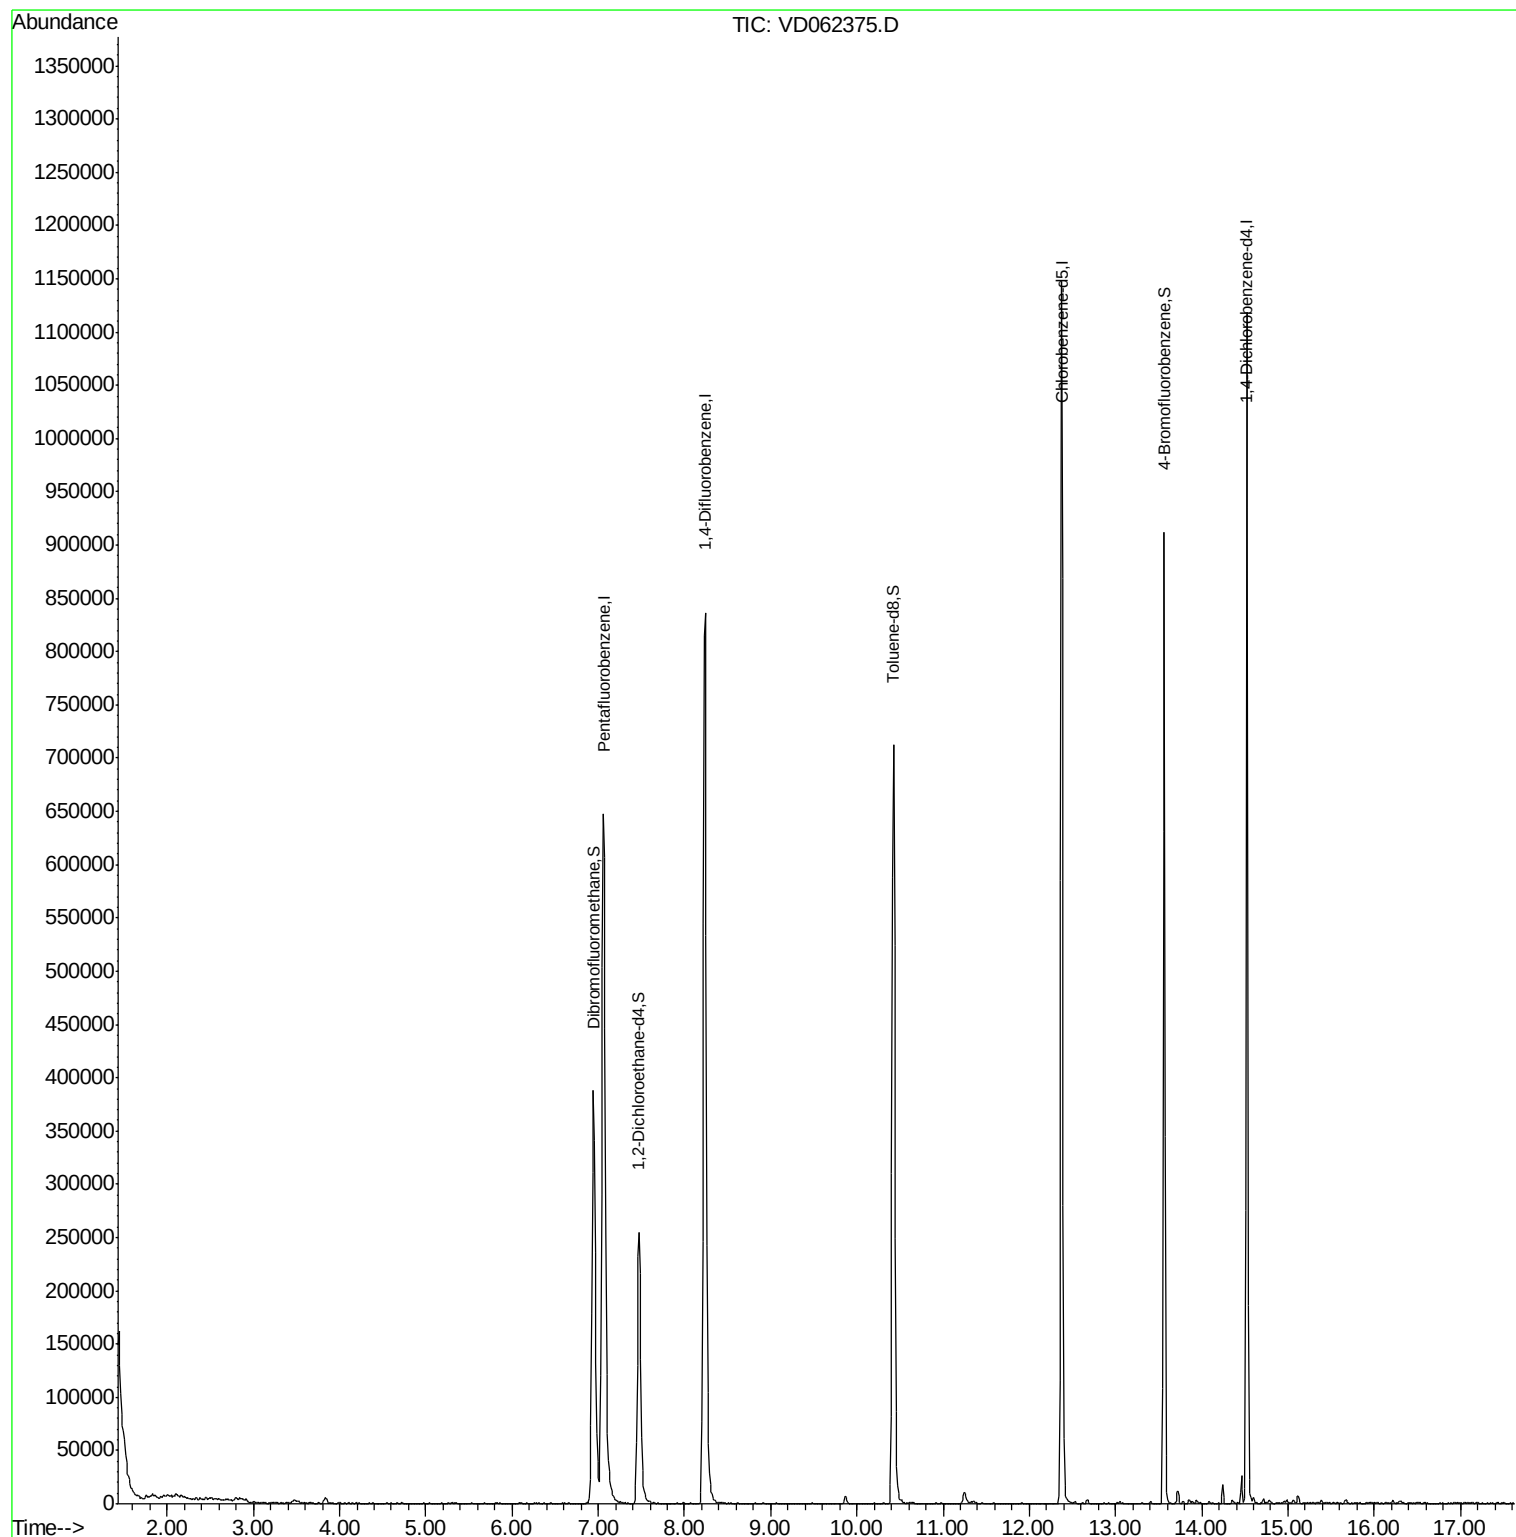

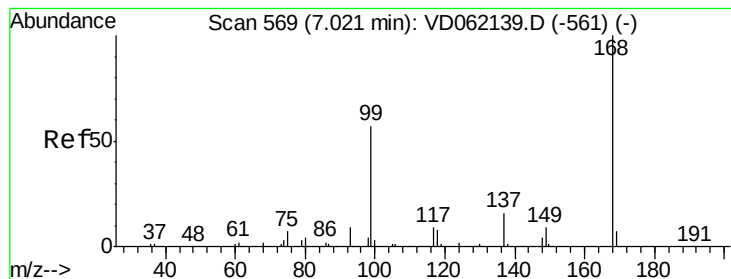

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.06 min Scan# 573

Delta R.T. 0.04 min

Lab File: VD062375.D

Acq: 15 May 2019 5:51

Instrument :

MSVOA_D

ClientSampleId :


OILY-STONES

Tgt Ion:168 Resp: 593519

Ion Ratio Lower Upper




168 100

99 72.0 46.5 69.7#

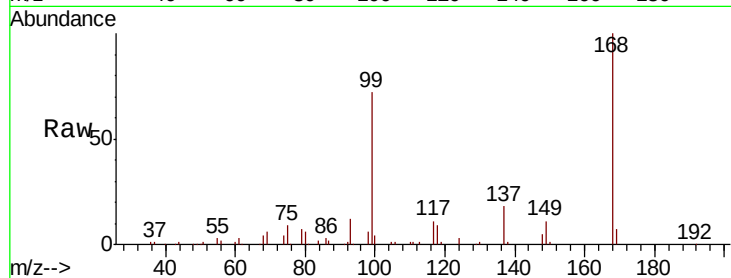

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

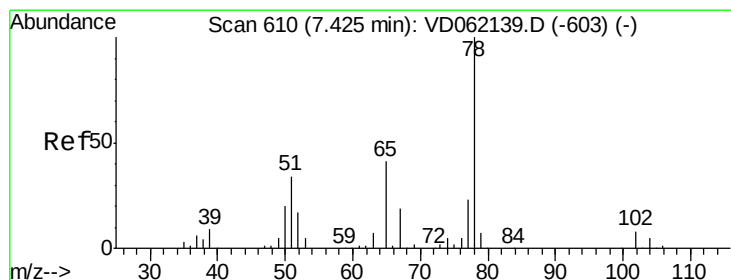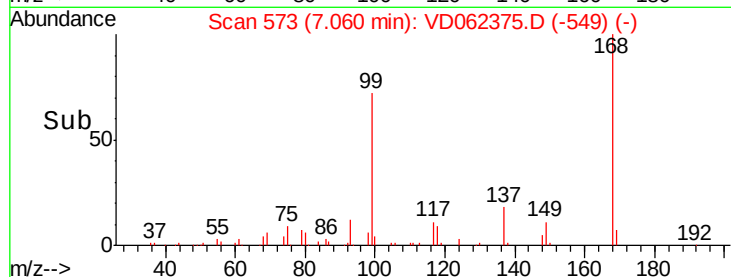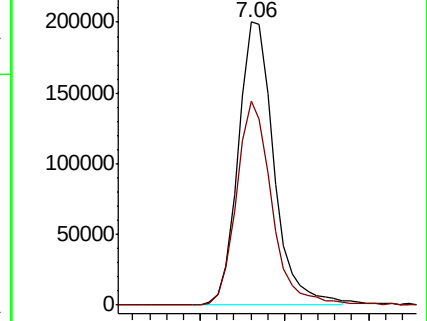

#33

1,2-Dichloroethane-d4

Concen: 56.782 ug/l

RT: 7.47 min Scan# 615

Delta R.T. 0.05 min

Lab File: VD062375.D


Acq: 15 May 2019 5:51

Tgt Ion: 65 Resp: 313189

Ion Ratio Lower Upper



65 100


67 41.4 0.0 98.0

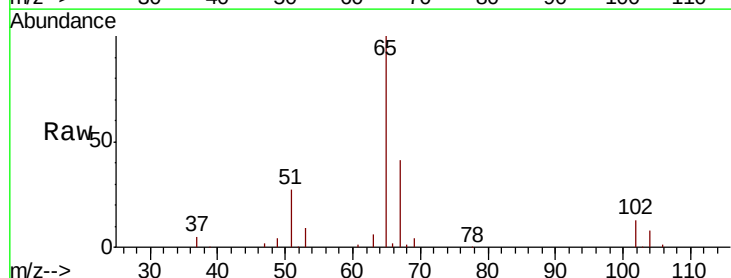

Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC

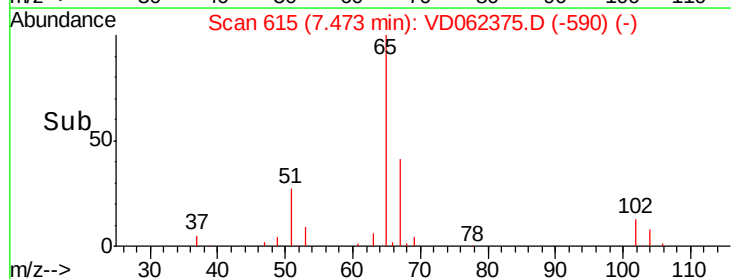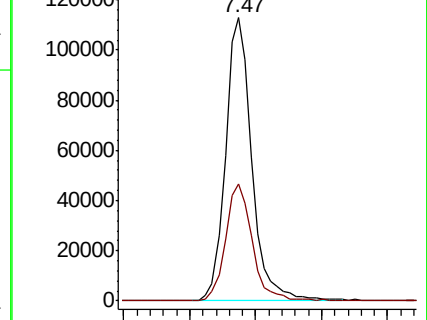


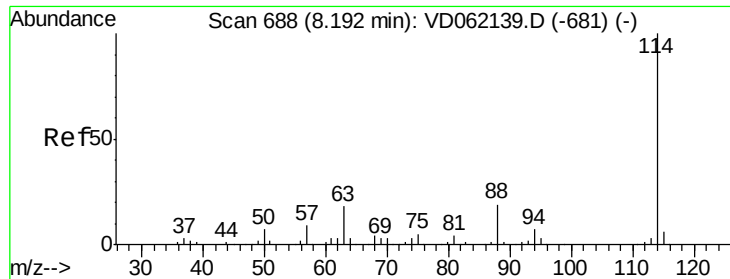




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.24 min Scan# 693
 Delta R.T. 0.05 min
 Lab File: VD062375.D
 Acq: 15 May 2019 5:51

Instrument :
 MSVOA_D
 ClientSampleId :
 OILY-STONES

Tgt Ion:114 Resp: 842017
 Ion Ratio Lower Upper
 114 100
 63 19.6 0.0 32.4
 88 20.5 0.0 33.6

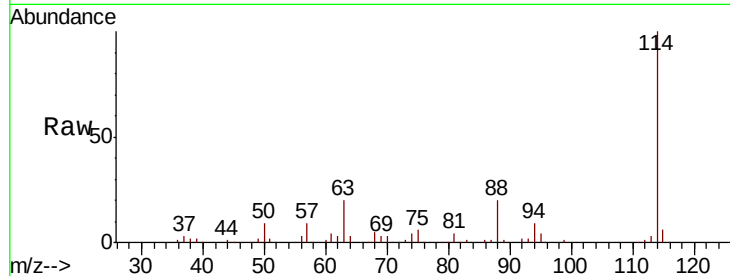


Abundance Ion 114.00 (113.70 to 114.70): V
 Ion 62.95 (62.65 to 63.65): V
 Ion 87.90 (87.60 to 88.60): V

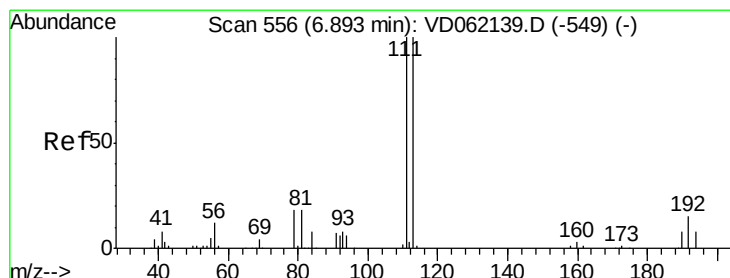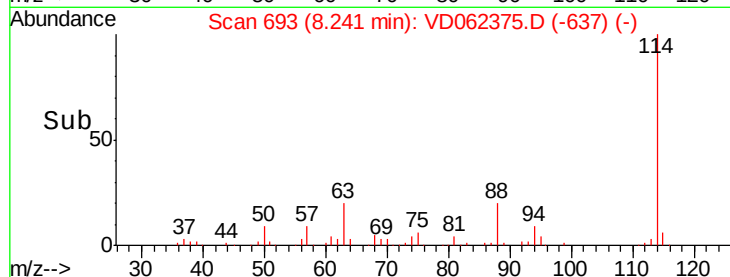
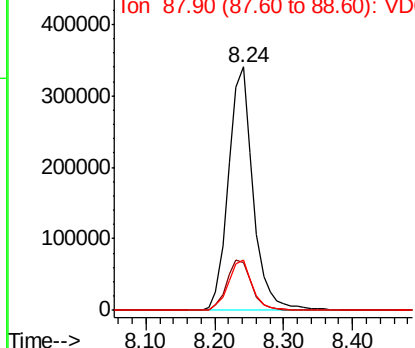



#35
 Dibromofluoromethane
 Concen: 47.983 ug/l
 RT: 6.94 min Scan# 561
 Delta R.T. 0.05 min
 Lab File: VD062375.D
 Acq: 15 May 2019 5:51

Tgt Ion:113 Resp: 335223
 Ion Ratio Lower Upper
 113 100
 111 110.3 78.5 117.7
 192 16.4 13.0 19.4

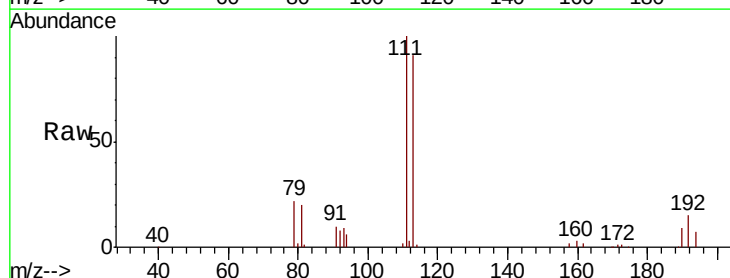

Abundance Ion 112.90 (112.60 to 113.60): V
 Ion 110.90 (110.60 to 111.60): V
 Ion 191.80 (191.50 to 192.50): V

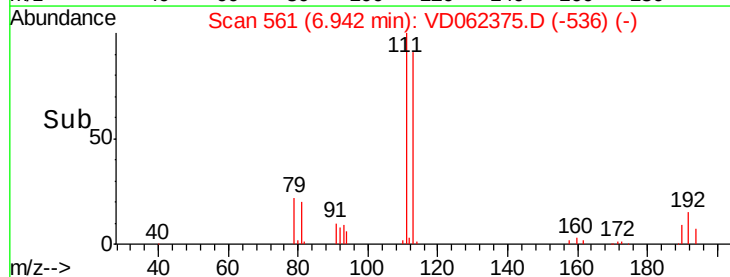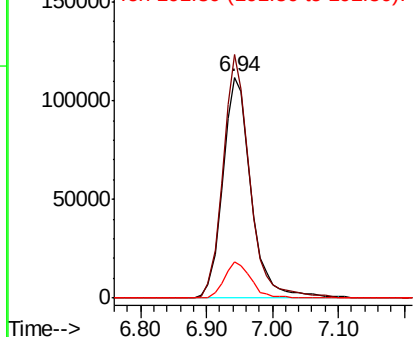


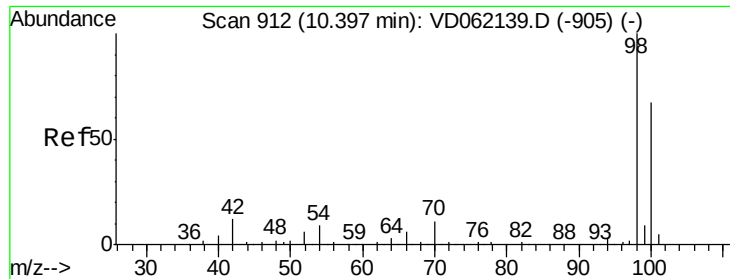




#50
Toluene-d8
Concen: 32.855 ug/l
RT: 10.43 min Scan# 915
Delta R.T. 0.03 min
Lab File: VD062375.D
Acq: 15 May 2019 5:51

Instrument :
MSVOA_D
ClientSampleId :
OILY-STONES

Tgt Ion: 98 Resp: 553418
Ion Ratio Lower Upper
98 100
100 68.4 53.8 80.8

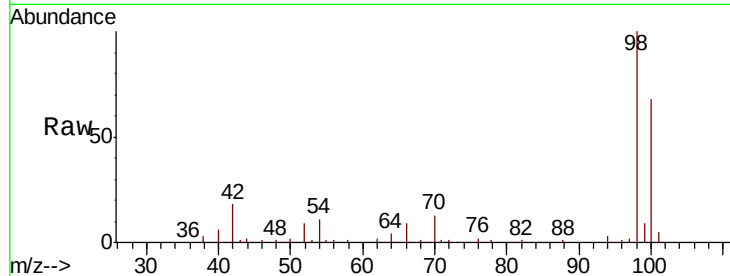


Abundance Ion 98.05 (97.75 to 98.75): VD062139.D (-905) (-)
Ion 100.05 (99.75 to 100.75): VD062139.D (-905) (-)

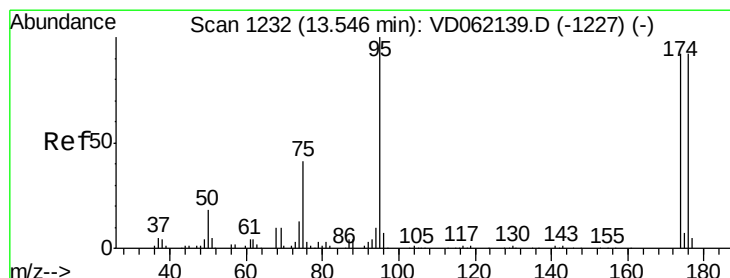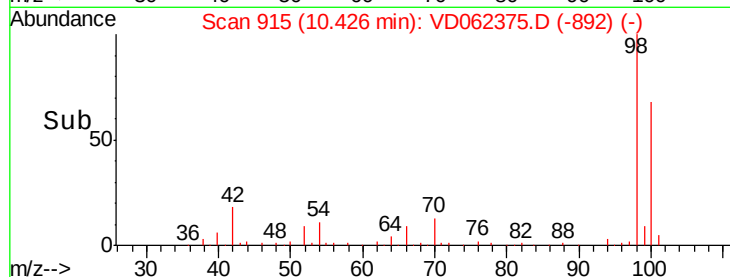
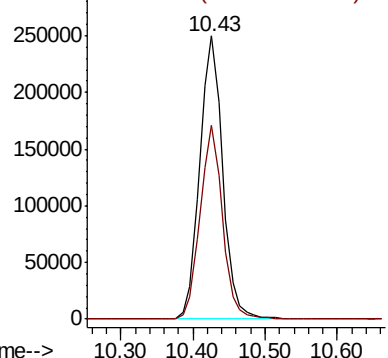



#62
4-Bromofluorobenzene
Concen: 36.817 ug/l
RT: 13.56 min Scan# 1234
Delta R.T. 0.02 min
Lab File: VD062375.D
Acq: 15 May 2019 5:51

Tgt Ion: 95 Resp: 249037
Ion Ratio Lower Upper
95 100
174 88.6 0.0 181.8
176 86.7 0.0 174.4

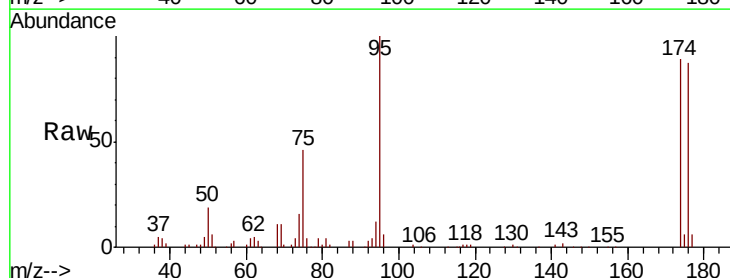

Abundance Ion 95.00 (94.70 to 95.70): VD062139.D (-1227) (-)
Ion 173.90 (173.60 to 174.60): VD062139.D (-1227) (-)
Ion 175.90 (175.60 to 176.60): VD062139.D (-1227) (-)

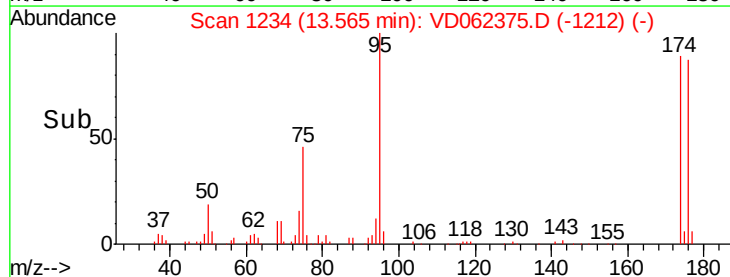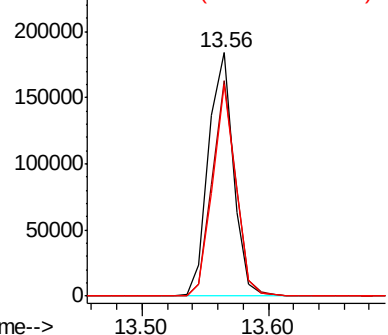


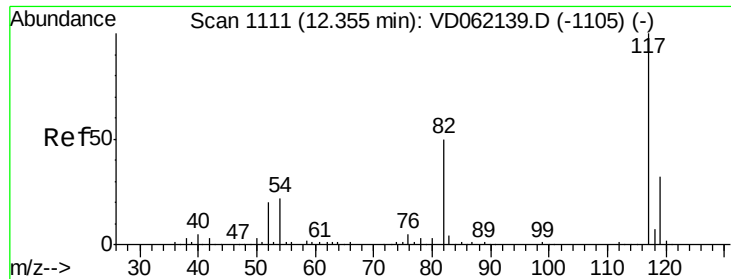




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 12.37 min Scan# 1113
Delta R.T. 0.02 min
Lab File: VD062375.D
Acq: 15 May 2019 5:51

Instrument :
MSVOA_D
ClientSampleId :
OILY-STONES

Tgt Ion:117 Resp: 556076
Ion Ratio Lower Upper
117 100
82 61.8 36.2 54.2#
119 31.9 26.2 39.4

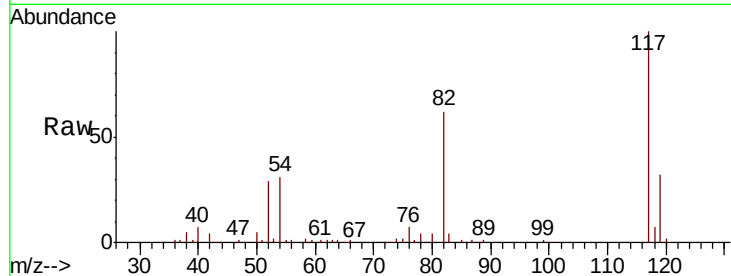


Abundance Ion 116.95 (116.65 to 117.65): V
Ion 82.05 (81.75 to 82.75): V
Ion 118.95 (118.65 to 119.65): V

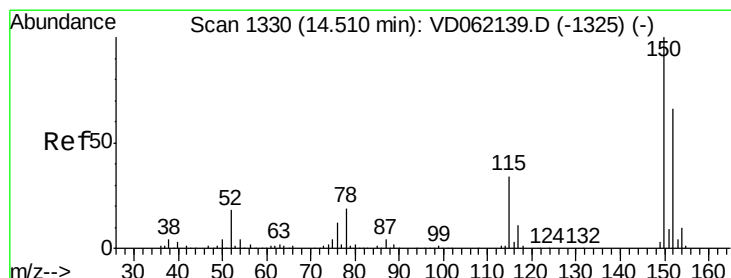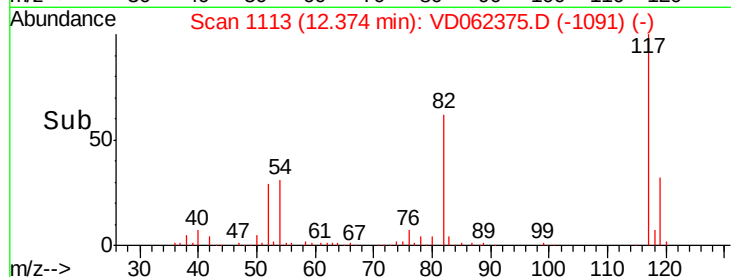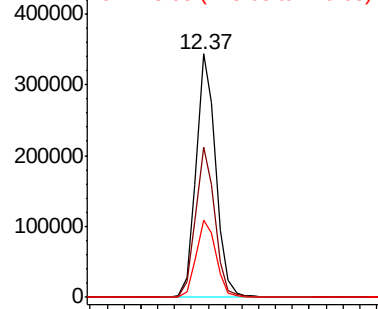

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 14.52 min Scan# 1331
Delta R.T. 0.01 min
Lab File: VD062375.D
Acq: 15 May 2019 5:51

Tgt Ion:152 Resp: 239795
Ion Ratio Lower Upper
152 100
115 66.1 30.9 92.7
150 157.2 0.0 314.8

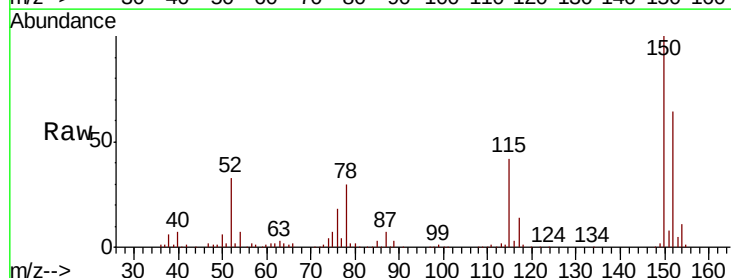

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 115.00 (114.70 to 115.70): V
Ion 149.90 (149.60 to 150.60): V

