


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD051419\
 Data File : VD062338.D
 Acq On : 14 May 2019 9:50
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D050719S.M
 Title : SW846 8260
 Last Update : Tue May 07 14:26:29 2019

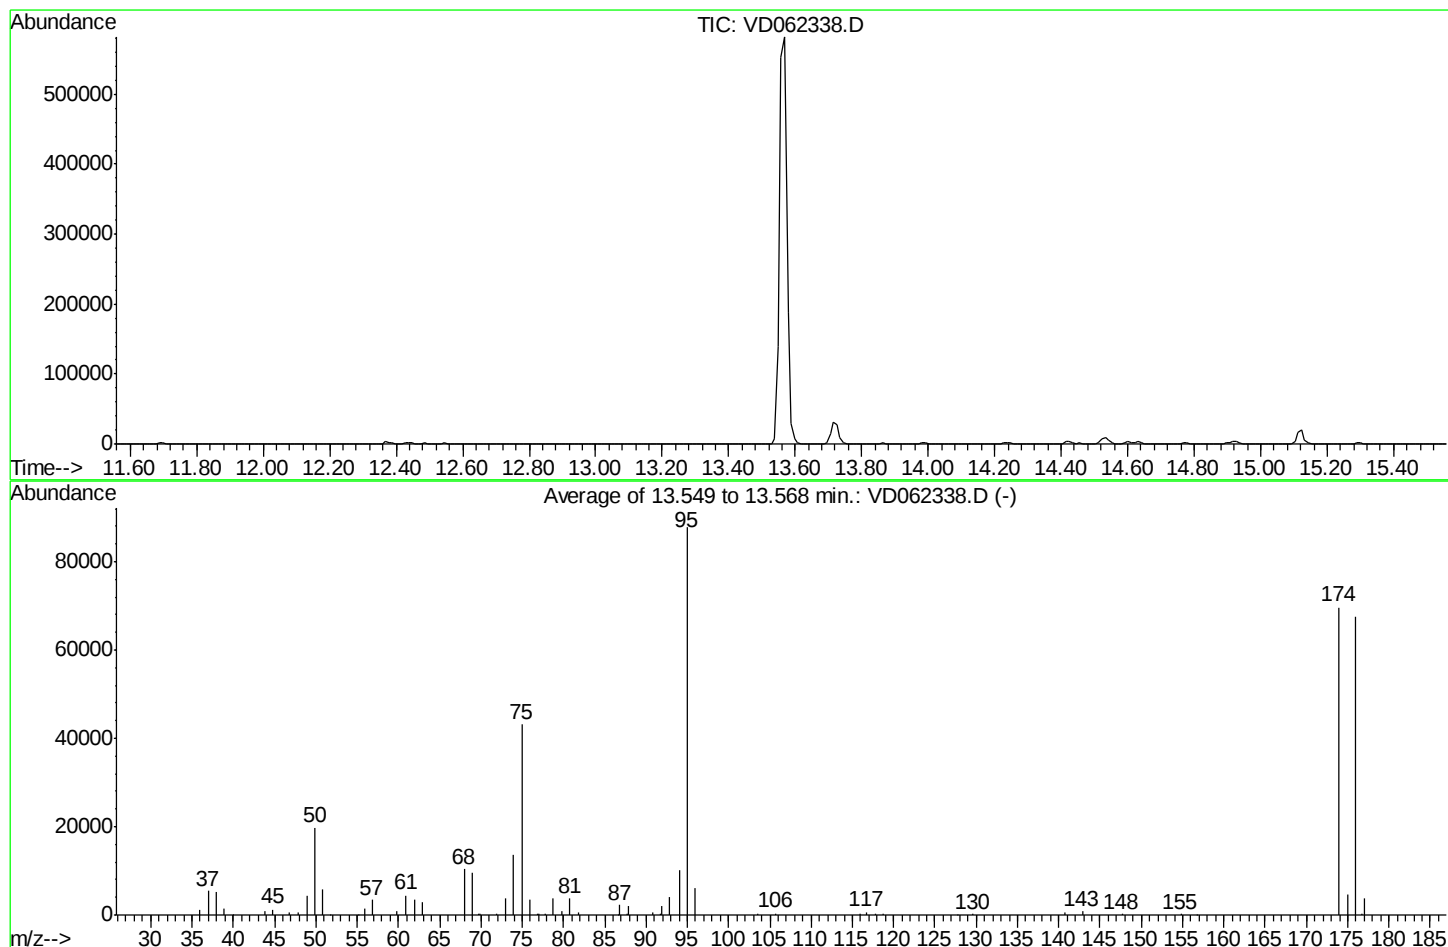

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	19829	PASS
75	95	30	60	49.1	43090	PASS
95	95	100	100	100.0	87749	PASS
96	95	5	9	7.0	6185	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	79.3	69555	PASS
175	174	5	9	6.8	4707	PASS
176	174	95	101	96.9	67406	PASS
177	176	5	9	5.4	3658	PASS