


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_D\DATA\VD051419\
Data File : VD062360.D
Acq On : 14 May 2019 22:00
Operator : FY/SY
Sample : BFB
Misc : 5.00g/5mL/MSVOA_D/SOIL
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D050719S.M
Title : SW846 8260
Last Update : Tue May 07 14:26:29 2019

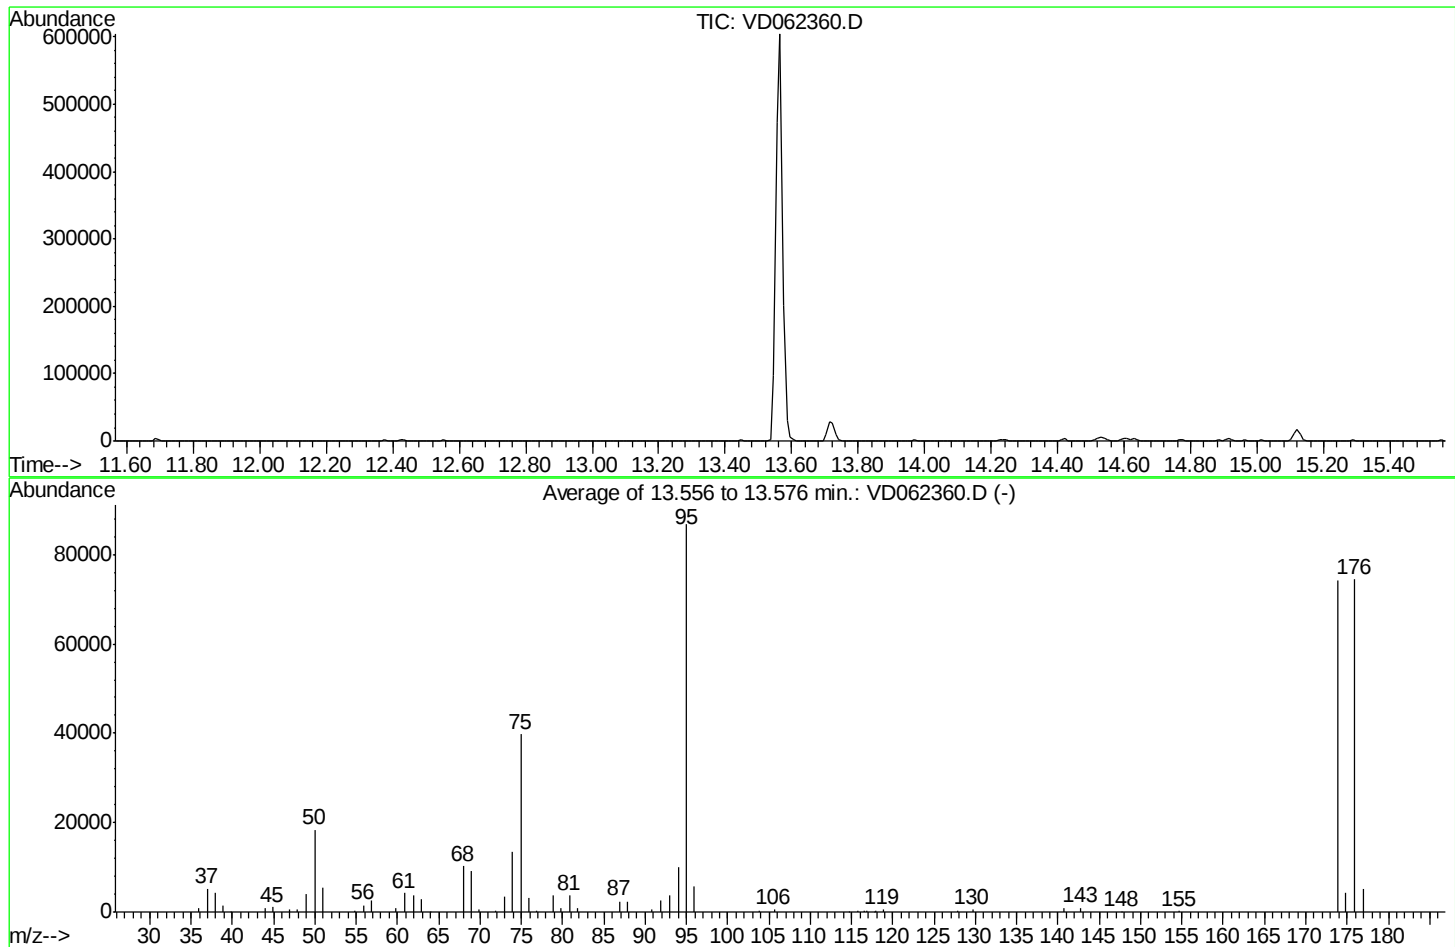

AutoFind: Scans 1233, 1234, 1235; Background Corrected with Scan 1228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	18416	PASS
75	95	30	60	45.8	39761	PASS
95	95	100	100	100.0	86768	PASS
96	95	5	9	6.7	5772	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.5	74224	PASS
175	174	5	9	5.9	4376	PASS
176	174	95	101	100.3	74418	PASS
177	176	5	9	6.8	5075	PASS