
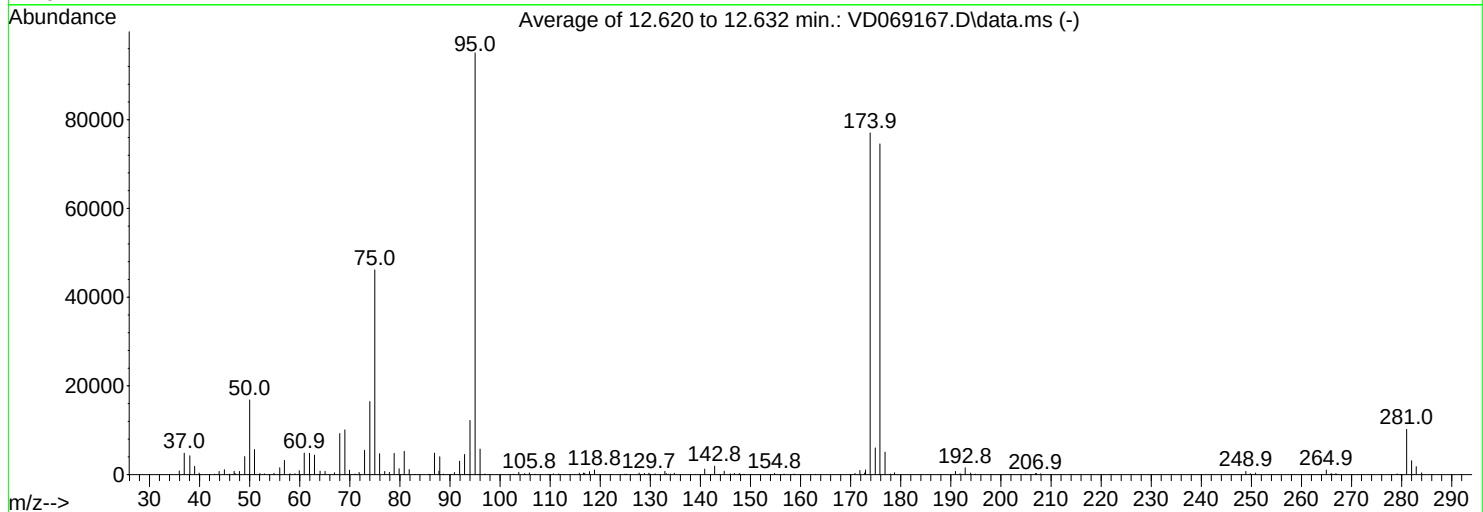


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051421\
Data File : VD069167.D
Acq On : 14 May 2021 09:38
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051221S.M
Title : SW846 8260
Last Update : Thu May 13 04:01:29 2021

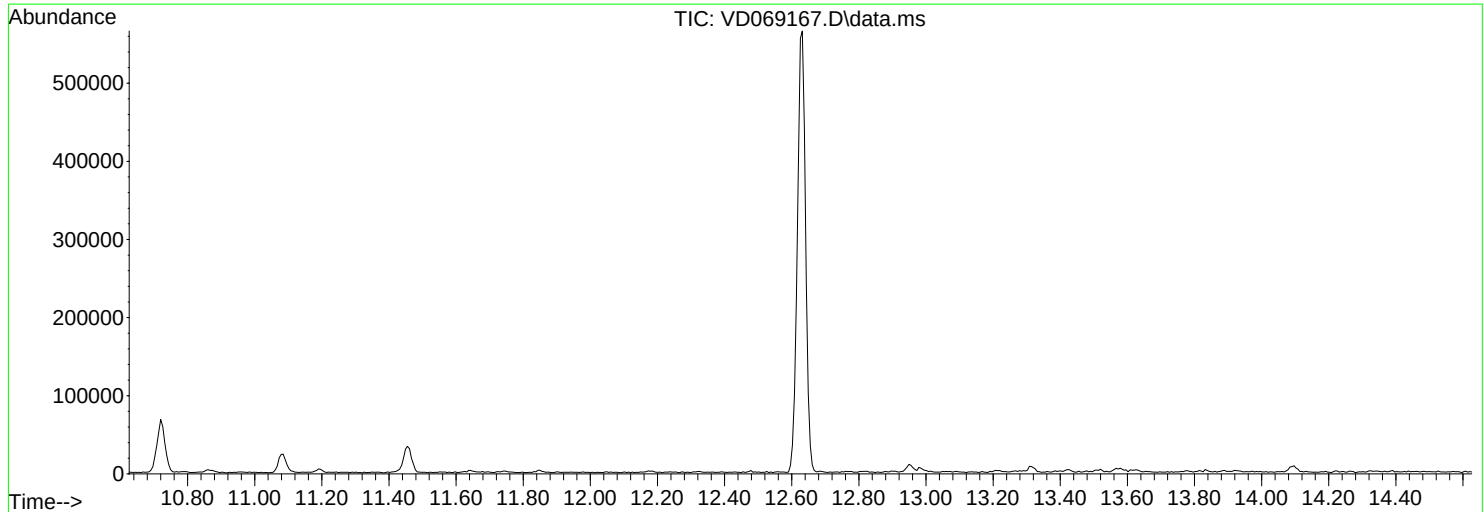

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1812

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.7	16847	PASS
75	95	30	60	48.6	46173	PASS
95	95	100	100	100.0	95072	PASS
96	95	5	9	6.1	5773	PASS
173	174	0.00	2	1.3	1032	PASS
174	95	50	100	81.0	77021	PASS
175	174	5	9	7.8	6033	PASS
176	174	95	101	96.8	74563	PASS
177	176	5	9	6.8	5076	PASS