


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD051520\
Data File : VD065745.D
Acq On : 15 May 2020 09:34
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D051320S.M
Title : SW846 8260
Last Update : Wed May 13 14:28:42 2020

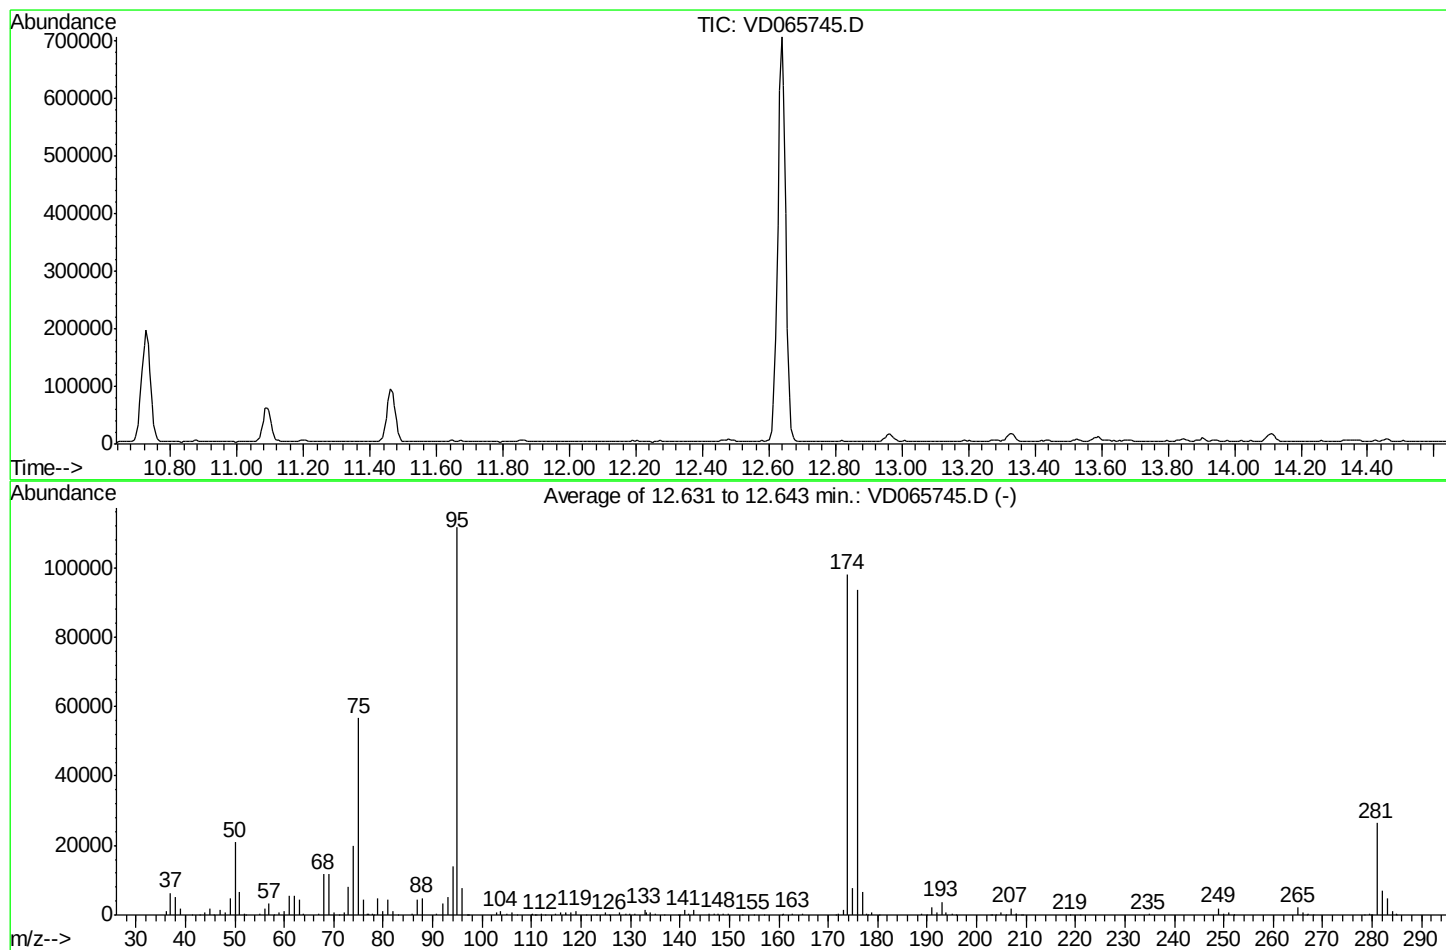

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	20832	PASS
75	95	30	60	50.8	56736	PASS
95	95	100	100	100.0	111605	PASS
96	95	5	9	7.1	7900	PASS
173	174	0.00	2	1.4	1392	PASS
174	95	50	100	87.7	97853	PASS
175	174	5	9	7.8	7639	PASS
176	174	95	101	95.6	93512	PASS
177	176	5	9	7.0	6557	PASS