

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051622\
 Data File : VD073035.D
 Acq On : 16 May 2022 15:12
 Operator : VA/SY
 Sample : N2816-16
 Misc : 5.58G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 P007-SS008-0006-01

Quant Time: May 17 03:28:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050222S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 03 08:33:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	359588	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	624941	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	608993	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	264166	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	192618	41.266	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	82.540%
35) Dibromofluoromethane	7.908	113	205492	46.819	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	93.640%
50) Toluene-d8	10.332	98	761953	48.397	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	96.800%
62) 4-Bromofluorobenzene	12.620	95	267452	45.559	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	91.120%


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051622\
Data File : VD073035.D
Acq On : 16 May 2022 15:12
Operator : VA/SY
Sample : N2816-16
Misc : 5.58G/5.00ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
P007-SS008-0006-01

Quant Time: May 17 03:28:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050222S.M
Quant Title : SW846 8260
QLast Update : Tue May 03 08:33:49 2022
Response via : Initial Calibration




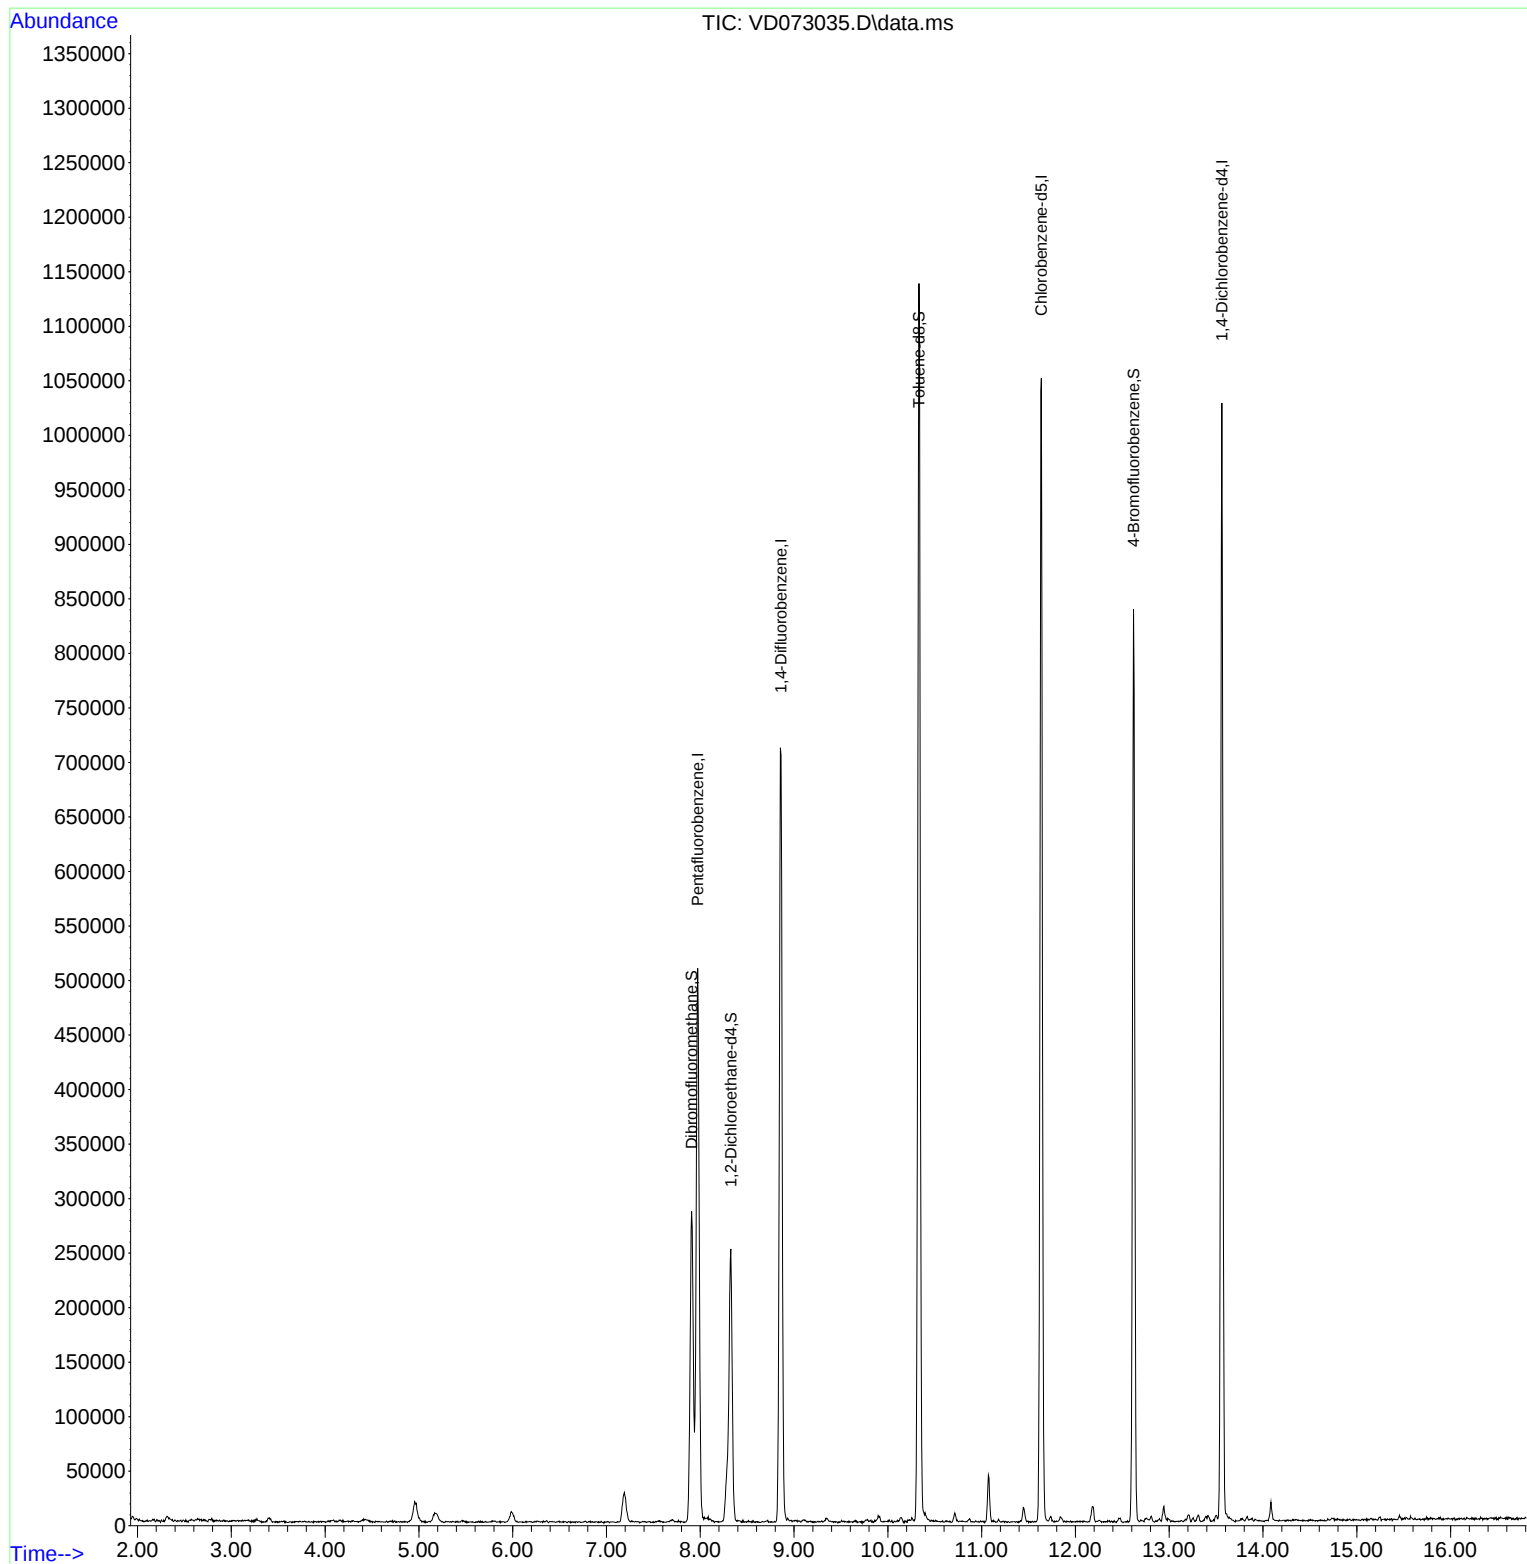


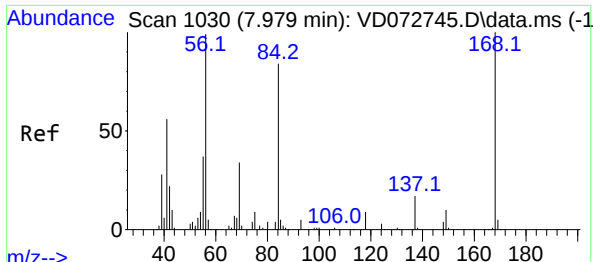

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. -0.006 min
Lab File: VD073035.D
Acq: 16 May 2022 15:12




Instrument :
MSVOA_D
ClientSampleId :
P007-SS008-0006-01

Tgt Ion:168 Resp: 359588
Ion Ratio Lower Upper
168 100
99 62.1 49.8 74.6

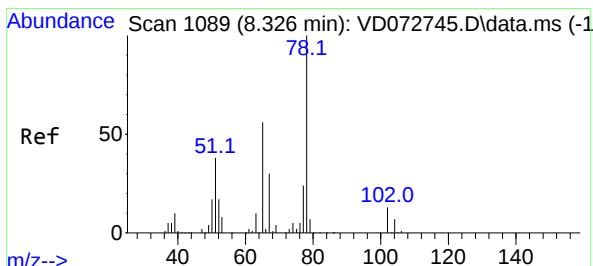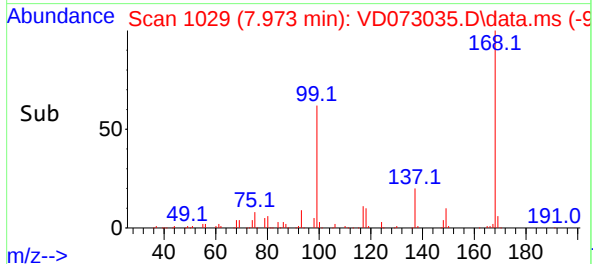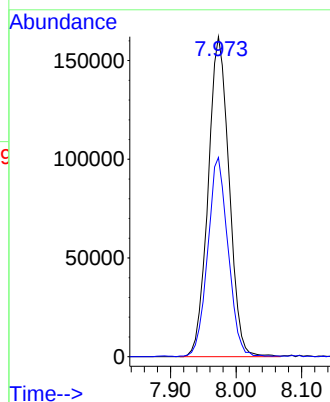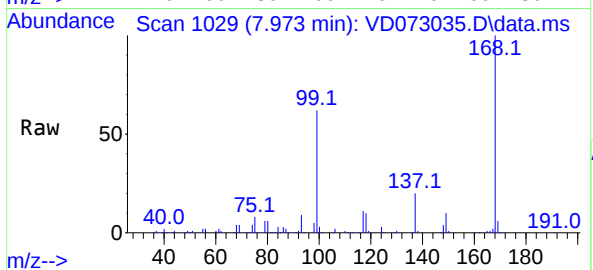

#33
1,2-Dichloroethane-d4
Concen: 41.266 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. -0.000 min
Lab File: VD073035.D
Acq: 16 May 2022 15:12

Tgt Ion: 65 Resp: 192618
Ion Ratio Lower Upper
65 100
67 52.9 0.0 101.4

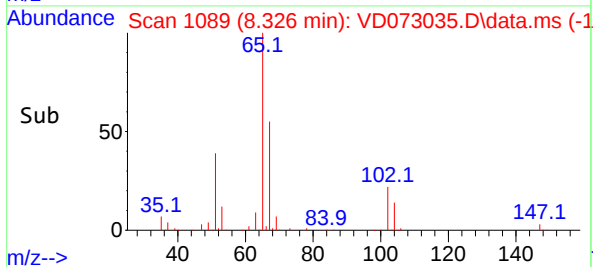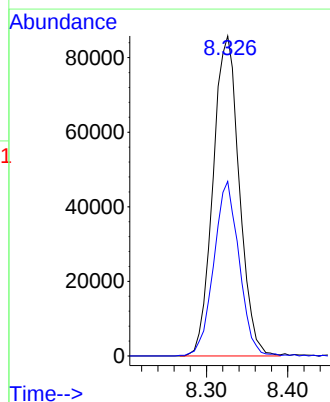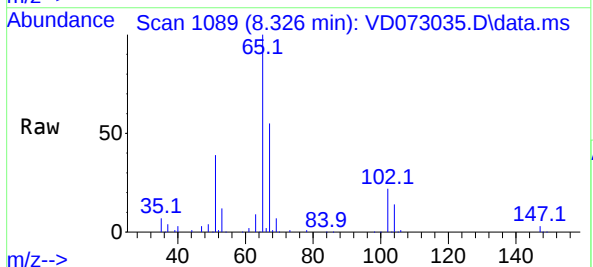



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.861 min Scan# 1180

Delta R.T. 0.000 min

Lab File: VD073035.D

Acq: 16 May 2022 15:12

Instrument :

MSVOA_D

ClientSampleId :

P007-SS008-0006-01





Tgt Ion:114 Resp: 624941

Ion Ratio Lower Upper

114 100

63 19.6 0.0 46.6

88 15.3 0.0 33.2

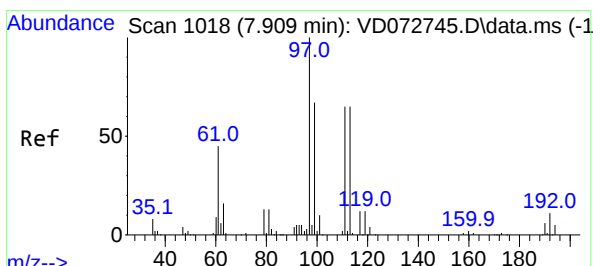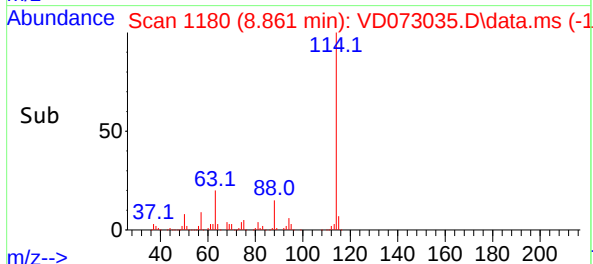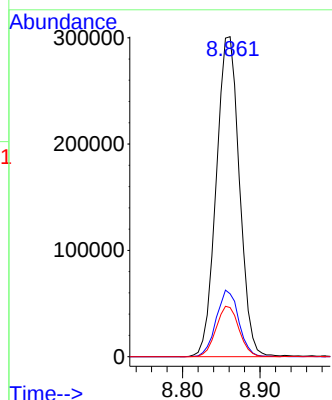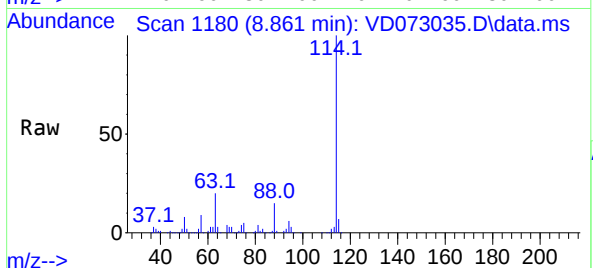

#35

Dibromofluoromethane

Concen: 46.819 ug/l

RT: 7.908 min Scan# 1018

Delta R.T. -0.001 min

Lab File: VD073035.D

Acq: 16 May 2022 15:12




Tgt Ion:113 Resp: 205492


Ion Ratio Lower Upper

113 100

111 102.9 83.8 125.6

192 17.7 14.6 21.8

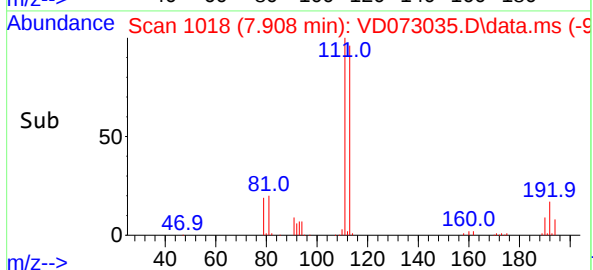
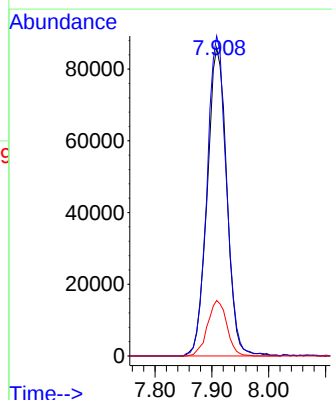
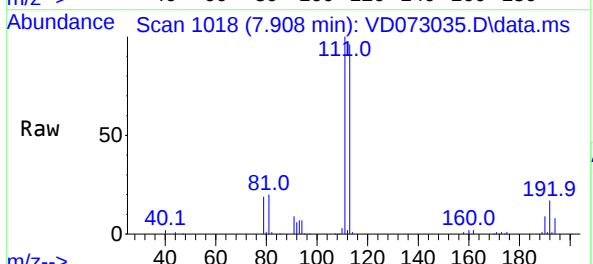


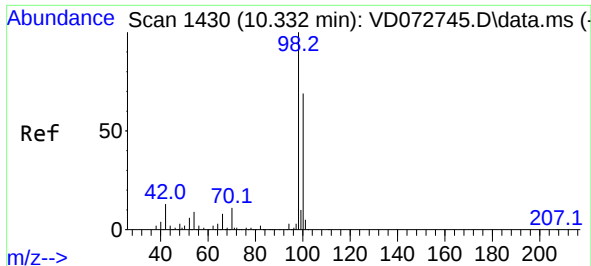

#50
Toluene-d8
Concen: 48.397 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD073035.D
Acq: 16 May 2022 15:12




Instrument :
MSVOA_D
ClientSampleId :
P007-SS008-0006-01


Tgt Ion: 98 Resp: 761953
Ion Ratio Lower Upper
98 100
100 66.8 52.4 78.6

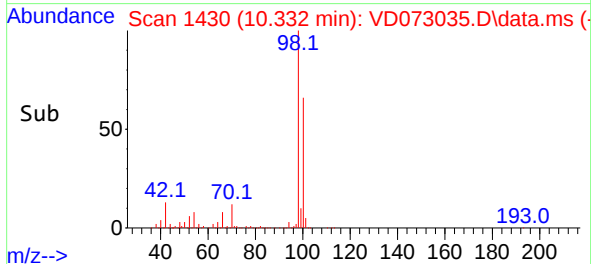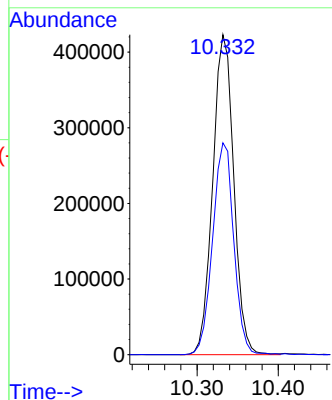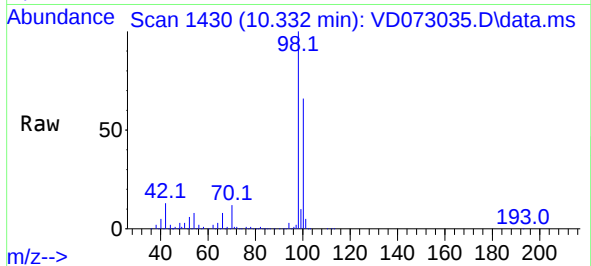

#62
4-Bromofluorobenzene
Concen: 45.559 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VD073035.D
Acq: 16 May 2022 15:12

Tgt Ion: 95 Resp: 267452
Ion Ratio Lower Upper
95 100
174 77.8 0.0 152.8
176 73.4 0.0 145.4


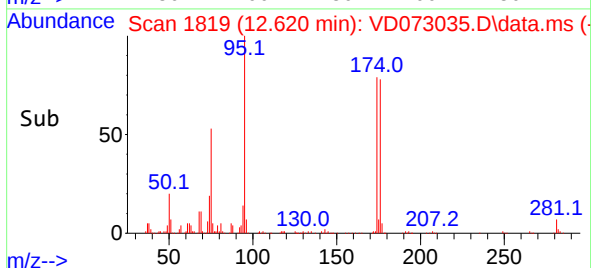
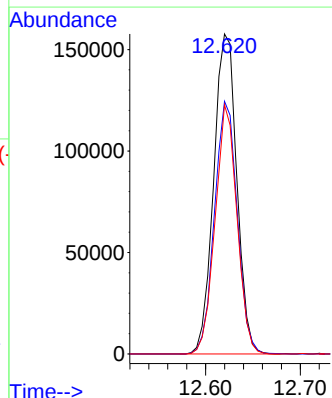
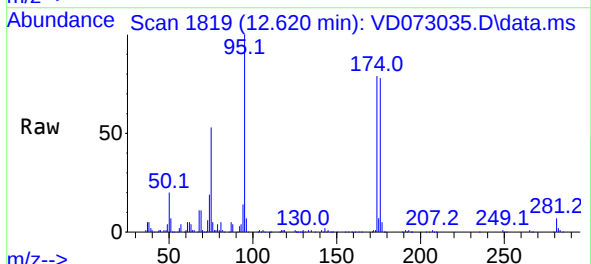


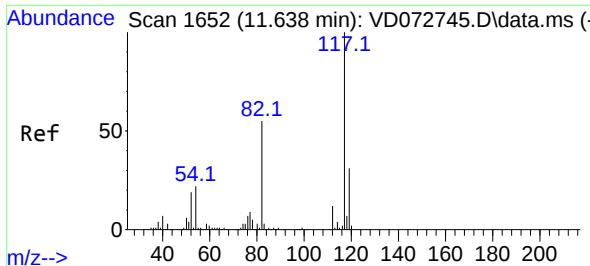

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 117
Delta R.T. -0.000 min
Lab File: VD073035.D
Acq: 16 May 2022 15:12

Instrument :
MSVOA_D
ClientSampleId :
P007-SS008-0006-01

Tgt Ion:117 Resp: 608993
Ion Ratio Lower Upper
117 100
82 55.6 45.3 67.9
119 33.2 26.6 40.0

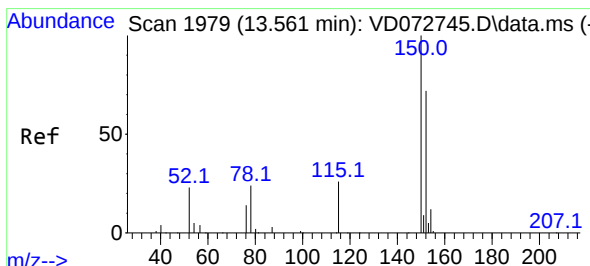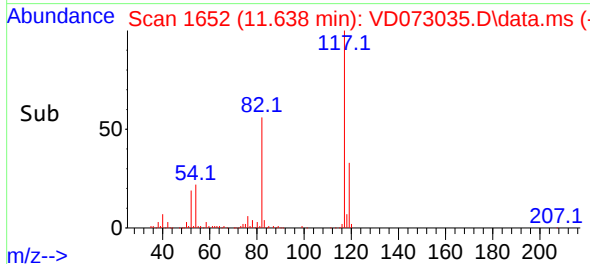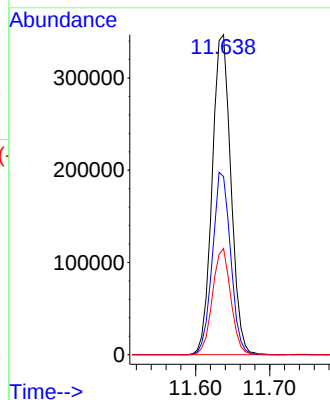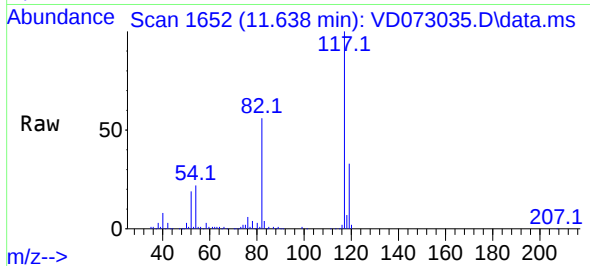

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. -0.000 min
Lab File: VD073035.D
Acq: 16 May 2022 15:12

Tgt Ion:152 Resp: 264166
Ion Ratio Lower Upper
152 100
115 60.7 31.3 93.8
150 159.4 0.0 348.6

