
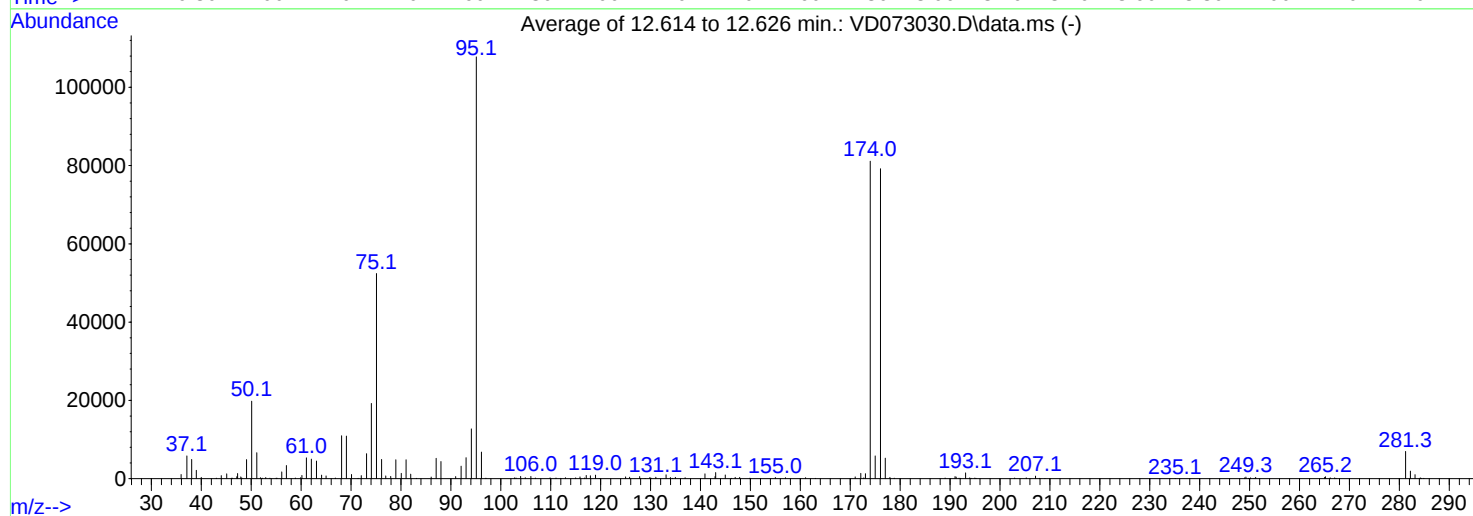


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051622\
 Data File : VD073030.D
 Acq On : 16 May 2022 10:42
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00 G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050222S.M
 Title : SW846 8260
 Last Update : Tue May 03 08:33:49 2022

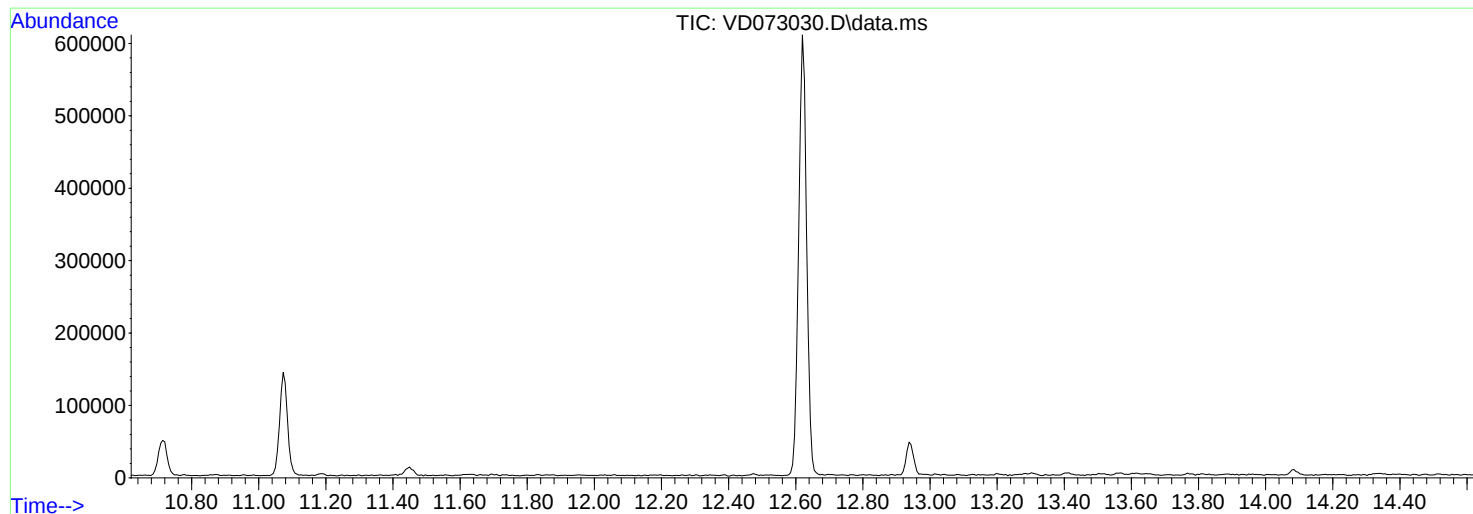

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	19773	PASS
75	95	30	60	48.6	52416	PASS
95	95	100	100	100.0	107787	PASS
96	95	5	9	6.3	6804	PASS
173	174	0.00	2	1.6	1288	PASS
174	95	50	100	75.3	81123	PASS
175	174	5	9	7.1	5796	PASS
176	174	95	101	97.6	79213	PASS
177	176	5	9	6.6	5249	PASS