
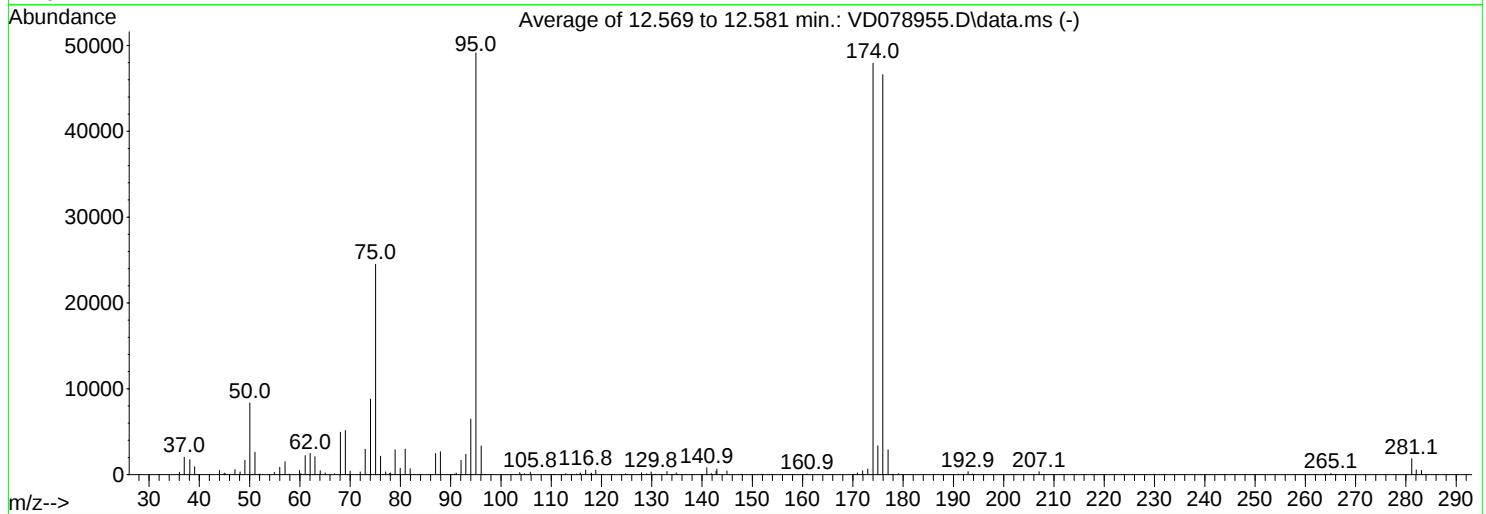


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051724\
Data File : VD078955.D
Acq On : 17 May 2024 09:07
Operator : RP/MD
Sample : BFB212
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB212

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Title : SFAM01.0
Last Update : Sat May 18 00:53:45 2024

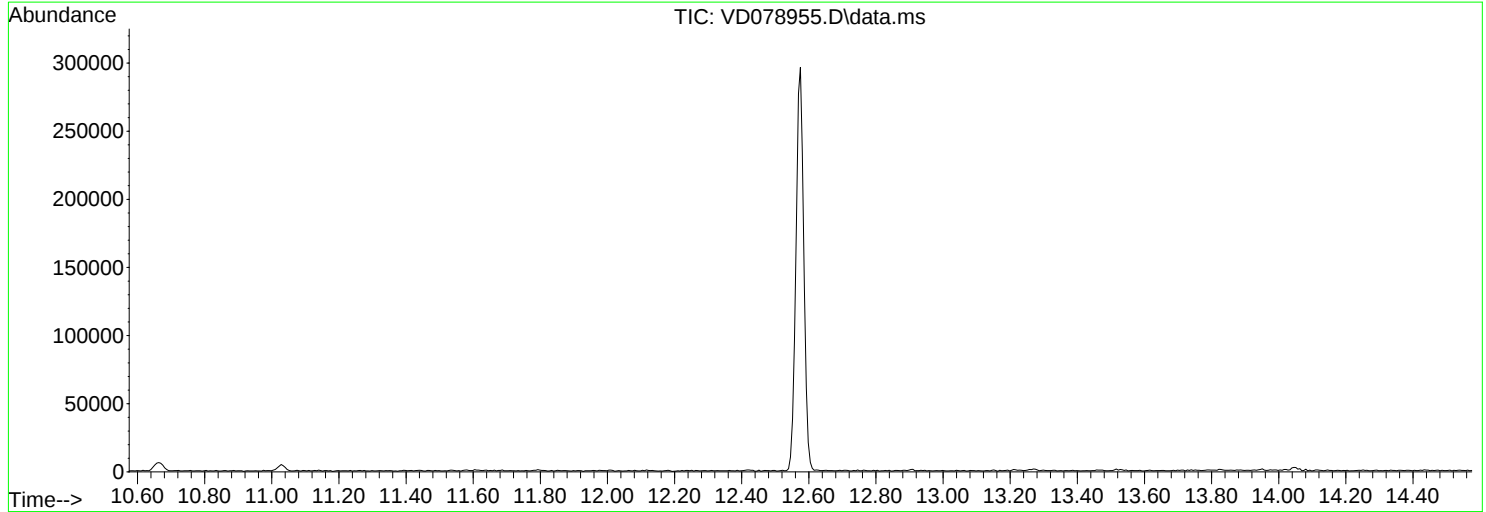

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	8354	PASS
75	95	30	80	49.9	24520	PASS
95	95	100	100	100.0	49144	PASS
96	95	5	9	6.8	3341	PASS
173	174	0.00	2	1.3	646	PASS
174	95	50	120	97.5	47933	PASS
175	174	5	9	7.0	3352	PASS
176	174	95	105	97.2	46613	PASS
177	176	5	10	6.2	2887	PASS

m/z	Abundance
39.90	672.0
44.00	199.0

Instrument :
MSVOA_D
ClientSampleId :
BFB212

m/z	Abundance
36.10	309.0
37.00	1789.0
38.10	2107.0
39.00	842.0
40.10	986.0
44.00	693.0
45.00	354.0
47.10	664.0
48.00	321.0
49.10	1638.0
50.00	8425.0
51.00	2650.0
51.90	216.0
54.90	310.0
56.00	974.0
57.10	1642.0
57.90	202.0
60.00	589.0
61.10	2110.0
62.10	2447.0
63.00	2252.0
64.10	427.0
68.10	4708.0
69.10	5724.0
70.00	617.0
72.10	314.0
73.00	2874.0
74.00	9895.0
75.00	25824.0
76.00	2191.0
77.10	349.0
77.90	223.0
79.00	2597.0
79.90	742.0
80.90	3443.0
81.90	721.0
87.00	2633.0
87.90	2761.0
90.80	255.0
92.00	1725.0
93.00	2395.0
94.00	7462.0
95.00	51160.0
96.00	4309.0
103.80	232.0
104.70	173.0
105.90	236.0
110.70	195.0
112.90	196.0
116.80	415.0
117.80	224.0
118.00	227.0
118.80	646.0
128.00	284.0
129.00	336.0
129.90	199.0
133.00	441.0
134.90	318.0
136.80	178.0
140.90	825.0
142.80	1231.0
145.00	593.0
170.90	344.0
172.10	398.0
172.90	554.0
174.00	49192.0
174.90	3704.0
176.00	45344.0
177.00	2895.0
177.80	164.0
179.20	171.0
192.90	240.0
207.00	433.0
281.20	1356.0
282.10	450.0
283.10	324.0

Instrument :
MSVOA_D
ClientSampleId :
BFB212

m/z	Abundance
36.10	278.0
37.00	2735.0
38.10	1883.0
39.10	920.0
39.90	412.0
44.10	725.0
45.20	361.0
47.10	667.0
48.10	396.0
49.10	1591.0
50.00	9561.0
51.10	2896.0
52.10	163.0
54.90	353.0
56.00	964.0
57.00	1785.0
59.80	406.0
60.20	410.0
61.00	2529.0
62.00	2949.0
63.00	2299.0
64.10	410.0
65.00	375.0
68.00	5789.0
69.10	5654.0
70.00	348.0
71.90	323.0
73.00	3138.0
74.00	9690.0
75.10	26616.0
76.00	2491.0
77.00	228.0
77.70	156.0
78.10	205.0
78.90	3587.0
79.90	734.0
81.00	3126.0
82.00	637.0
87.00	2548.0
88.00	3210.0
91.10	309.0
92.00	1593.0
93.00	2514.0
94.00	7234.0
95.00	54296.0
96.10	3287.0
103.80	299.0
104.70	170.0
105.90	381.0
112.90	192.0
115.00	212.0
115.80	380.0
116.90	732.0
118.00	275.0
118.90	298.0
127.90	210.0
129.80	376.0
133.00	460.0
135.10	186.0
140.90	784.0
141.90	164.0
143.00	1059.0
144.90	381.0
147.80	165.0
160.90	212.0
170.90	301.0
171.90	489.0
173.00	848.0
174.00	53544.0
175.00	3155.0
175.90	50984.0
177.00	3163.0
192.80	547.0
193.80	237.0
207.10	225.0
265.10	188.0
281.10	2183.0
282.00	615.0
283.10	627.0

Instrument :
MSVOA_D
ClientSampleId :
BFB212

m/z	Abundance
35.90	234.0
37.00	1558.0
38.10	1281.0
39.10	974.0
39.90	539.0
43.90	626.0
44.90	234.0
47.10	441.0
48.20	232.0
49.00	1808.0
50.10	7076.0
51.00	2292.0
55.00	155.0
56.10	612.0
57.10	1084.0
59.90	443.0
61.10	2040.0
62.10	2026.0
63.00	1738.0
64.00	543.0
65.10	238.0
66.90	331.0
68.00	4313.0
69.00	4052.0
70.10	290.0
72.00	336.0
73.00	2872.0
74.10	6801.0
75.00	21120.0
76.10	1739.0
77.00	391.0
78.00	393.0
79.00	2463.0
80.00	697.0
80.90	2382.0
81.90	728.0
87.00	2187.0
88.00	2018.0
91.10	266.0
92.10	1664.0
93.00	2183.0
94.10	4692.0
95.00	41976.0
96.00	2427.0
96.80	169.0
103.70	194.0
105.80	229.0
115.70	263.0
116.80	453.0
118.90	645.0
124.80	343.0
128.00	193.0
129.90	362.0
130.80	153.0
133.10	219.0
134.80	287.0
141.00	772.0
141.80	188.0
142.90	927.0
144.90	320.0
170.10	161.0
171.80	435.0
173.00	537.0
174.00	41064.0
174.90	3197.0
176.00	43512.0
177.00	2602.0
179.00	160.0
191.00	177.0
193.00	281.0
207.10	325.0
265.10	277.0
266.10	166.0
281.10	2073.0
282.10	625.0
283.10	509.0

Instrument :
MSVOA_D
ClientSampleId :
BFB212