

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051822\
 Data File : VD073105.D
 Acq On : 18 May 2022 18:10
 Operator : VA/SY
 Sample : N2832-06
 Misc : 5.04G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB07

Quant Time: May 19 04:46:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051722S.M
 Quant Title : SW846 8260
 QLast Update : Wed May 18 04:58:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	304159	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	546442	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.632	117	562270	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	258777	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	173445	45.599	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	91.200%
35) Dibromofluoromethane	7.908	113	184440	48.073	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	96.140%
50) Toluene-d8	10.332	98	673411	48.382	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	96.760%
62) 4-Bromofluorobenzene	12.620	95	236942	47.001	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	94.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051822\
Data File : VD073105.D
Acq On : 18 May 2022 18:10
Operator : VA/SY
Sample : N2832-06
Misc : 5.04G/5.00ml/MSVOA_D/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB07


Quant Time: May 19 04:46:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051722S.M
Quant Title : SW846 8260
QLast Update : Wed May 18 04:58:34 2022
Response via : Initial Calibration

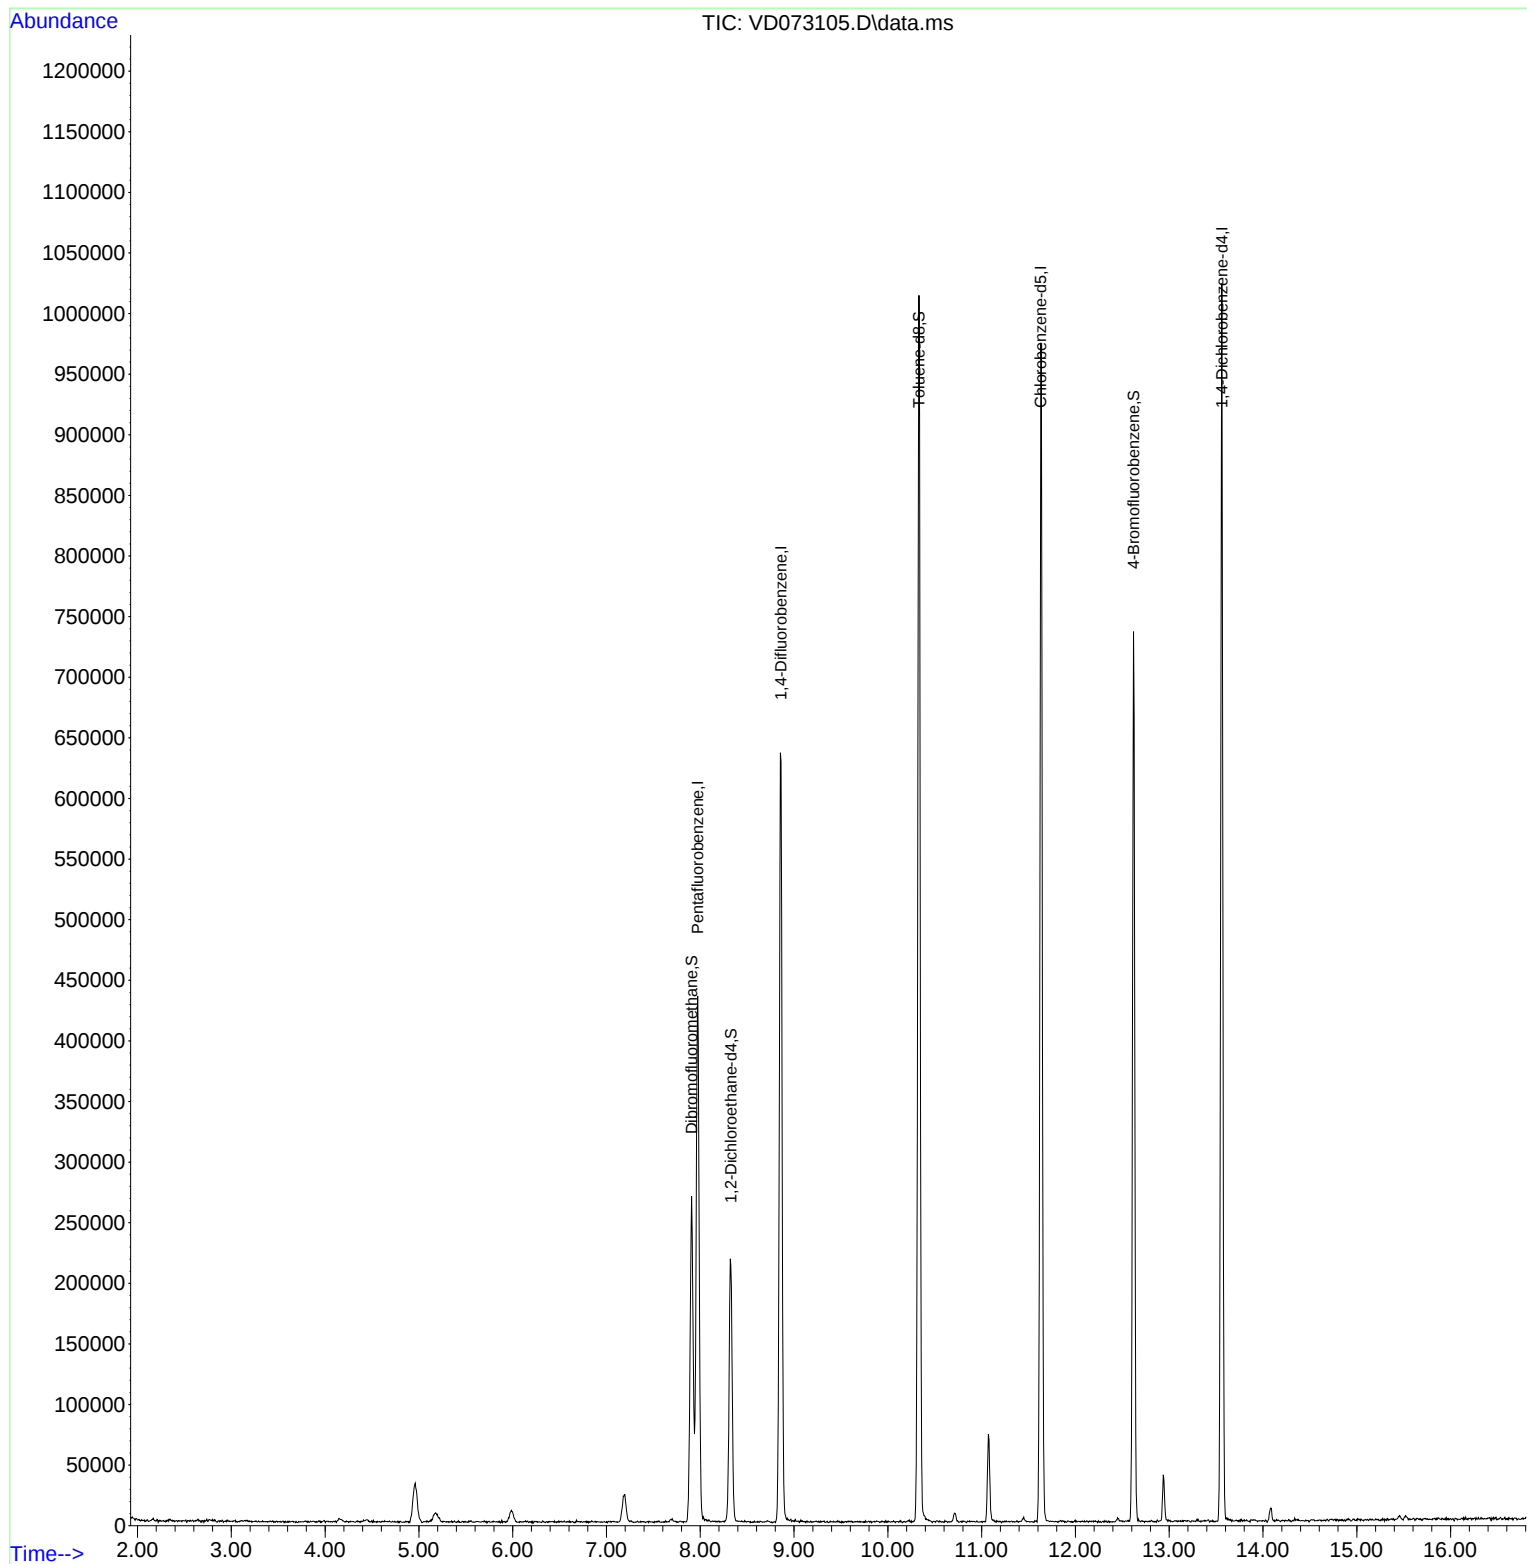



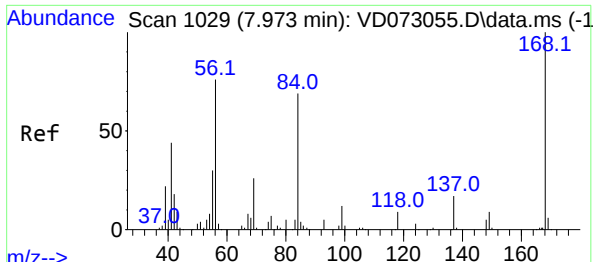


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. 0.000 min
Lab File: VD073105.D
Acq: 18 May 2022 18:10

Instrument :
MSVOA_D
ClientSampleId :
SB07



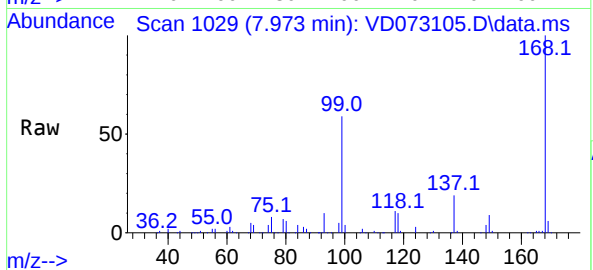



Tgt Ion:168 Resp: 304159
Ion Ratio Lower Upper
168 100
99 59.3 49.8 74.6

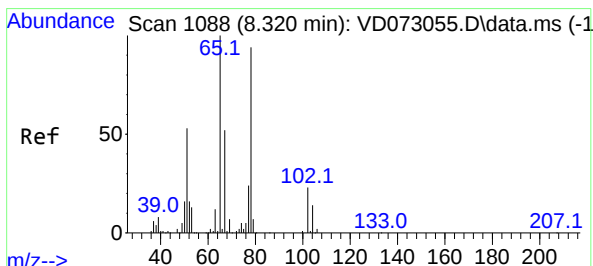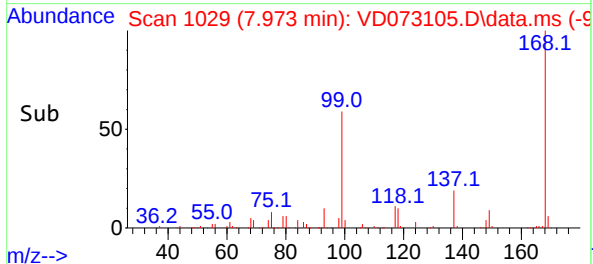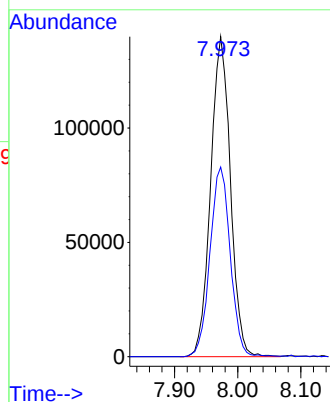

#33
1,2-Dichloroethane-d4
Concen: 45.599 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. 0.006 min
Lab File: VD073105.D
Acq: 18 May 2022 18:10

Tgt Ion: 65 Resp: 173445
Ion Ratio Lower Upper
65 100
67 52.5 0.0 101.4

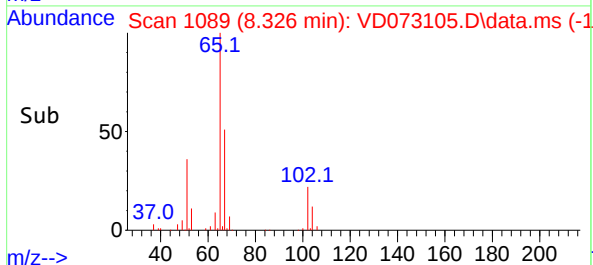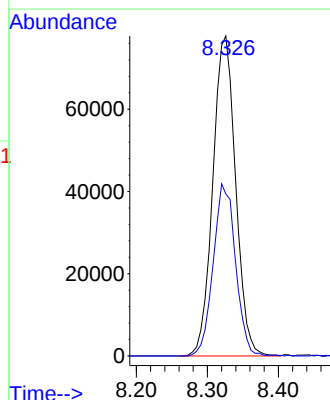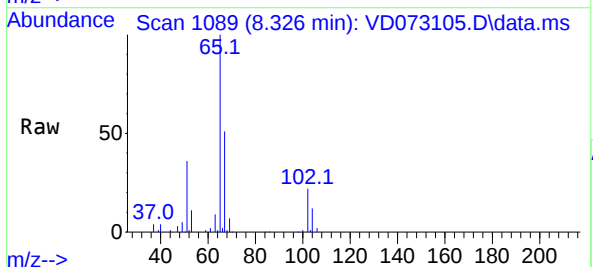

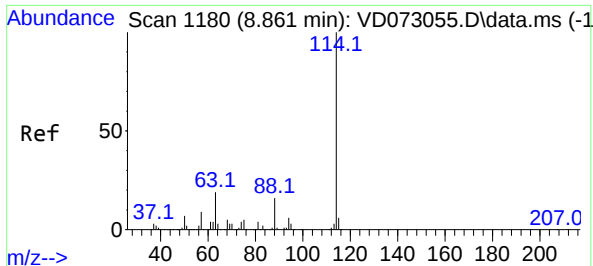

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.861 min Scan# 1180

Delta R.T. -0.000 min

Lab File: VD073105.D

Acq: 18 May 2022 18:10

Instrument :

MSVOA_D

ClientSampleId :

SB07





Tgt Ion:114 Resp: 546442

Ion Ratio Lower Upper

114 100

63 19.0 0.0 46.6

88 16.3 0.0 33.2

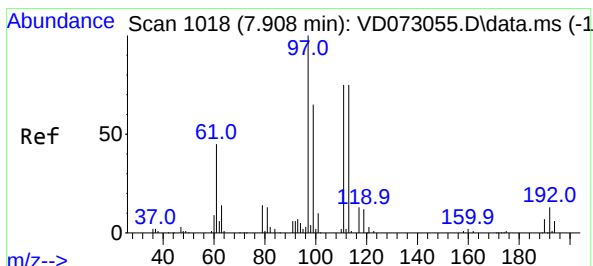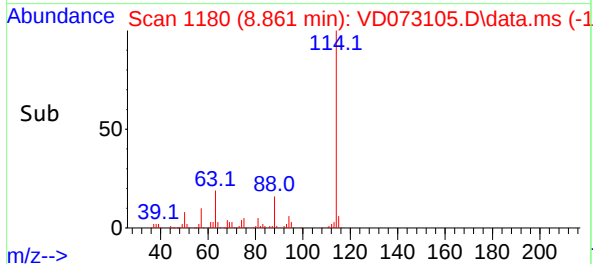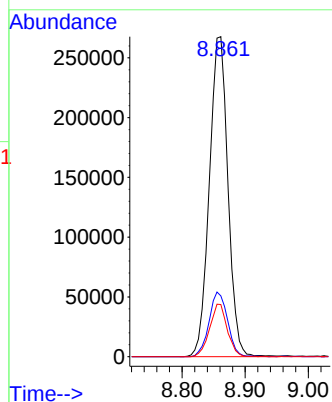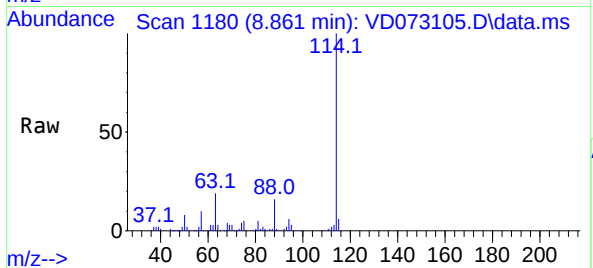

#35

Dibromofluoromethane

Concen: 48.073 ug/l

RT: 7.908 min Scan# 1018

Delta R.T. -0.000 min

Lab File: VD073105.D

Acq: 18 May 2022 18:10




Tgt Ion:113 Resp: 184440


Ion Ratio Lower Upper

113 100

111 104.2 83.8 125.6

192 18.6 14.6 21.8


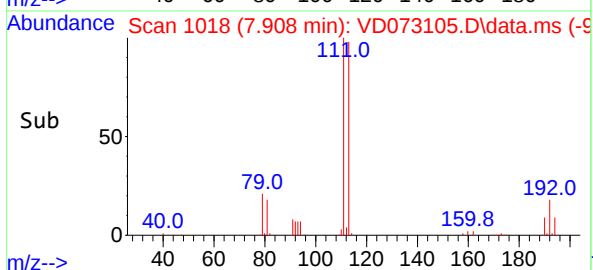
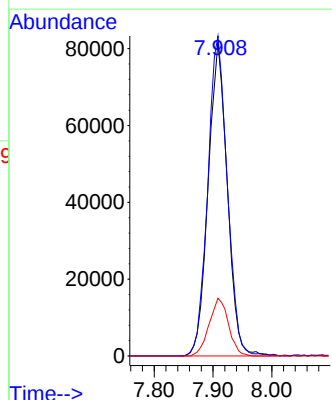
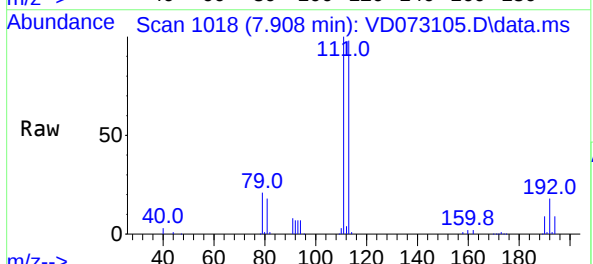


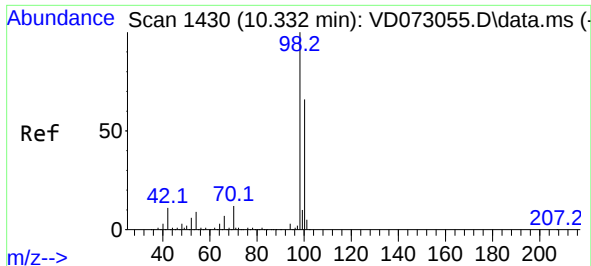

#50
Toluene-d8
Concen: 48.382 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD073105.D
Acq: 18 May 2022 18:10




Instrument :
MSVOA_D
ClientSampleId :
SB07


Tgt Ion: 98 Resp: 673411
Ion Ratio Lower Upper
98 100
100 66.4 52.4 78.6

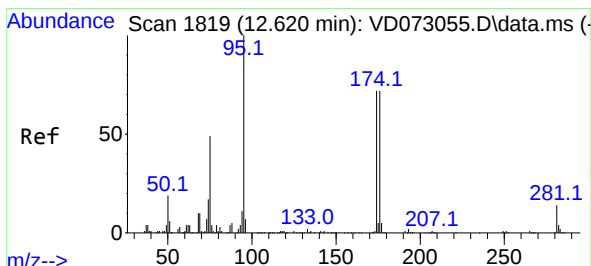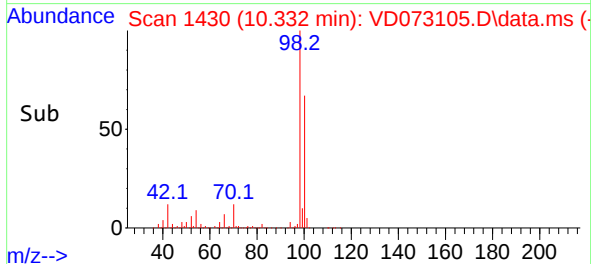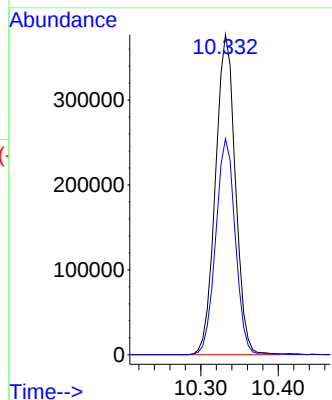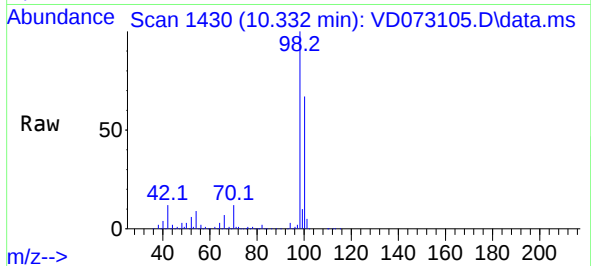

#62
4-Bromofluorobenzene
Concen: 47.001 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VD073105.D
Acq: 18 May 2022 18:10

Tgt Ion: 95 Resp: 236942
Ion Ratio Lower Upper
95 100
174 77.3 0.0 152.8
176 75.8 0.0 145.4


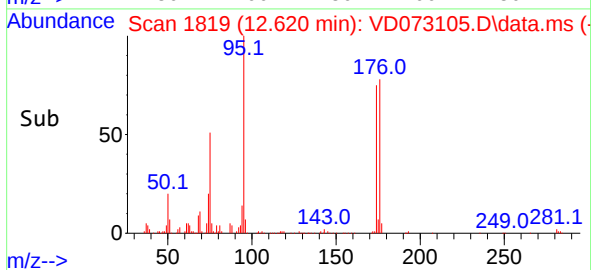
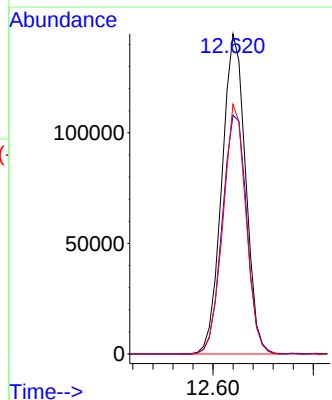
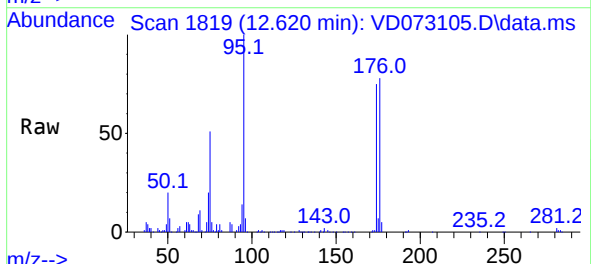


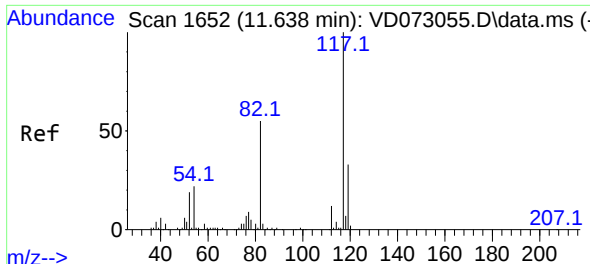

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.632 min Scan# 117
Delta R.T. -0.006 min
Lab File: VD073105.D
Acq: 18 May 2022 18:10

Instrument :
MSVOA_D
ClientSampleId :
SB07

Tgt Ion:117 Resp: 562270
Ion Ratio Lower Upper
117 100
82 54.6 45.3 67.9
119 31.0 26.6 40.0

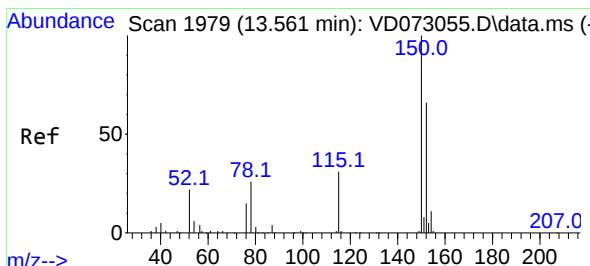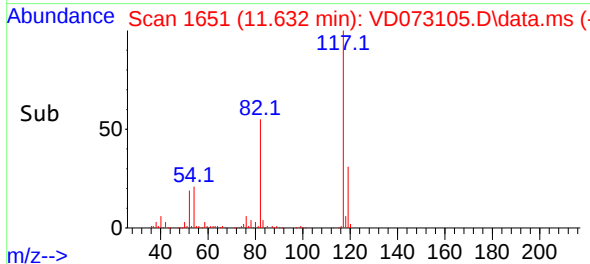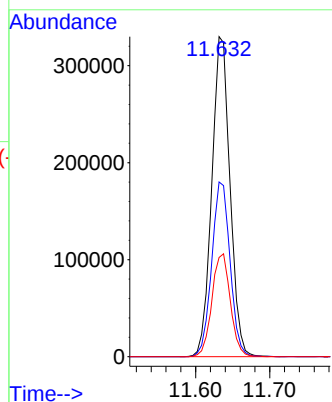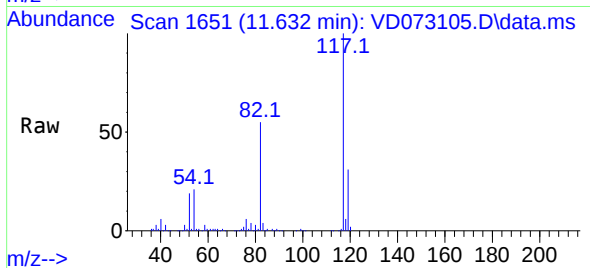

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. -0.000 min
Lab File: VD073105.D
Acq: 18 May 2022 18:10

Tgt Ion:152 Resp: 258777
Ion Ratio Lower Upper
152 100
115 59.9 31.3 93.8
150 154.7 0.0 348.6

