
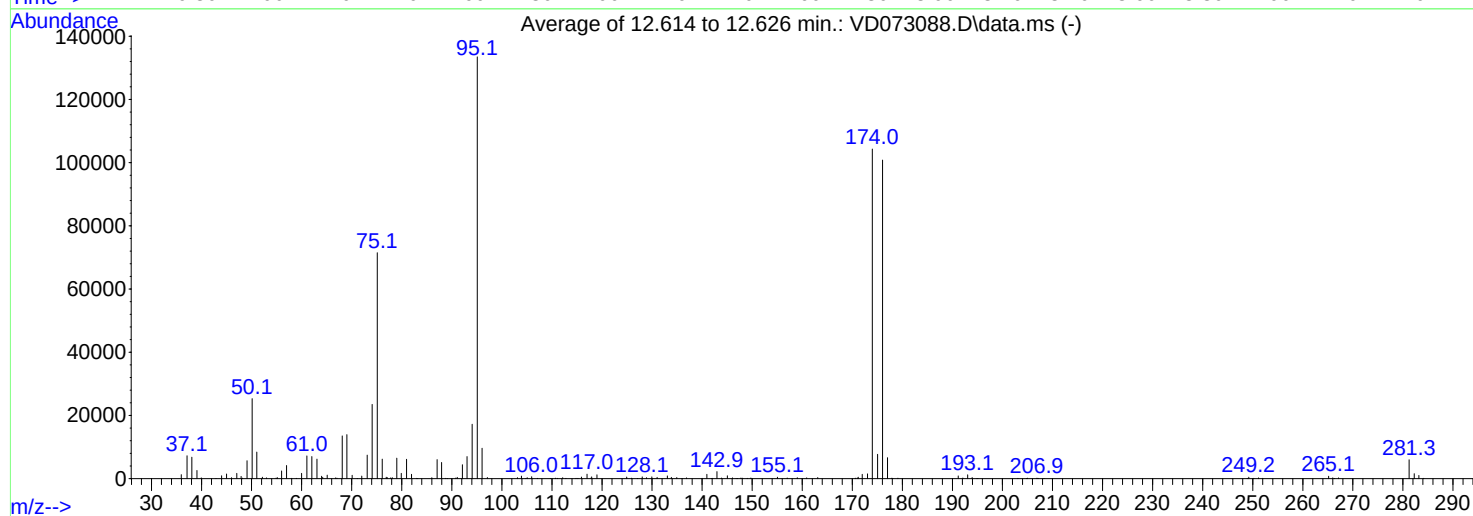


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051822\
 Data File : VD073088.D
 Acq On : 18 May 2022 09:28
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00 G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051722S.M
 Title : SW846 8260
 Last Update : Wed May 18 04:58:34 2022

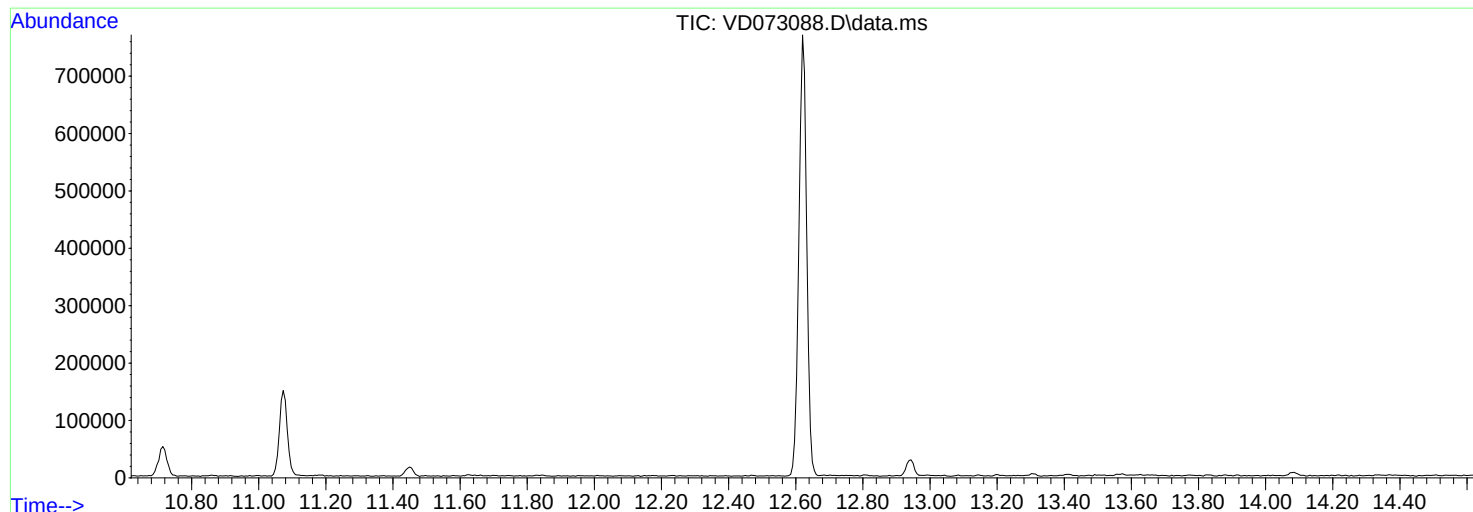

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	25325	PASS
75	95	30	60	53.6	71491	PASS
95	95	100	100	100.0	133488	PASS
96	95	5	9	7.2	9611	PASS
173	174	0.00	2	1.5	1535	PASS
174	95	50	100	78.2	104331	PASS
175	174	5	9	7.4	7713	PASS
176	174	95	101	96.6	100832	PASS
177	176	5	9	6.6	6662	PASS