
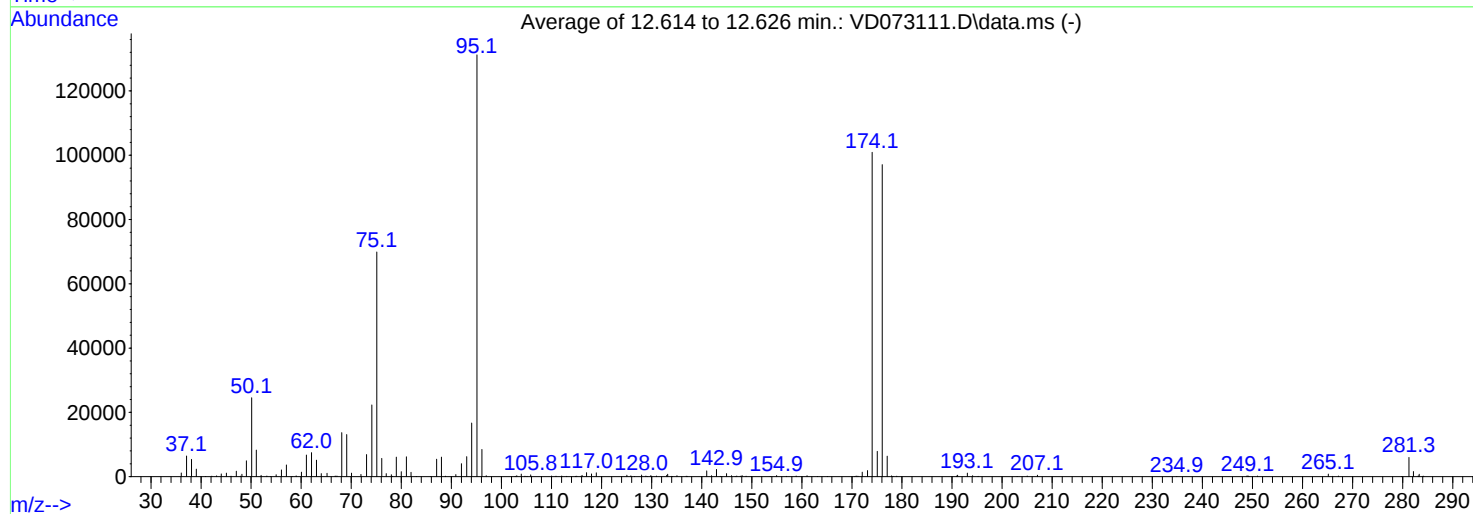


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051822\
 Data File : VD073111.D
 Acq On : 18 May 2022 21:31
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051722S.M
 Title : SW846 8260
 Last Update : Wed May 18 04:58:34 2022

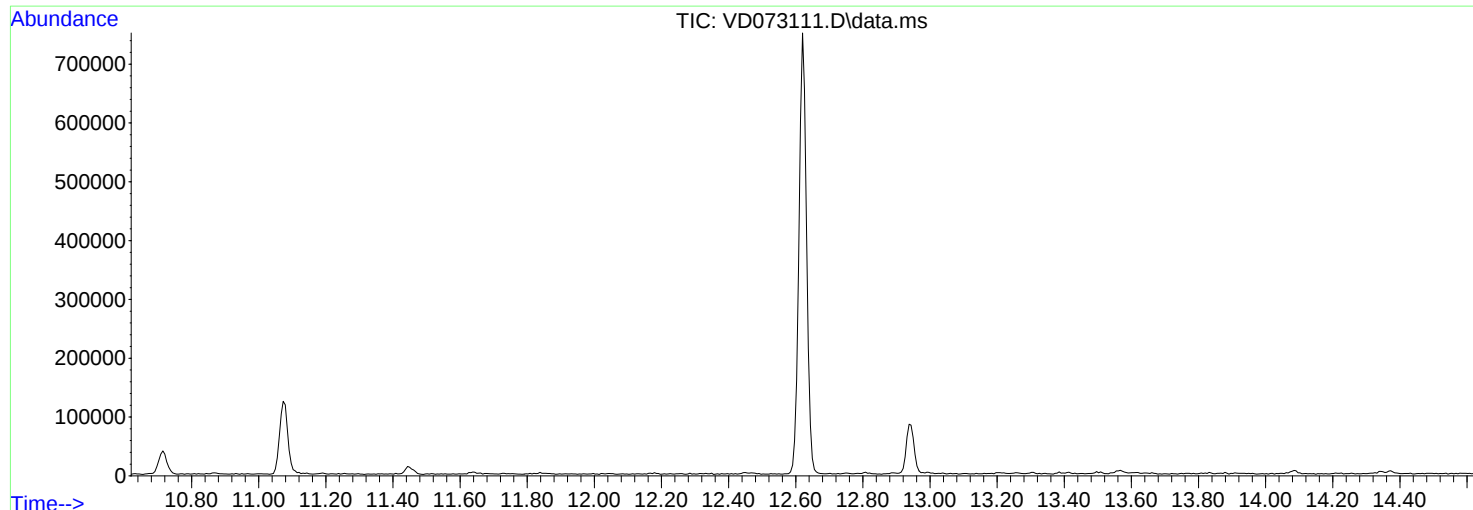

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	24549	PASS
75	95	30	60	53.3	69883	PASS
95	95	100	100	100.0	131235	PASS
96	95	5	9	6.5	8486	PASS
173	174	0.00	2	1.9	1886	PASS
174	95	50	100	76.9	100899	PASS
175	174	5	9	7.8	7875	PASS
176	174	95	101	96.2	97061	PASS
177	176	5	9	6.6	6384	PASS