


Dichlorodifluoromethane

Response Ratio

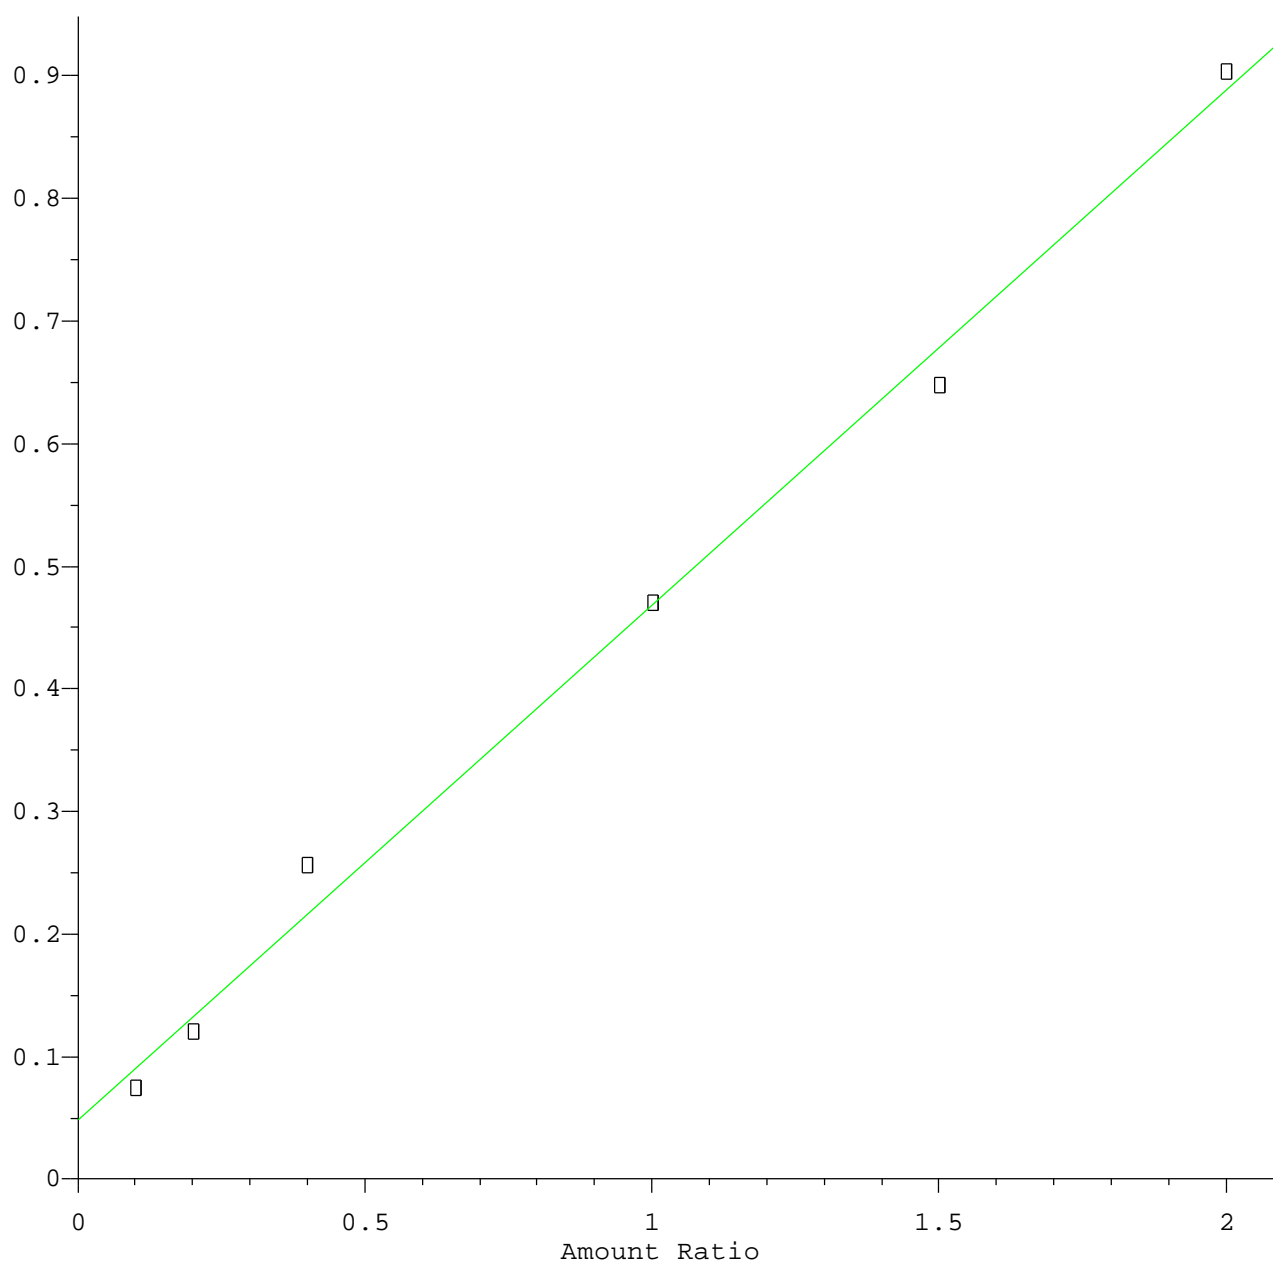


Resp Ratio = $4.20 \times 10^{-1} \times \text{Amt} + 4.80 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D052019S.M
Calibration Table Last Updated: Tue May 21 03:32:39 2019

Methylene Chloride

Response Ratio

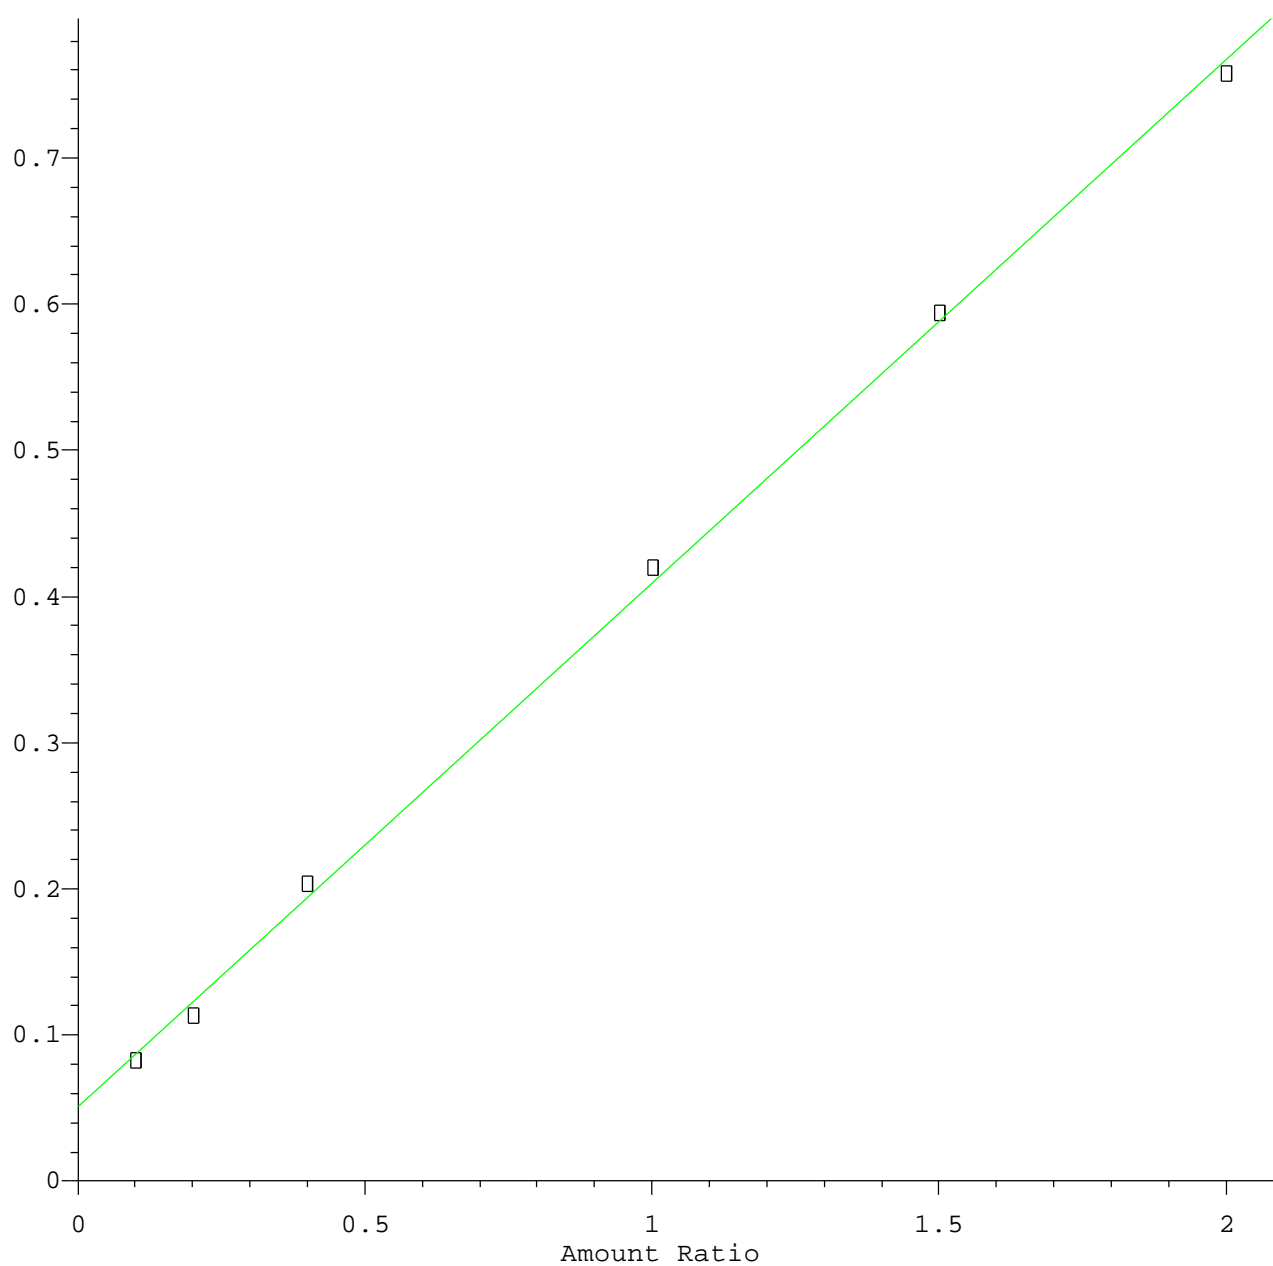

Resp Ratio = $3.58 \times 10^{-1} \times \text{Amt} + 5.12 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D052019S.M
Calibration Table Last Updated: Tue May 21 03:32:39 2019