


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD052119\
Data File : VD062473.D
Acq On : 21 May 2019 10:27
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D052019S.M
Title : SW846 8260
Last Update : Tue May 21 03:32:39 2019

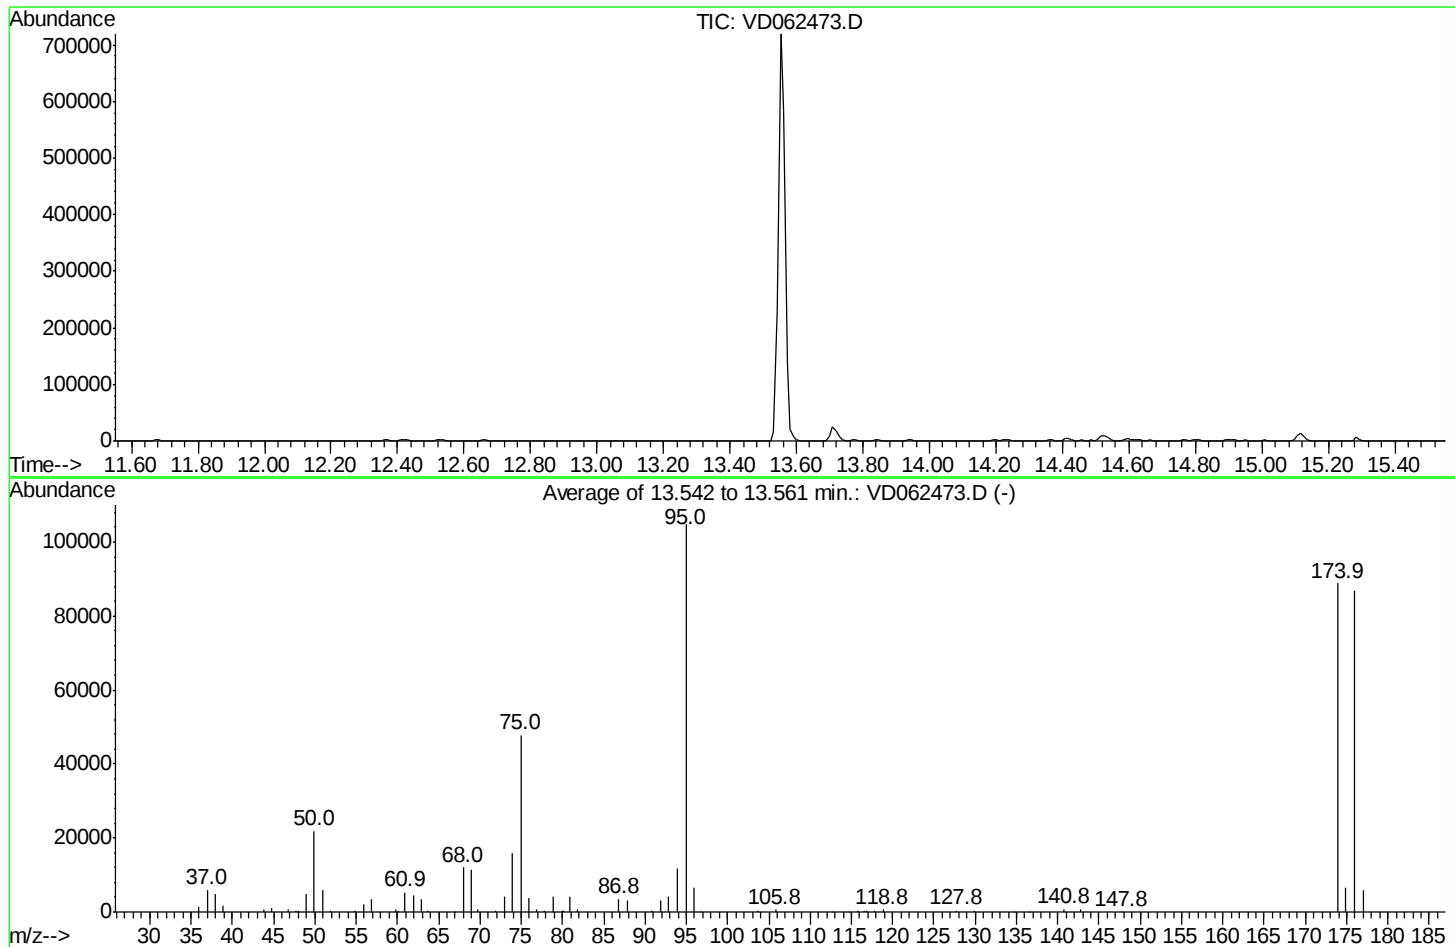

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	21930	PASS
75	95	30	60	45.6	47778	PASS
95	95	100	100	100.0	104765	PASS
96	95	5	9	6.3	6607	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.8	88872	PASS
175	174	5	9	7.3	6458	PASS
176	174	95	101	97.5	86674	PASS
177	176	5	9	6.7	5783	PASS