
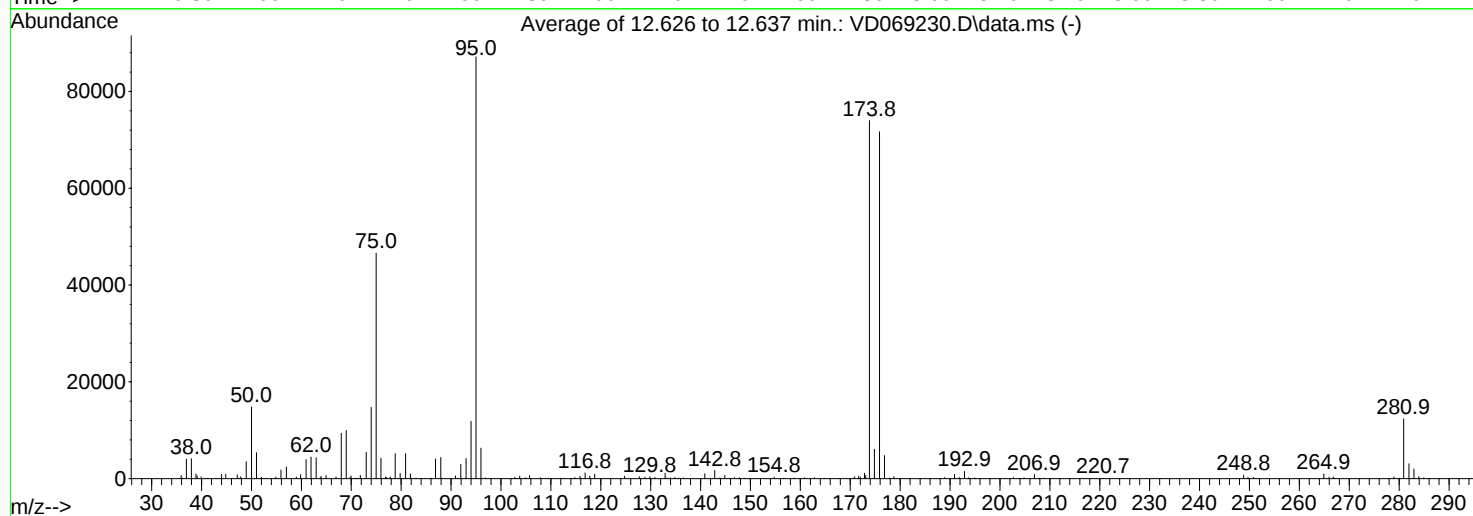


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD0512121\
Data File : VD069230.D
Acq On : 21 May 2021 10:53
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051221S.M
Title : SW846 8260
Last Update : Thu May 13 04:01:29 2021

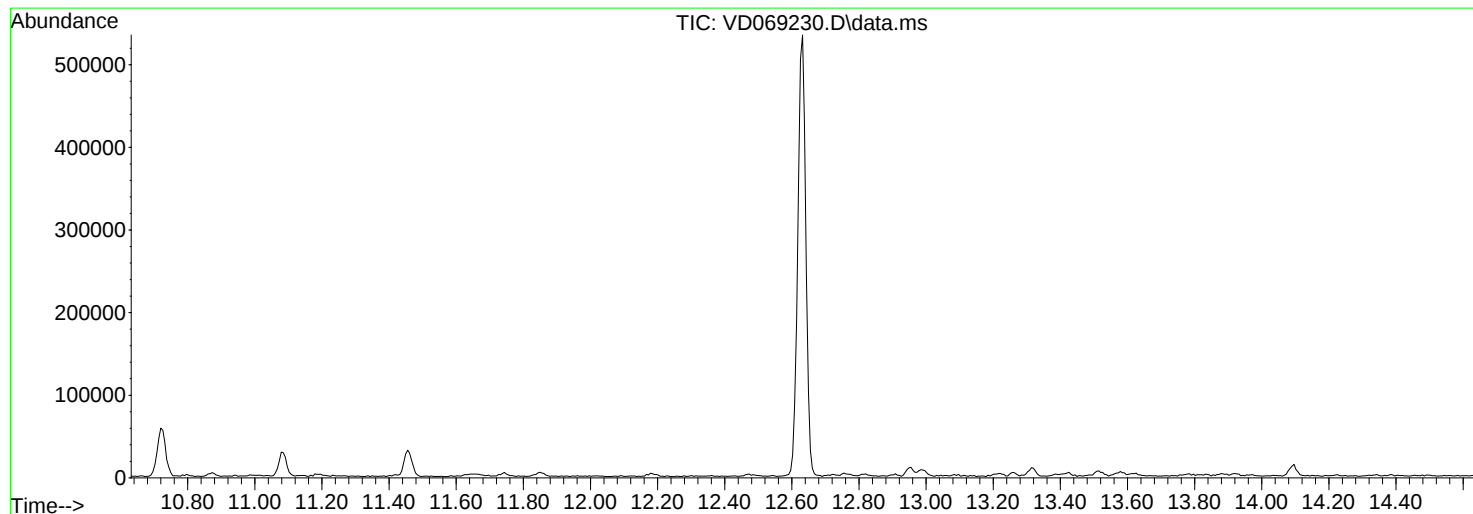

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.0	14855	PASS
75	95	30	60	53.5	46595	PASS
95	95	100	100	100.0	87144	PASS
96	95	5	9	7.3	6328	PASS
173	174	0.00	2	1.5	1141	PASS
174	95	50	100	84.9	73989	PASS
175	174	5	9	8.2	6089	PASS
176	174	95	101	96.9	71683	PASS
177	176	5	9	6.6	4762	PASS