
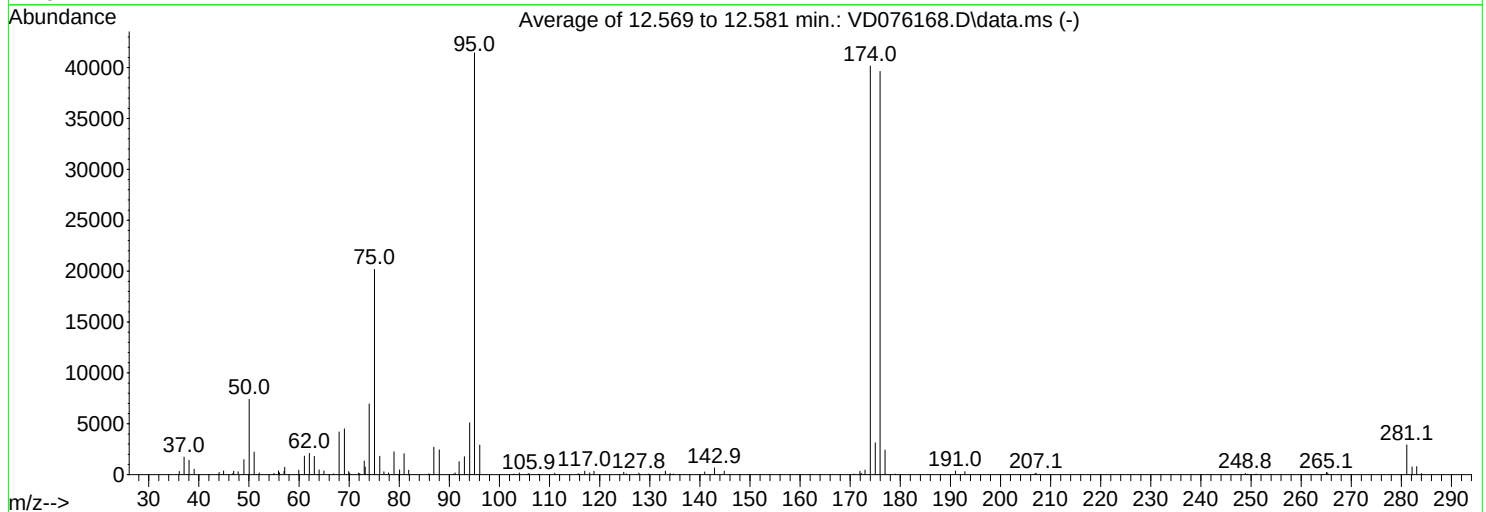


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052223\
Data File : VD076168.D
Acq On : 22 May 2023 09:10
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051523S.M
Title : SW846 8260
Last Update : Tue May 16 10:08:53 2023

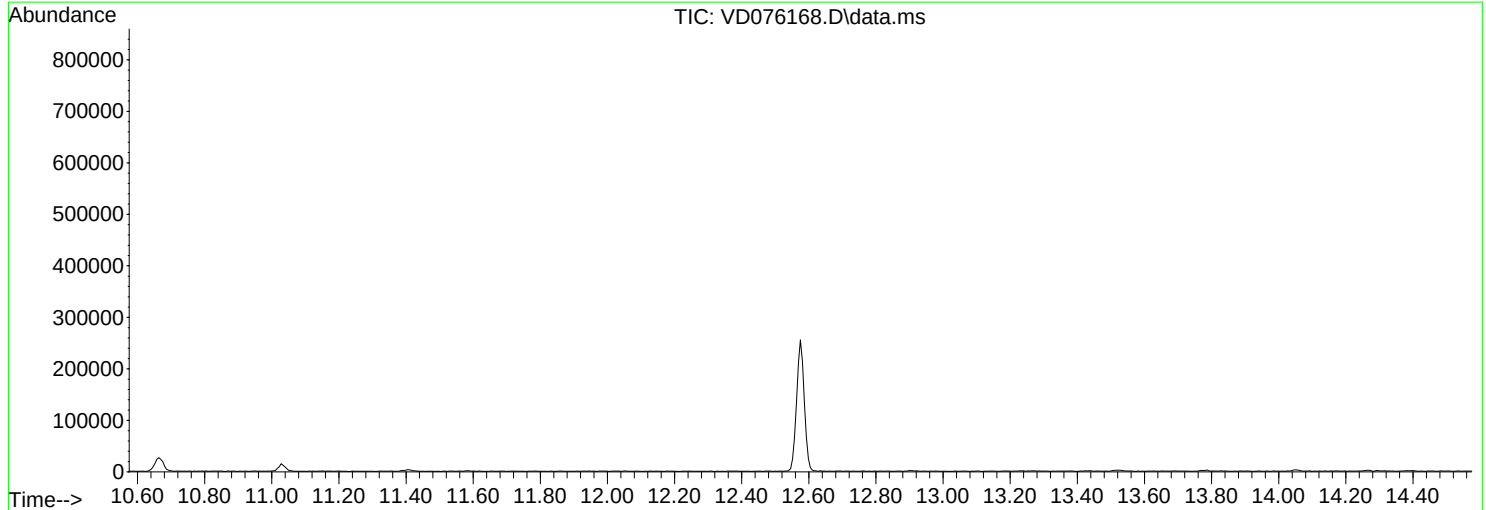

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	7414	PASS
75	95	30	60	48.7	20179	PASS
95	95	100	100	100.0	41453	PASS
96	95	5	9	7.0	2906	PASS
173	174	0.00	2	1.1	453	PASS
174	95	50	100	96.9	40165	PASS
175	174	5	9	7.8	3132	PASS
176	174	95	101	98.7	39627	PASS
177	176	5	9	6.1	2429	PASS