


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD052419\
 Data File : VD062525.D
 Acq On : 24 May 2019 9:33
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00g/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D052019S.M
 Title : SW846 8260
 Last Update : Tue May 21 03:32:39 2019

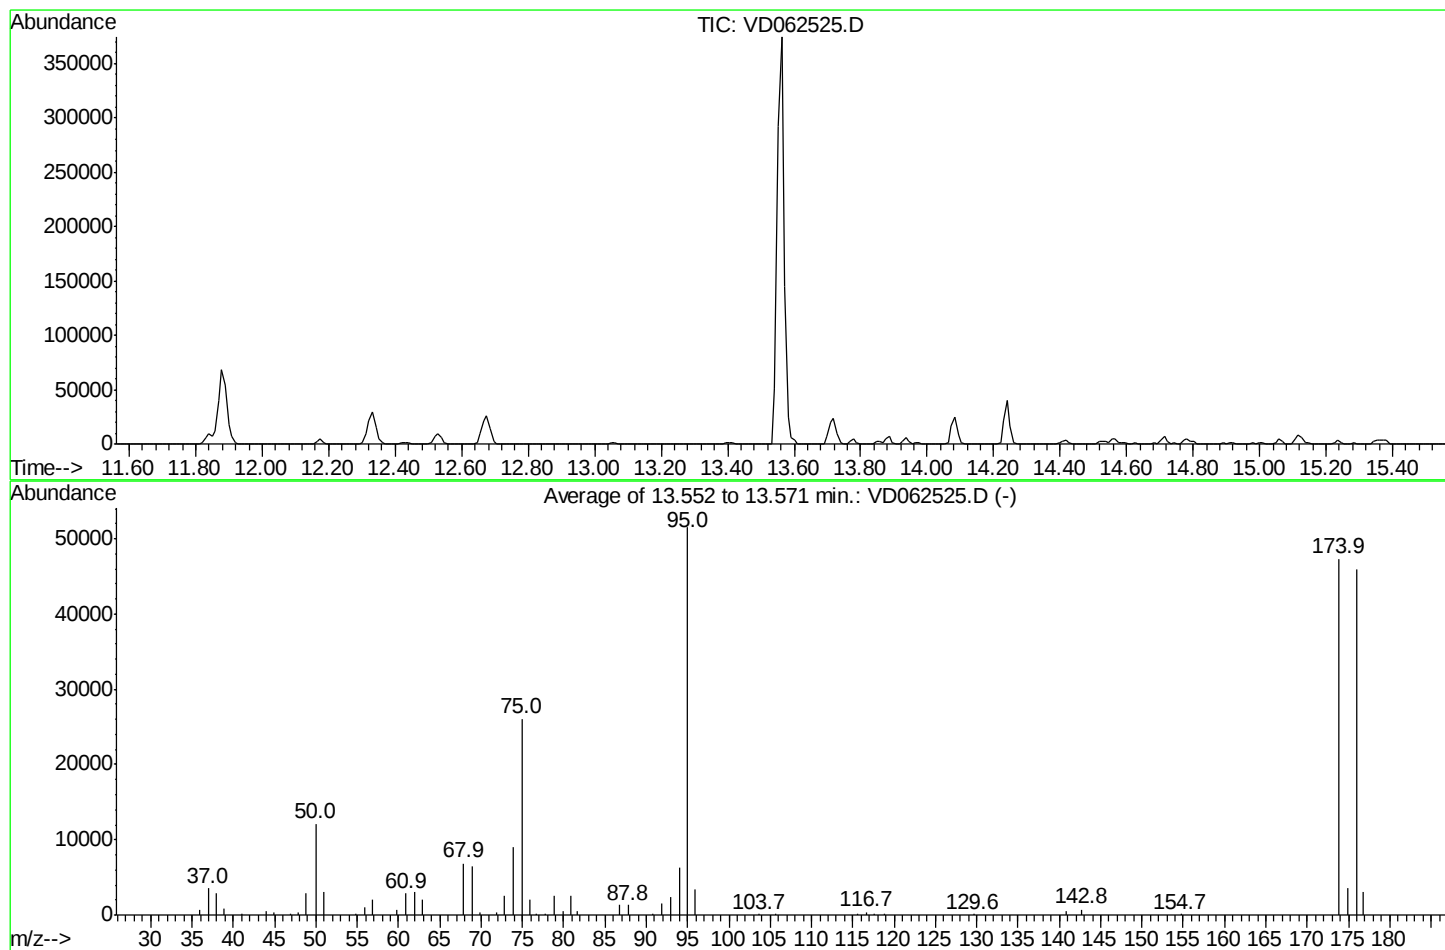

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	12124	PASS
75	95	30	60	50.6	26069	PASS
95	95	100	100	100.0	51530	PASS
96	95	5	9	6.7	3462	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	91.9	47370	PASS
175	174	5	9	7.6	3623	PASS
176	174	95	101	96.9	45888	PASS
177	176	5	9	6.9	3149	PASS