

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052424\
Data File : VD079016.D
Acq On : 24 May 2024 14:04
Operator : RP/MD
Sample : P2570-15
Misc : 5.85G/10ml/MSVOA_D/SOIL/VIAL A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BH5R1




Manual IntegrationsAPPROVED

Quant Time: May 24 23:25:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 24 02:12:30 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

05/30/2024
Supervised By :Semsettin
Yesilyurt

05/30/2024

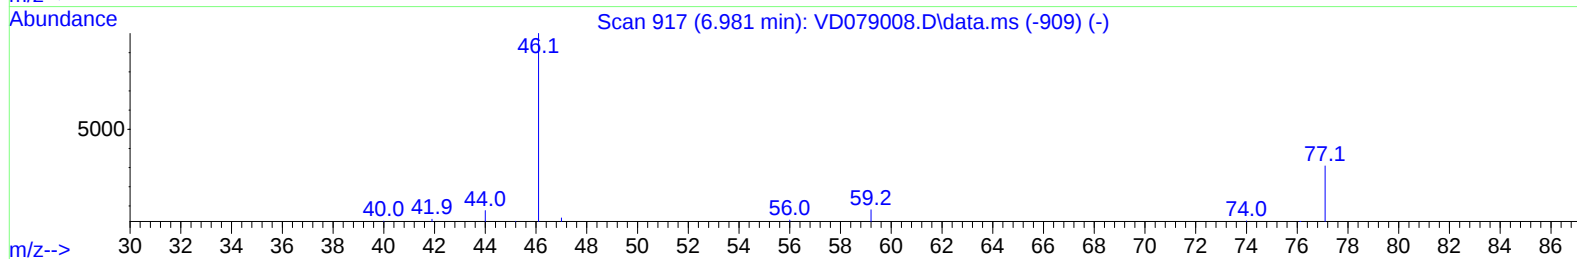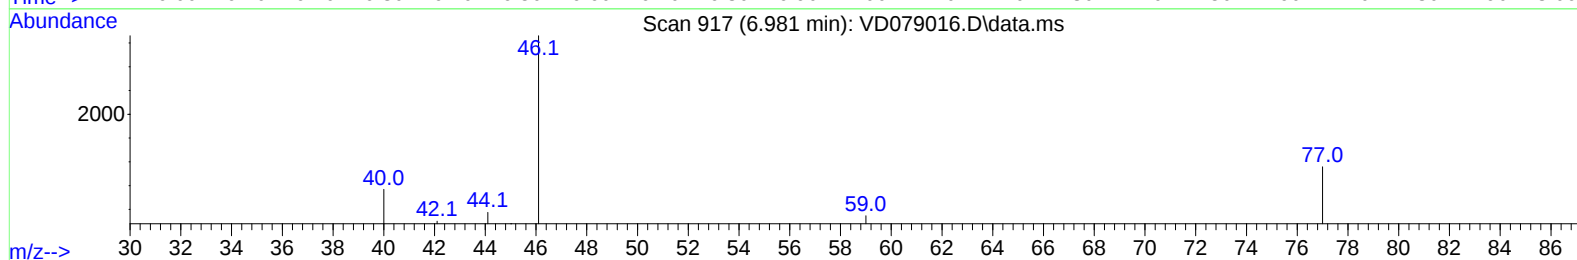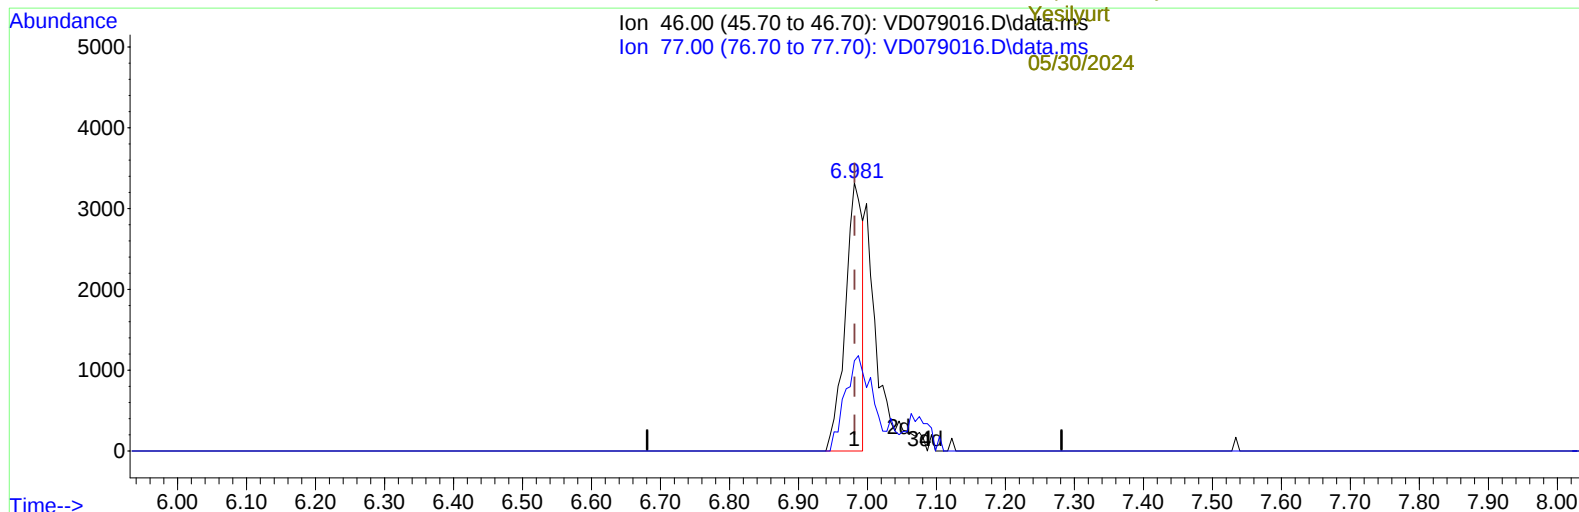

TIC: VD079016.D\data.ms

(21) 2-Butanone-d5 (S)

6.981min (-0.000) 9.99 ug/L

response 5754

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	29.20	41.35#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052424\
Data File : VD079016.D
Acq On : 24 May 2024 14:04
Operator : RP/MD
Sample : P2570-15
Misc : 5.85G/10ml/MSVOA_D/SOIL/VIAL A
ALS Vial : 11 Sample Multiplier: 1




Instrument :
MSVOA_D
ClientSampleId :
BH5R1

Manual IntegrationsAPPROVED

Reviewed By :Mahesh
Dadoda

05/30/2024
Supervised By :Semsettin
Yesilyurt

Quant Time: May 24 23:25:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 24 02:12:30 2024
Response via : Initial Calibration

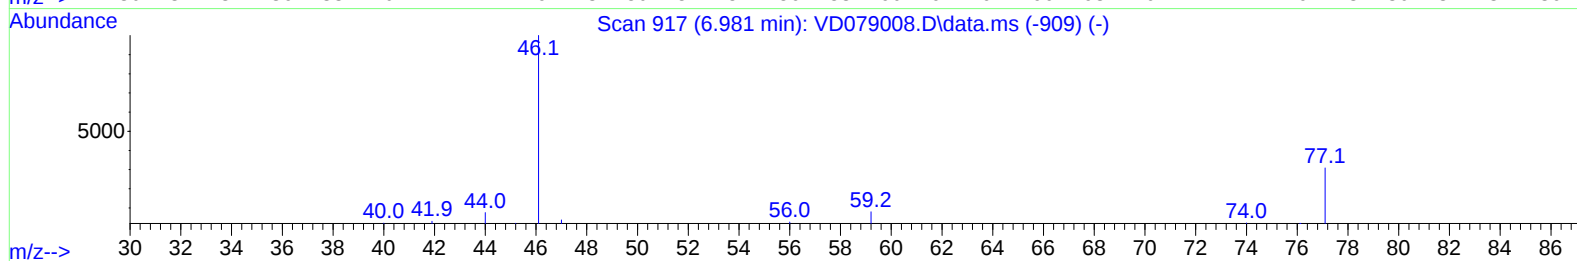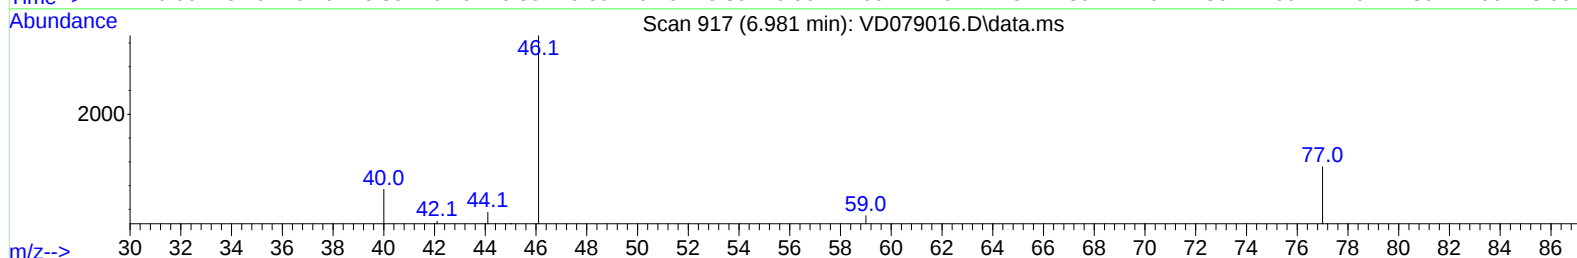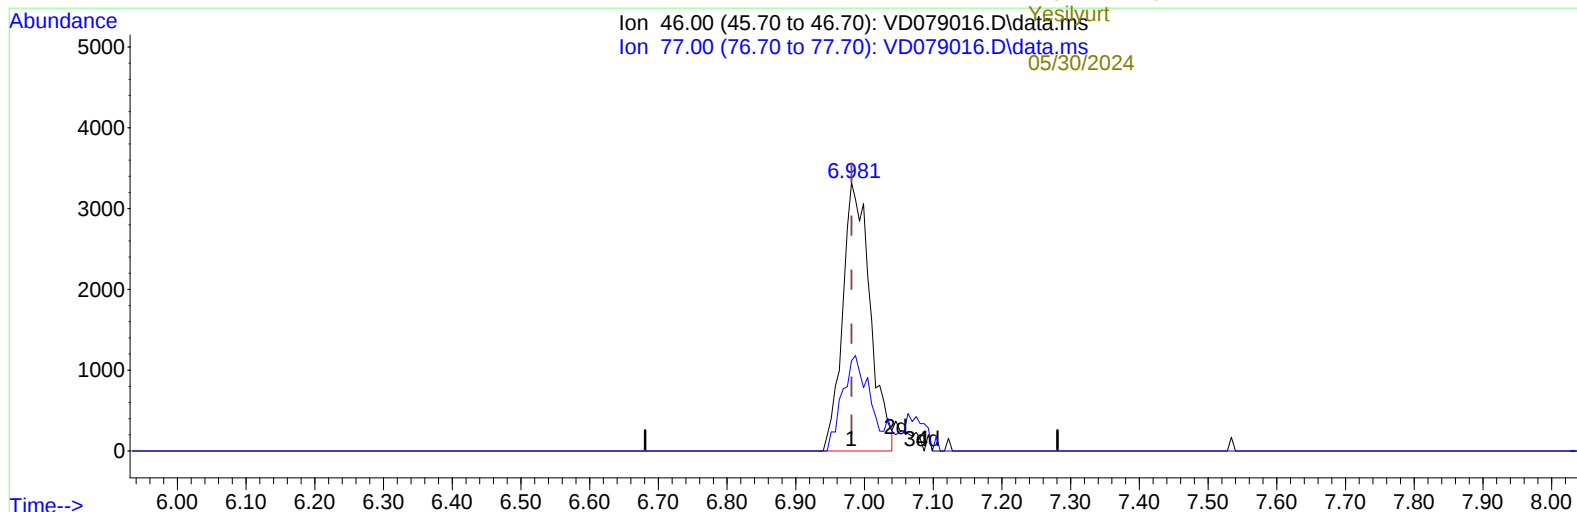

TIC: VD079016.D\data.ms

(21) 2-Butanone-d5 (S)

6.981min (-0.000) 15.92 ug/L m

response 9168

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	29.20	25.95
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052424\
 Data File : VD079016.D
 Acq On : 24 May 2024 14:04
 Operator : RP/MD
 Sample : P2570-15
 Misc : 5.85G/10ml/MSVOA_D/SOIL/VIAL A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BH5R1

Manual IntegrationsAPPROVED

Quant Time: May 24 23:25:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 24 02:12:30 2024
 Response via : Initial Calibration

Reviewed By :Mahesh
 Dadoda

05/30/2024
 Supervised By :Semsettin
 Yesilyurt

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.775	114		165955	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117		138974	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152		42037	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.269	65		74088	18.211	ug/L	0.00
Spiked Amount	25.000			Recovery	=	72.840%	
7) Chloroethane-d5	2.793	69		83827	19.249	ug/L	0.00
Spiked Amount	25.000			Recovery	=	77.000%	
11) 1,1-Dichloroethene-d2	3.911	65		11967	15.080	ug/L	0.00
Spiked Amount	25.000			Recovery	=	60.320%	
21) 2-Butanone-d5	6.981	46		9168m	15.921	ug/L	0.00
Spiked Amount	50.000			Recovery	=	31.840%	
24) Chloroform-d	7.563	84		73203	14.817	ug/L	0.00
Spiked Amount	25.000			Recovery	=	59.280%	
26) 1,2-Dichloroethane-d4	8.228	65		35833	15.273	ug/L	0.00
Spiked Amount	25.000			Recovery	=	61.080%#	
32) Benzene-d6	8.199	84		132024	18.618	ug/L	0.00
Spiked Amount	25.000			Recovery	=	74.480%	
36) 1,2-Dichloropropane-d6	9.210	67		43050	19.925	ug/L	0.00
Spiked Amount	25.000			Recovery	=	79.680%	
41) Toluene-d8	10.269	98		98178	15.020	ug/L	0.00
Spiked Amount	25.000			Recovery	=	60.080%	
43) trans-1,3-Dichloroprop...	10.528	79		12073	12.130	ug/L	0.00
Spiked Amount	25.000			Recovery	=	48.520%	
47) 2-Hexanone-d5	10.881	63		7114	16.428	ug/L	0.00
Spiked Amount	50.000			Recovery	=	32.860%	
56) 1,1,2,2-Tetrachloroeth...	12.651	84		35458	14.426	ug/L	0.00
Spiked Amount	25.000			Recovery	=	57.720%	
66) 1,2-Dichlorobenzene-d4	13.810	152		16027	11.233	ug/L	0.00
Spiked Amount	25.000			Recovery	=	44.920%#	
Target Compounds							
16) Methylene chloride	4.799	84		22408	5.700	ug/L	Qvalue 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052424\
Data File : VD079016.D
Acq On : 24 May 2024 14:04
Operator : RP/MD
Sample : P2570-15
Misc : 5.85G/10ml/MSVOA_D/SOIL/VIAL A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BH5R1

Manual IntegrationsAPPROVED

Reviewed By :Mahesh
Dadoda

05/30/2024
Supervised By :Semsettin
Yesilyurt

05/30/2024

